

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047974.D
 Acq On : 12 Apr 2022 22:29
 Operator : SY/MD
 Sample : N2345-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J84

Quant Time: Apr 13 04:51:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 13 04:40:51 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	347262	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	370175	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	190147	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	126431	50.206	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 100.420%		
7) Chloroethane-d5	1.916	69	108876	54.832	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 109.660%		
11) 1,1-Dichloroethene-d2	2.571	63	164568	35.719	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 71.440%		
21) 2-Butanone-d5	4.620	46	202395	93.639	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 93.640%		
24) Chloroform-d	5.067	84	226553	49.169	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 98.340%		
26) 1,2-Dichloroethane-d4	5.703	65	144787	51.234	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 102.460%		
32) Benzene-d6	5.729	84	465123	49.935	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 99.860%		
36) 1,2-Dichloropropane-d6	6.693	67	149831	52.377	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 104.760%		
41) Toluene-d8	7.899	98	414349	45.657	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 91.320%		
43) trans-1,3-Dichloroprop...	8.179	79	62143	42.880	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 85.760%		
47) 2-Hexanone-d5	8.632	63	144652	86.380	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 86.380%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	224581	45.746	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 91.500%		
66) 1,2-Dichlorobenzene-d4	12.195	152	176244	52.099	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 104.200%		
Target Compounds						
13) Acetone	2.626	43	4664	2.319	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047974.D
Acq On : 12 Apr 2022 22:29
Operator : SY/MD
Sample : N2345-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J84


Quant Time: Apr 13 04:51:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 13 04:40:51 2022
Response via : Initial Calibration

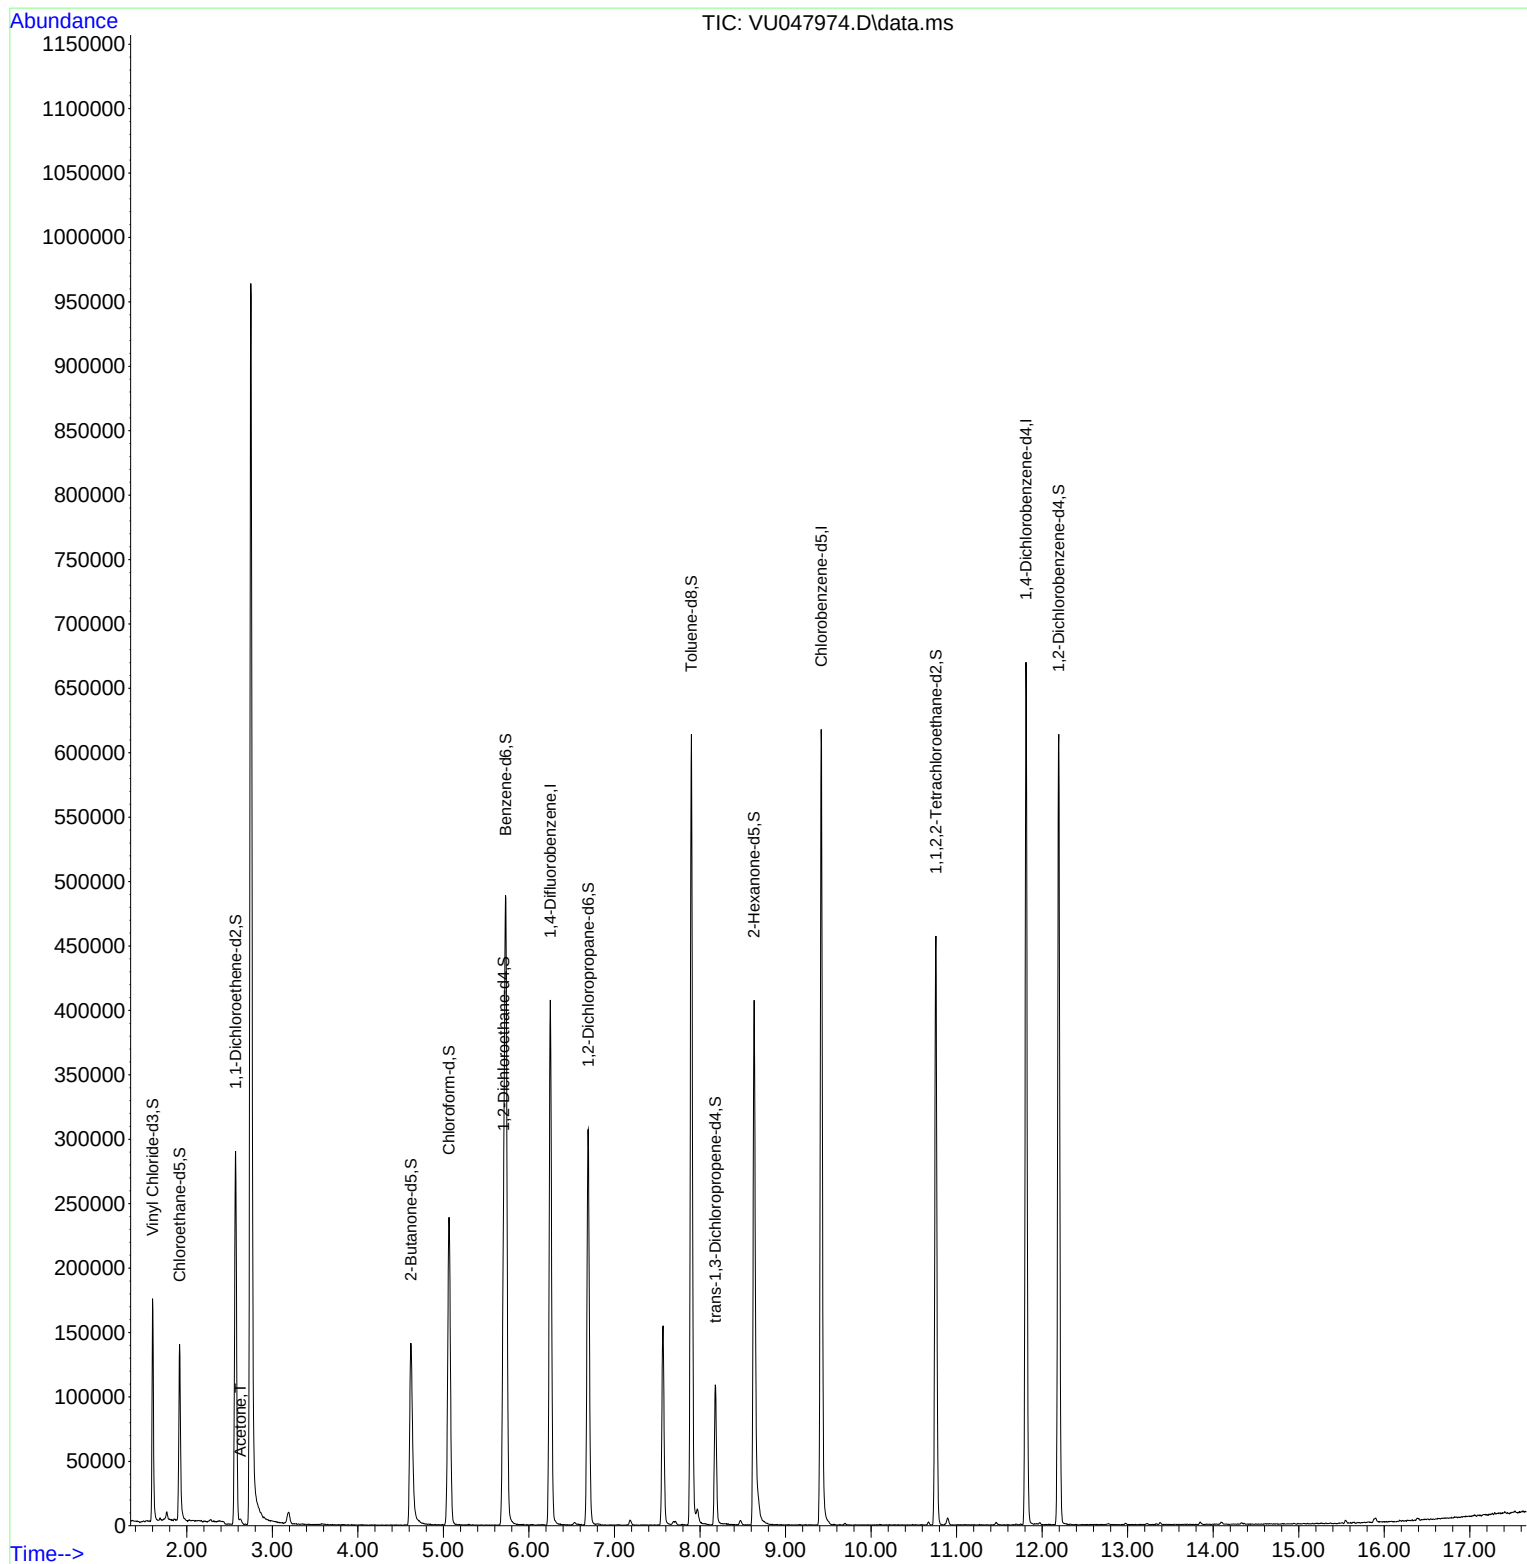

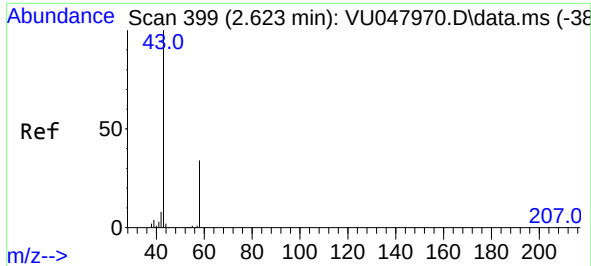

#13
 Acetone
 Concen: 2.319 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU047974.D
 Acq: 12 Apr 2022 22:29

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J84

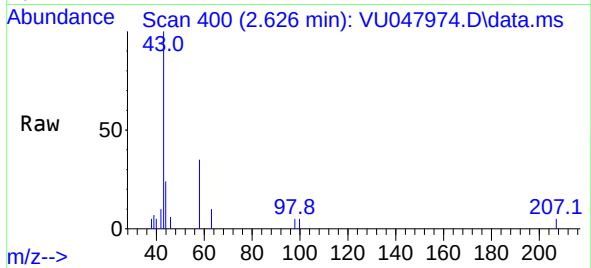

Tgt Ion: 43 Resp: 4664
 Ion Ratio Lower Upper
 43 100
 58 33.6 0.0 70.0

