

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047943.D
 Acq On : 12 Apr 2022 10:29
 Operator : SY/MD
 Sample : VU0412WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK085

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rBV	136878	160145	12.75%	1.541%
2	1.916	170	179	202	rVB	116477	164264	13.08%	1.580%
3	2.510	362	364	369	rVB2	368	264	0.02%	0.003%
4	2.572	370	383	398	rBV	243547	403364	32.12%	3.881%
5	2.694	418	421	424	rBV3	313	206	0.02%	0.002%
6	2.797	445	453	465	rVB2	1215	2182	0.17%	0.021%
7	2.896	479	484	494	rVB3	414	690	0.05%	0.007%
8	2.938	494	497	499	rBV	465	294	0.02%	0.003%
9	3.051	520	532	543	rVB5	2030	4012	0.32%	0.039%
10	3.099	543	547	551	rBV2	238	222	0.02%	0.002%
11	3.247	588	593	595	rBV2	217	215	0.02%	0.002%
12	3.359	622	628	634	rVV4	1023	1294	0.10%	0.012%
13	3.581	691	697	699	rBV2	262	275	0.02%	0.003%
14	3.771	749	756	758	rBV3	385	372	0.03%	0.004%
15	4.089	850	855	862	rVB2	218	247	0.02%	0.002%
16	4.192	881	887	890	rBV2	271	264	0.02%	0.003%
17	4.256	904	907	910	rBV2	245	227	0.02%	0.002%
18	4.372	940	943	949	rVB2	384	353	0.03%	0.003%
19	4.469	966	973	974	rBV2	236	252	0.02%	0.002%
20	4.623	1007	1021	1042	rBV	146389	346821	27.61%	3.337%
21	4.822	1081	1083	1087	rBV	413	355	0.03%	0.003%
22	5.067	1142	1159	1186	rBV	233521	509880	40.60%	4.905%
23	5.163	1187	1189	1195	rVB4	418	294	0.02%	0.003%
24	5.295	1220	1230	1234	rBV4	538	909	0.07%	0.009%
25	5.391	1252	1260	1261	rBV2	685	709	0.06%	0.007%
26	5.430	1270	1272	1277	rVB2	336	226	0.02%	0.002%
27	5.456	1277	1280	1283	rBV	280	232	0.02%	0.002%
28	5.520	1297	1300	1301	rBV2	324	214	0.02%	0.002%
29	5.636	1332	1336	1342	rVB3	237	245	0.02%	0.002%
30	5.726	1342	1364	1395	rBV2	455174	1255937	100.00%	12.083%
31	6.102	1476	1481	1483	rBV2	297	259	0.02%	0.002%
32	6.250	1513	1527	1557	rBV	404894	773546	61.59%	7.442%
33	6.542	1609	1618	1625	rVB6	1877	2990	0.24%	0.029%
34	6.591	1630	1633	1637	rVB2	375	267	0.02%	0.003%
35	6.629	1641	1645	1647	rBV	334	212	0.02%	0.002%
36	6.694	1651	1665	1691	rBV	294522	575477	45.82%	5.537%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047943.D
 Acq On : 12 Apr 2022 10:29
 Operator : SY/MD
 Sample : VU0412WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK085

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.983	1751	1755	1758	rBV	291	242	0.02%	0.002%
38	7.105	1789	1793	1796	rBV2	370	351	0.03%	0.003%
39	7.121	1796	1798	1802	rVB	395	249	0.02%	0.002%
40	7.186	1811	1818	1830	rVB5	2639	4054	0.32%	0.039%
41	7.276	1843	1846	1850	rVB	333	267	0.02%	0.003%
42	7.295	1850	1852	1855	rVB	409	229	0.02%	0.002%
43	7.314	1855	1858	1860	rBV2	380	259	0.02%	0.002%
44	7.436	1892	1896	1900	rBV2	386	359	0.03%	0.003%
45	7.507	1914	1918	1921	rBV	340	252	0.02%	0.002%
46	7.568	1922	1937	1956	rBV	152691	271261	21.60%	2.610%
47	7.690	1970	1975	1985	rVB5	1710	2667	0.21%	0.026%
48	7.793	2000	2007	2019	rVB4	2484	4053	0.32%	0.039%
49	7.899	2023	2040	2056	rBV	548073	956227	76.14%	9.200%
50	8.182	2115	2128	2150	rBV	108717	187945	14.96%	1.808%
51	8.404	2192	2197	2204	rVB4	741	840	0.07%	0.008%
52	8.472	2212	2218	2221	rBV4	508	593	0.05%	0.006%
53	8.558	2239	2245	2250	rBV5	964	1310	0.10%	0.013%
54	8.632	2255	2268	2302	rBV	430046	792570	63.11%	7.625%
55	8.806	2319	2322	2323	rBV	778	456	0.04%	0.004%
56	8.954	2365	2368	2372	rVB2	394	294	0.02%	0.003%
57	8.986	2372	2378	2381	rBV	388	401	0.03%	0.004%
58	9.086	2404	2409	2412	rBV2	289	288	0.02%	0.003%
59	9.333	2481	2486	2489	rBV3	356	308	0.02%	0.003%
60	9.417	2499	2512	2539	rBV	611168	1053067	83.85%	10.131%
61	9.574	2555	2561	2567	rVB4	1371	1756	0.14%	0.017%
62	9.700	2591	2600	2609	rBV4	2124	3433	0.27%	0.033%
63	10.108	2717	2727	2739	rVB6	2275	4421	0.35%	0.043%
64	10.237	2764	2767	2770	rBV	279	215	0.02%	0.002%
65	10.269	2774	2777	2780	rBV2	396	336	0.03%	0.003%
66	10.401	2812	2818	2822	rBV3	284	293	0.02%	0.003%
67	10.491	2838	2846	2853	rVV3	1256	1926	0.15%	0.019%
68	10.545	2861	2863	2867	rVB2	354	245	0.02%	0.002%
69	10.578	2867	2873	2877	rBV2	290	291	0.02%	0.003%
70	10.671	2895	2902	2910	rVB3	1035	1483	0.12%	0.014%
71	10.758	2915	2929	2946	rBV	459561	754952	60.11%	7.263%
72	10.822	2946	2949	2958	rVV5	1378	1655	0.13%	0.016%
73	10.870	2961	2964	2967	rVV3	312	255	0.02%	0.002%
74	11.092	3026	3033	3040	rVB	1008	1309	0.10%	0.013%
75	11.263	3083	3086	3089	rBV	467	307	0.02%	0.003%
76	11.333	3105	3108	3113	rVB2	332	339	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047943.D
 Acq On : 12 Apr 2022 10:29
 Operator : SY/MD
 Sample : VU0412WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK085

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.472	3144	3151	3161	rVB5	2310	3760	0.30%	0.036%
78	11.587	3182	3187	3190	rVB	401	341	0.03%	0.003%
79	11.610	3190	3194	3200	rBV3	344	516	0.04%	0.005%
80	11.748	3230	3237	3244	rBV3	2598	3403	0.27%	0.033%
81	11.812	3245	3257	3277	rVV	691283	1095403	87.22%	10.539%
82	11.925	3290	3292	3296	rVB3	516	283	0.02%	0.003%
83	12.037	3325	3327	3333	rVB2	444	399	0.03%	0.004%
84	12.079	3337	3340	3342	rBV	423	354	0.03%	0.003%
85	12.195	3361	3376	3391	rBV	600773	985345	78.45%	9.480%
86	12.288	3403	3405	3406	rBV2	448	211	0.02%	0.002%
87	12.767	3551	3554	3559	rBV5	406	393	0.03%	0.004%
88	12.822	3567	3571	3575	rBV2	370	453	0.04%	0.004%
89	12.957	3606	3613	3616	rBV3	399	533	0.04%	0.005%
90	12.996	3622	3625	3627	rBV3	777	552	0.04%	0.005%
91	13.057	3641	3644	3646	rBV2	392	248	0.02%	0.002%
92	13.227	3689	3697	3705	rVB6	3519	5121	0.41%	0.049%
93	13.266	3705	3709	3712	rBV2	313	297	0.02%	0.003%
94	13.430	3754	3760	3765	rBV3	418	595	0.05%	0.006%
95	13.533	3789	3792	3794	rBV2	384	290	0.02%	0.003%
96	13.848	3881	3890	3899	rVB5	4941	7817	0.62%	0.075%
97	14.092	3956	3966	3981	rBV2	11467	18825	1.50%	0.181%
98	14.333	4032	4041	4055	rBV3	5240	8836	0.70%	0.085%
99	14.577	4114	4117	4122	rBV3	368	286	0.02%	0.003%
100	14.835	4194	4197	4203	rBV2	431	424	0.03%	0.004%


Sum of corrected areas: 10394158

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047943.D
Acq On : 12 Apr 2022 10:29
Operator : SY/MD
Sample : VU0412WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK085

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

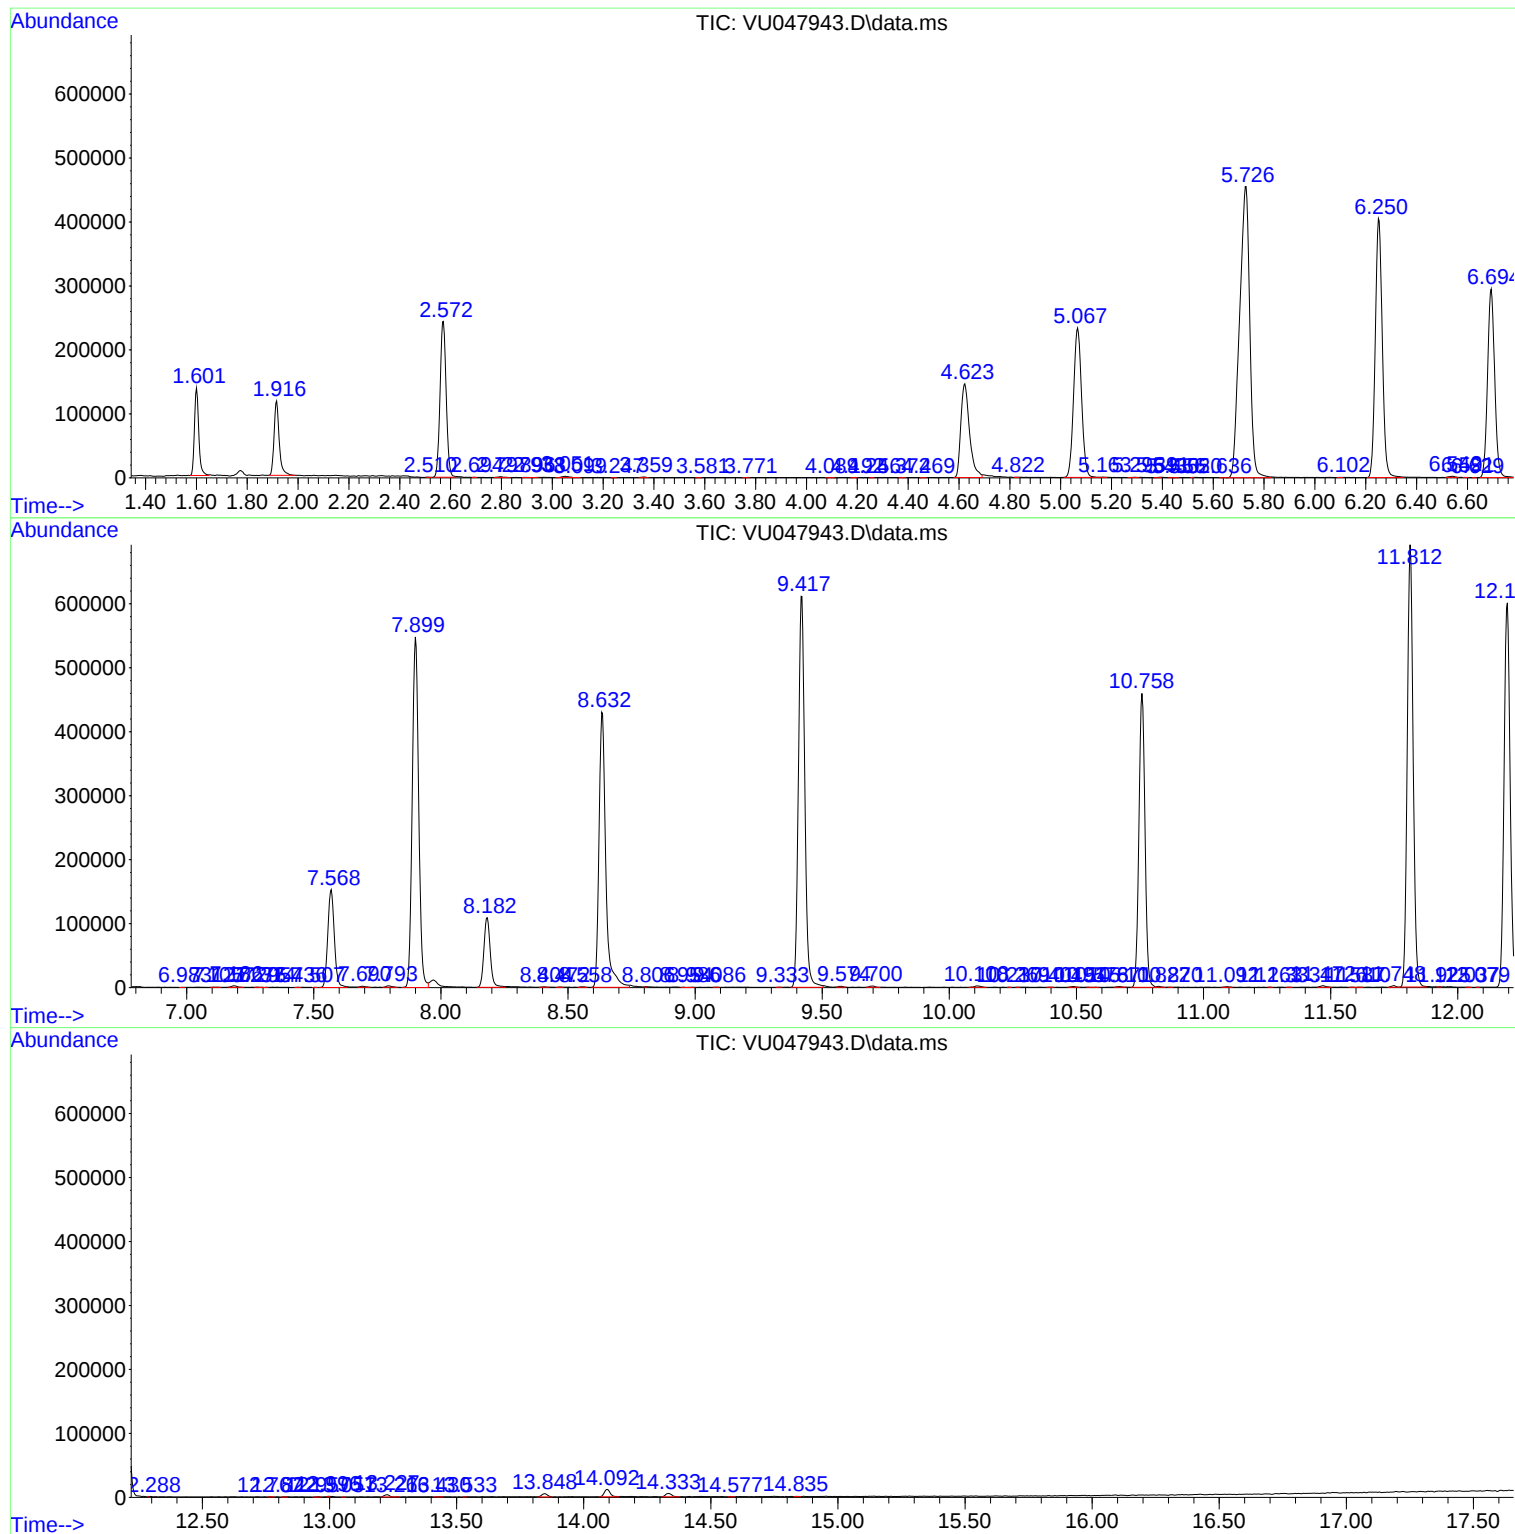

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047943.D
Acq On : 12 Apr 2022 10:29
Operator : SY/MD
Sample : VU0412WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK085

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047943.D
Acq On : 12 Apr 2022 10:29
Operator : SY/MD
Sample : VU0412WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK085

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc