

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047944.D
 Acq On : 12 Apr 2022 10:51
 Operator : SY/MD
 Sample : N2316-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rVB	129185	151584	12.53%	1.502%
2	1.916	170	179	200	rVB	113053	155116	12.82%	1.537%
3	2.571	370	383	401	rBV	228986	384055	31.74%	3.806%
4	2.729	429	432	437	rVV4	295	264	0.02%	0.003%
5	2.790	446	451	454	rBV2	818	878	0.07%	0.009%
6	2.832	462	464	469	rVB2	516	289	0.02%	0.003%
7	2.858	469	472	474	rBV	312	245	0.02%	0.002%
8	2.893	480	483	485	rBV2	314	229	0.02%	0.002%
9	2.951	498	501	503	rBV	354	306	0.03%	0.003%
10	3.006	515	518	521	rBV3	298	267	0.02%	0.003%
11	3.054	524	533	542	rBV4	2066	3889	0.32%	0.039%
12	3.173	568	570	576	rBV3	371	426	0.04%	0.004%
13	3.356	621	627	628	rBV3	652	588	0.05%	0.006%
14	3.430	648	650	656	rVV	377	332	0.03%	0.003%
15	3.478	662	665	669	rBV	281	208	0.02%	0.002%
16	3.514	673	676	680	rBV2	305	288	0.02%	0.003%
17	3.533	680	682	685	rBV2	432	329	0.03%	0.003%
18	3.584	695	698	702	rVB2	358	294	0.02%	0.003%
19	3.639	711	715	720	rBV2	378	365	0.03%	0.004%
20	3.706	732	736	739	rBV2	345	268	0.02%	0.003%
21	3.784	755	760	767	rVB3	268	351	0.03%	0.003%
22	3.825	767	773	776	rBV3	297	317	0.03%	0.003%
23	3.870	784	787	791	rVB	433	379	0.03%	0.004%
24	3.893	791	794	798	rBV2	363	284	0.02%	0.003%
25	3.951	809	812	815	rVB2	283	202	0.02%	0.002%
26	4.150	871	874	879	rVB2	380	258	0.02%	0.003%
27	4.179	879	883	887	rBV2	437	512	0.04%	0.005%
28	4.240	900	902	906	rVB2	355	209	0.02%	0.002%
29	4.266	907	910	912	rBV	403	260	0.02%	0.003%
30	4.462	968	971	974	rBV	326	269	0.02%	0.003%
31	4.501	980	983	988	rVB2	371	342	0.03%	0.003%
32	4.578	1003	1007	1009	rBV2	253	231	0.02%	0.002%
33	4.626	1009	1022	1059	rBV	140464	361380	29.86%	3.581%
34	4.854	1090	1093	1096	rBV2	364	299	0.02%	0.003%
35	5.067	1141	1159	1178	rBV	222974	493266	40.76%	4.888%
36	5.192	1196	1198	1202	rVB2	509	298	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047944.D
 Acq On : 12 Apr 2022 10:51
 Operator : SY/MD
 Sample : N2316-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.279	1222	1225	1229	rBV2	501	484	0.04%	0.005%
38	5.523	1294	1301	1303	rBV4	535	592	0.05%	0.006%
39	5.726	1342	1364	1394	rBV2	441579	1210079	100.00%	11.991%
40	5.896	1412	1417	1419	rBV2	310	273	0.02%	0.003%
41	5.957	1433	1436	1439	rBV2	255	230	0.02%	0.002%
42	6.083	1471	1475	1478	rBV2	241	225	0.02%	0.002%
43	6.192	1506	1509	1512	rBV	638	430	0.04%	0.004%
44	6.250	1513	1527	1552	rBV	388197	741287	61.26%	7.345%
45	6.529	1608	1614	1616	rBV5	1575	1636	0.14%	0.016%
46	6.693	1649	1665	1687	rBV	281527	556233	45.97%	5.512%
47	6.800	1693	1698	1709	rVB8	1454	2339	0.19%	0.023%
48	6.864	1714	1718	1721	rBV	274	229	0.02%	0.002%
49	7.018	1762	1766	1769	rBV2	285	288	0.02%	0.003%
50	7.092	1786	1789	1791	rBV2	597	454	0.04%	0.004%
51	7.144	1801	1805	1808	rBV2	376	207	0.02%	0.002%
52	7.189	1808	1819	1828	rVV3	2174	3998	0.33%	0.040%
53	7.279	1842	1847	1855	rVB2	399	542	0.04%	0.005%
54	7.356	1867	1871	1874	rBV2	277	270	0.02%	0.003%
55	7.481	1907	1910	1916	rVB3	403	414	0.03%	0.004%
56	7.513	1916	1920	1923	rBV2	295	234	0.02%	0.002%
57	7.568	1923	1937	1958	rBV	146915	264502	21.86%	2.621%
58	7.687	1968	1974	1985	rBV6	1782	3045	0.25%	0.030%
59	7.755	1991	1995	1998	rBV5	511	369	0.03%	0.004%
60	7.796	2000	2008	2016	rBV5	1643	2344	0.19%	0.023%
61	7.899	2023	2040	2056	rBV	525400	916480	75.74%	9.081%
62	8.179	2116	2127	2141	rBV2	103666	179311	14.82%	1.777%
63	8.404	2191	2197	2202	rVB4	714	913	0.08%	0.009%
64	8.433	2202	2206	2208	rBV2	263	237	0.02%	0.002%
65	8.504	2226	2228	2231	rBV2	327	222	0.02%	0.002%
66	8.555	2238	2244	2249	rVB3	895	974	0.08%	0.010%
67	8.636	2256	2269	2311	rBV	449650	831296	68.70%	8.237%
68	8.806	2320	2322	2327	rVB3	778	640	0.05%	0.006%
69	8.918	2355	2357	2365	rVB3	798	1007	0.08%	0.010%
70	9.002	2380	2383	2388	rVB3	262	238	0.02%	0.002%
71	9.028	2388	2391	2394	rBV2	527	263	0.02%	0.003%
72	9.050	2396	2398	2403	rVB3	262	206	0.02%	0.002%
73	9.163	2428	2433	2436	rBV2	282	274	0.02%	0.003%
74	9.217	2448	2450	2454	rVB2	352	247	0.02%	0.002%
75	9.308	2474	2478	2481	rBV2	205	202	0.02%	0.002%
76	9.417	2499	2512	2549	rBV	594810	1009675	83.44%	10.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047944.D
 Acq On : 12 Apr 2022 10:51
 Operator : SY/MD
 Sample : N2316-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.568	2553	2559	2565	rBV4	914	1304	0.11%	0.013%
78	9.697	2591	2599	2605	rBV2	2022	2984	0.25%	0.030%
79	10.105	2719	2726	2739	rVB5	1922	3327	0.27%	0.033%
80	10.272	2775	2778	2782	rVB2	342	239	0.02%	0.002%
81	10.298	2782	2786	2789	rVB	393	350	0.03%	0.003%
82	10.314	2789	2791	2795	rBV2	364	318	0.03%	0.003%
83	10.481	2838	2843	2851	rVB4	873	1271	0.11%	0.013%
84	10.671	2895	2902	2909	rBV3	1366	1767	0.15%	0.018%
85	10.758	2915	2929	2944	rBV	457948	749148	61.91%	7.423%
86	11.089	3027	3032	3043	rBV3	788	1320	0.11%	0.013%
87	11.700	3219	3222	3224	rVB2	448	214	0.02%	0.002%
88	11.751	3230	3238	3244	rBV6	1829	2529	0.21%	0.025%
89	11.812	3244	3257	3275	rBV	663239	1055367	87.21%	10.458%
90	12.192	3362	3375	3396	rVV	586507	958670	79.22%	9.499%
91	12.317	3411	3414	3419	rBV2	382	328	0.03%	0.003%
92	12.468	3458	3461	3464	rBV	245	231	0.02%	0.002%
93	12.999	3623	3626	3629	rBV2	601	486	0.04%	0.005%
94	13.221	3689	3695	3704	rBV6	1814	2663	0.22%	0.026%
95	13.346	3731	3734	3738	rBV	568	405	0.03%	0.004%
96	13.844	3883	3889	3898	rVB2	3383	4539	0.38%	0.045%
97	13.963	3923	3926	3929	rBV2	313	301	0.02%	0.003%
98	14.092	3959	3966	3977	rVB2	4826	7560	0.62%	0.075%
99	14.333	4034	4041	4049	rBV4	3257	4403	0.36%	0.044%
100	14.571	4113	4115	4118	rBV3	373	219	0.02%	0.002%




Sum of corrected areas: 10091909

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047944.D
Acq On : 12 Apr 2022 10:51
Operator : SY/MD
Sample : N2316-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

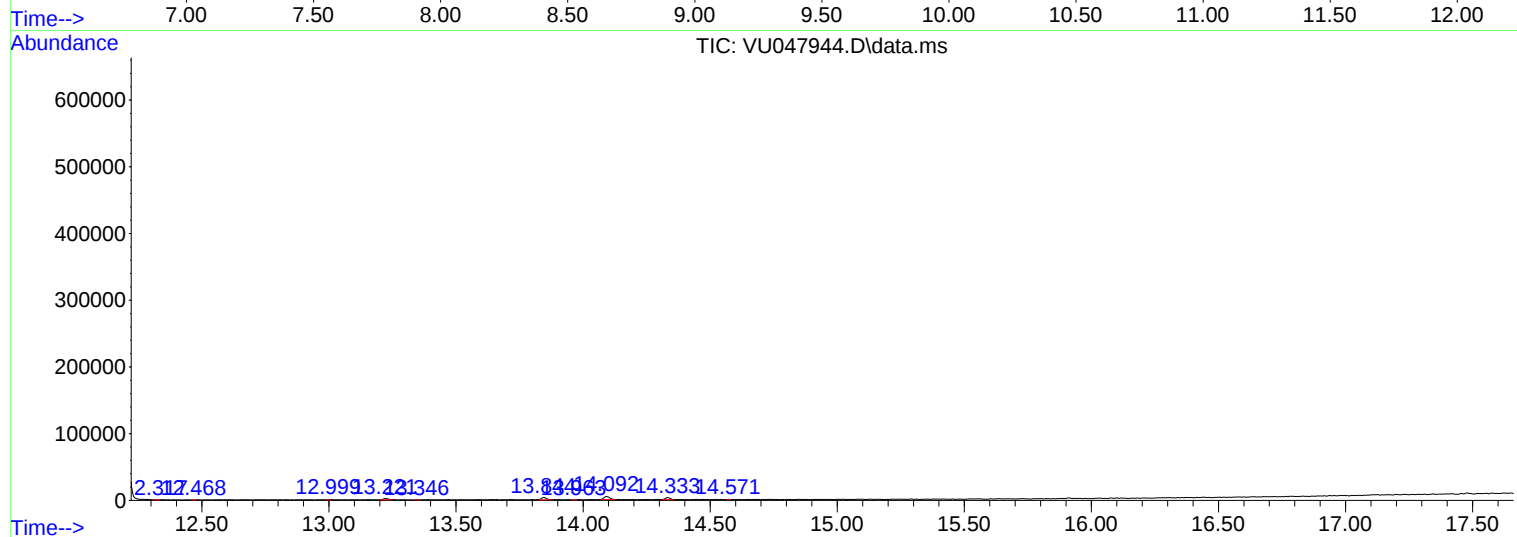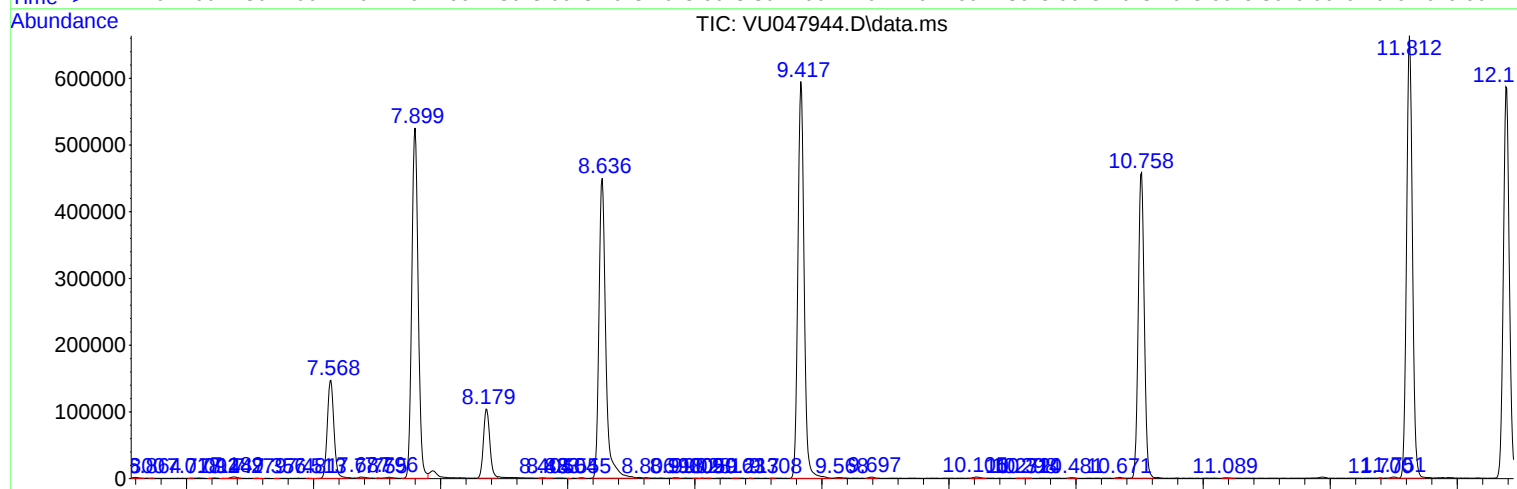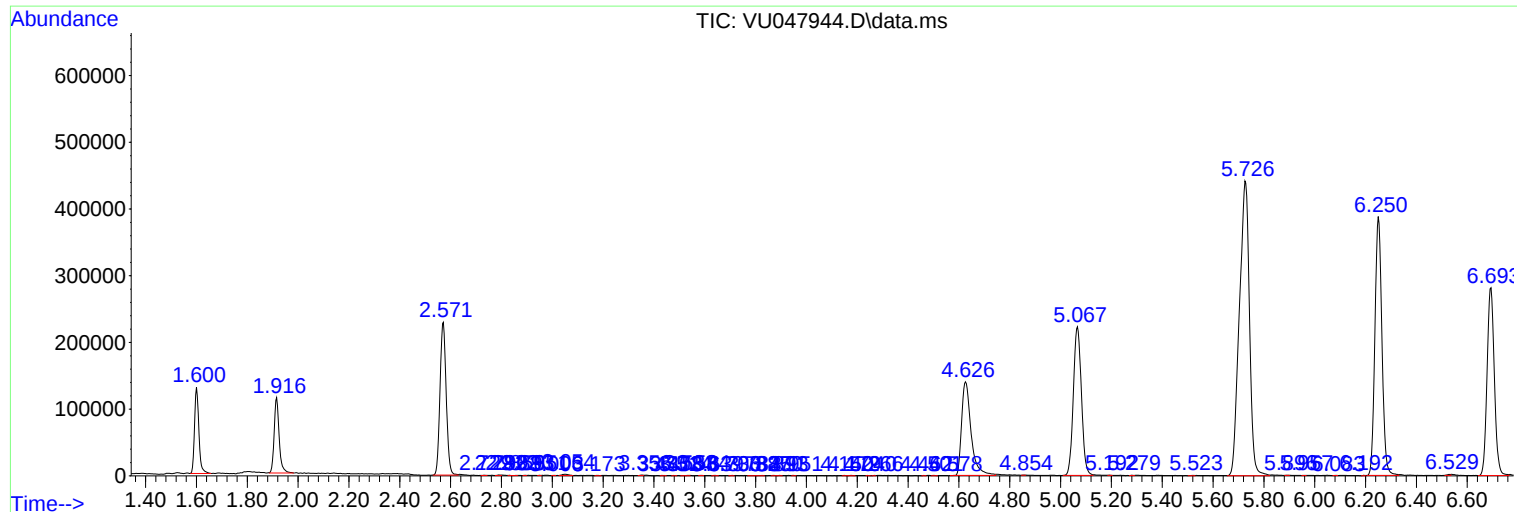

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047944.D
Acq On : 12 Apr 2022 10:51
Operator : SY/MD
Sample : N2316-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047944.D
Acq On : 12 Apr 2022 10:51
Operator : SY/MD
Sample : N2316-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc