

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047947.D
 Acq On : 12 Apr 2022 12:00
 Operator : SY/MD
 Sample : N2316-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV	197102	236065	15.76%	2.027%
2	1.912	169	178	195	rBV	155024	214157	14.30%	1.839%
3	2.517	364	366	369	rBV	311	240	0.02%	0.002%
4	2.568	370	382	401	rVV	324338	533062	35.59%	4.578%
5	2.681	414	417	419	rVB	427	240	0.02%	0.002%
6	2.707	419	425	428	rBV5	301	298	0.02%	0.003%
7	2.797	446	453	457	rBV4	617	801	0.05%	0.007%
8	2.954	498	502	503	rBV2	344	222	0.01%	0.002%
9	3.047	522	531	541	rVV4	2032	3456	0.23%	0.030%
10	3.170	566	569	573	rVB2	245	191	0.01%	0.002%
11	3.202	577	579	583	rVB2	271	193	0.01%	0.002%
12	3.353	622	626	627	rBV	388	233	0.02%	0.002%
13	3.491	665	669	672	rBV	235	252	0.02%	0.002%
14	3.523	674	679	686	rVB3	239	295	0.02%	0.003%
15	3.764	751	754	759	rVB3	257	265	0.02%	0.002%
16	3.877	784	789	791	rBV	297	245	0.02%	0.002%
17	3.977	817	820	822	rVV	241	192	0.01%	0.002%
18	4.105	856	860	862	rVB2	264	201	0.01%	0.002%
19	4.308	919	923	925	rBV2	293	190	0.01%	0.002%
20	4.430	957	961	963	rBV	282	212	0.01%	0.002%
21	4.623	1008	1021	1061	rBV	154848	384420	25.67%	3.301%
22	4.890	1101	1104	1108	rVB4	364	244	0.02%	0.002%
23	5.067	1142	1159	1181	rBV	268290	587546	39.23%	5.046%
24	5.224	1204	1208	1212	rVB3	321	288	0.02%	0.002%
25	5.247	1212	1215	1218	rBV	299	242	0.02%	0.002%
26	5.292	1223	1229	1233	rBV3	498	683	0.05%	0.006%
27	5.530	1298	1303	1306	rBV2	287	294	0.02%	0.003%
28	5.729	1342	1365	1394	rBV2	548461	1497837	100.00%	12.863%
29	6.038	1458	1461	1465	rVV3	360	346	0.02%	0.003%
30	6.124	1486	1488	1495	rVB	299	274	0.02%	0.002%
31	6.250	1513	1527	1554	rBV	412577	785708	52.46%	6.747%
32	6.382	1565	1568	1572	rVB3	586	378	0.03%	0.003%
33	6.420	1577	1580	1585	rVB3	429	338	0.02%	0.003%
34	6.533	1605	1615	1627	rVB7	2249	4553	0.30%	0.039%
35	6.600	1631	1636	1639	rVB3	460	454	0.03%	0.004%
36	6.620	1639	1642	1644	rBV2	420	266	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047947.D
 Acq On : 12 Apr 2022 12:00
 Operator : SY/MD
 Sample : N2316-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1689	rBV	338651	665872	44.46%	5.718%
38	6.970	1748	1751	1755	rVB2	292	205	0.01%	0.002%
39	6.996	1755	1759	1763	rBV2	358	255	0.02%	0.002%
40	7.028	1763	1769	1770	rBV2	216	208	0.01%	0.002%
41	7.182	1809	1817	1829	rVV4	3805	6883	0.46%	0.059%
42	7.382	1876	1879	1887	rVB2	325	485	0.03%	0.004%
43	7.568	1923	1937	1956	rBV	173978	309463	20.66%	2.658%
44	7.690	1968	1975	1979	rBV4	1844	2312	0.15%	0.020%
45	7.800	2004	2009	2014	rVB2	545	498	0.03%	0.004%
46	7.825	2014	2017	2020	rVB2	386	280	0.02%	0.002%
47	7.899	2027	2040	2056	rBV	686007	1186157	79.19%	10.186%
48	8.179	2113	2127	2148	rBV	123941	214915	14.35%	1.846%
49	8.475	2216	2219	2223	rVB	409	318	0.02%	0.003%
50	8.507	2226	2229	2233	rVB4	430	341	0.02%	0.003%
51	8.530	2233	2236	2240	rBV2	293	297	0.02%	0.003%
52	8.558	2240	2245	2247	rBV2	243	238	0.02%	0.002%
53	8.636	2255	2269	2303	rBV	480103	883018	58.95%	7.583%
54	8.915	2354	2356	2361	rVB3	415	307	0.02%	0.003%
55	8.967	2370	2372	2379	rVB3	394	253	0.02%	0.002%
56	9.195	2438	2443	2448	rBV3	316	287	0.02%	0.002%
57	9.221	2448	2451	2455	rBV3	258	240	0.02%	0.002%
58	9.292	2470	2473	2477	rVB2	359	279	0.02%	0.002%
59	9.317	2477	2481	2485	rBV2	340	306	0.02%	0.003%
60	9.417	2498	2512	2549	rBV	623719	1059460	70.73%	9.098%
61	9.648	2581	2584	2588	rVV2	199	197	0.01%	0.002%
62	9.690	2592	2597	2606	rVV4	1084	1499	0.10%	0.013%
63	9.806	2628	2633	2635	rBV3	227	203	0.01%	0.002%
64	9.951	2673	2678	2683	rBV2	241	269	0.02%	0.002%
65	10.102	2721	2725	2728	rBV	516	373	0.02%	0.003%
66	10.230	2762	2765	2770	rVB2	350	242	0.02%	0.002%
67	10.330	2793	2796	2802	rBV2	259	335	0.02%	0.003%
68	10.468	2836	2839	2842	rBV3	334	239	0.02%	0.002%
69	10.555	2863	2866	2869	rBV2	264	222	0.01%	0.002%
70	10.671	2895	2902	2914	rVB3	3048	4496	0.30%	0.039%
71	10.758	2915	2929	2948	rVV	499992	814819	54.40%	6.997%
72	10.828	2948	2951	2957	rVB3	447	322	0.02%	0.003%
73	10.867	2960	2963	2968	rBV3	386	371	0.02%	0.003%
74	10.925	2978	2981	2987	rVB	289	242	0.02%	0.002%
75	10.973	2992	2996	2999	rVB	330	209	0.01%	0.002%
76	11.002	2999	3005	3008	rBV4	425	404	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047947.D
 Acq On : 12 Apr 2022 12:00
 Operator : SY/MD
 Sample : N2316-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.118	3038	3041	3044	rBV2	342	256	0.02%	0.002%
78	11.205	3063	3068	3072	rBV4	373	420	0.03%	0.004%
79	11.459	3138	3147	3151	rBV4	2228	2987	0.20%	0.026%
80	11.504	3158	3161	3168	rVB2	322	200	0.01%	0.002%
81	11.539	3168	3172	3176	rVB2	301	235	0.02%	0.002%
82	11.584	3179	3186	3191	rBV4	524	624	0.04%	0.005%
83	11.697	3216	3221	3226	rBV4	1440	1279	0.09%	0.011%
84	11.751	3233	3238	3245	rVB5	738	874	0.06%	0.008%
85	11.812	3245	3257	3283	rBV	682708	1082622	72.28%	9.297%
86	12.021	3319	3322	3326	rVB2	272	200	0.01%	0.002%
87	12.099	3341	3346	3350	rBV2	323	370	0.02%	0.003%
88	12.195	3359	3376	3393	rBV	701104	1135872	75.83%	9.754%
89	12.398	3435	3439	3442	rBV3	536	497	0.03%	0.004%
90	12.504	3468	3472	3474	rBV2	335	263	0.02%	0.002%
91	12.539	3479	3483	3486	rBV	400	328	0.02%	0.003%
92	12.758	3540	3551	3553	rBV2	425	689	0.05%	0.006%
93	12.970	3614	3617	3620	rVB2	387	271	0.02%	0.002%
94	12.989	3620	3623	3626	rBV3	364	213	0.01%	0.002%
95	13.224	3692	3696	3698	rBV2	652	521	0.03%	0.004%
96	13.844	3886	3889	3898	rVB2	1293	1342	0.09%	0.012%
97	13.944	3917	3920	3924	rBV	346	278	0.02%	0.002%
98	14.169	3988	3990	3992	rBV3	319	212	0.01%	0.002%
99	14.333	4036	4041	4047	rVB4	1204	1573	0.11%	0.014%
100	14.549	4105	4108	4111	rBV2	493	347	0.02%	0.003%




Sum of corrected areas: 11644673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047947.D
Acq On : 12 Apr 2022 12:00
Operator : SY/MD
Sample : N2316-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

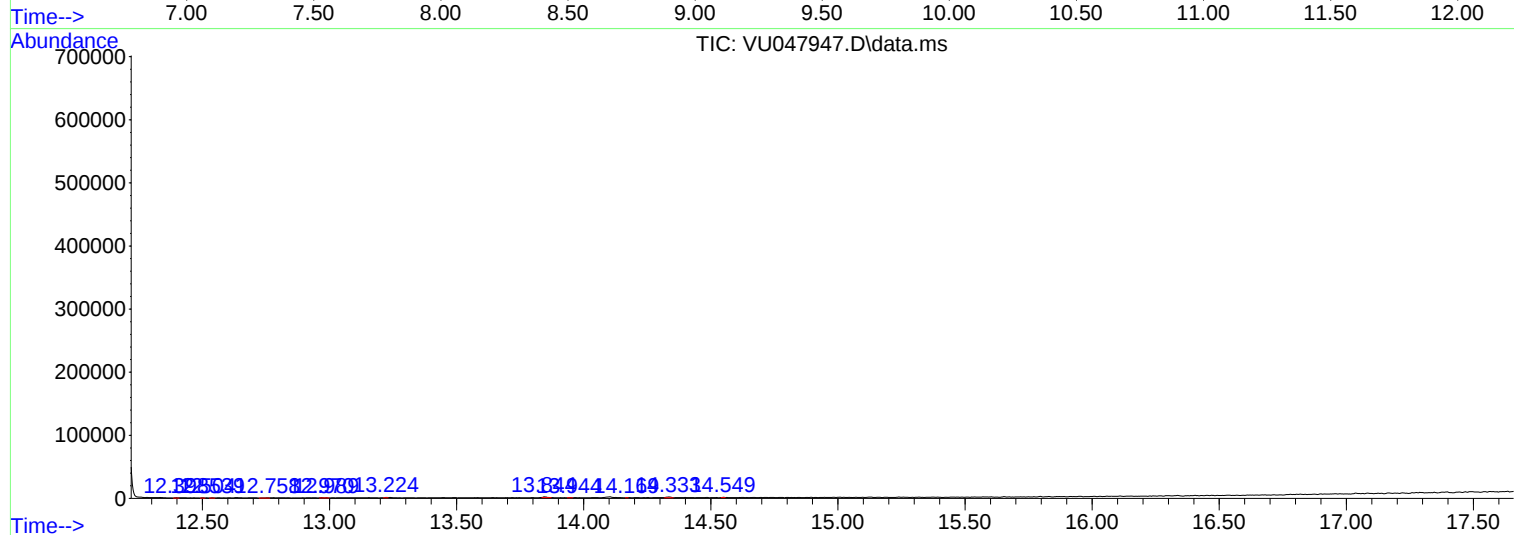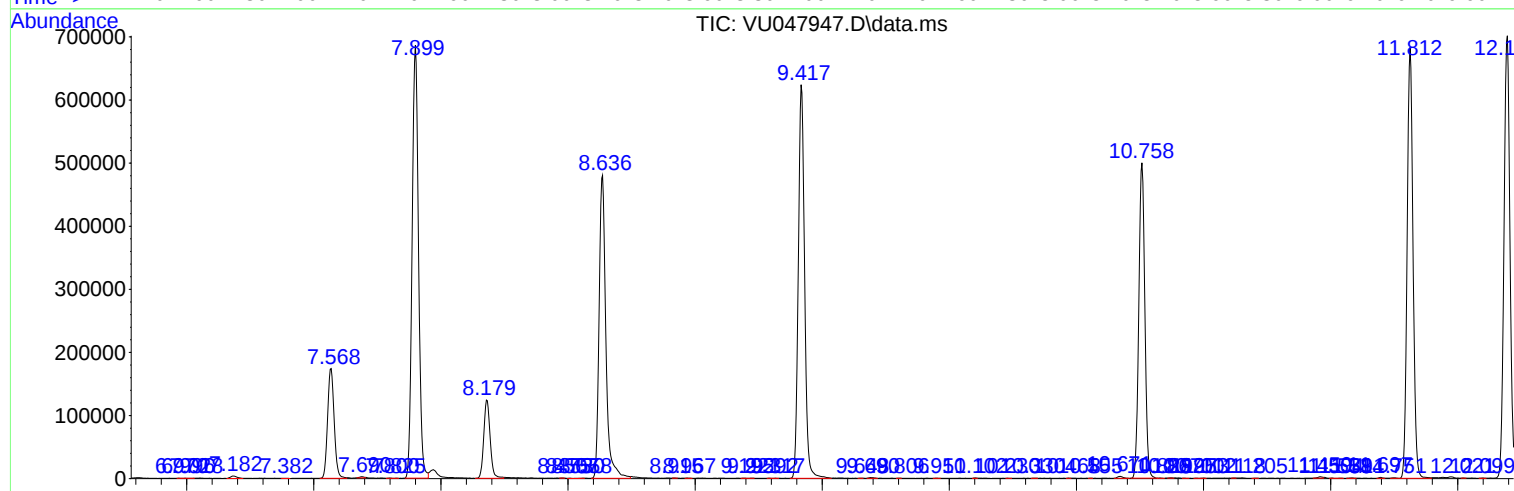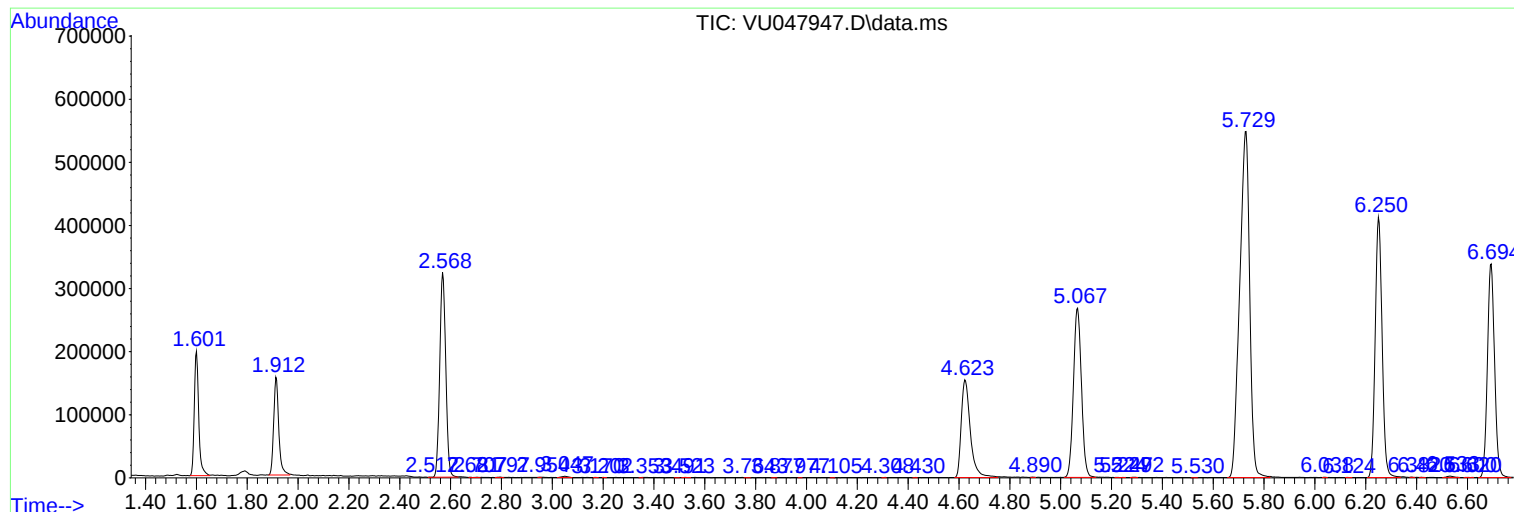

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047947.D
Acq On : 12 Apr 2022 12:00
Operator : SY/MD
Sample : N2316-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047947.D
Acq On : 12 Apr 2022 12:00
Operator : SY/MD
Sample : N2316-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------