

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047949.D
 Acq On : 12 Apr 2022 12:46
 Operator : SY/MD
 Sample : N2343-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	102	rVB	178709	209704	15.43%	1.951%
2	1.916	170	179	197	rVB	142639	192880	14.19%	1.794%
3	2.568	370	382	409	rBV	292506	485964	35.76%	4.521%
4	2.764	439	443	445	rBV2	277	241	0.02%	0.002%
5	2.838	462	466	469	rVB2	405	328	0.02%	0.003%
6	2.954	499	502	504	rBV3	446	286	0.02%	0.003%
7	3.012	515	520	522	rBV3	228	207	0.02%	0.002%
8	3.054	524	533	539	rVV5	1625	2596	0.19%	0.024%
9	3.108	547	550	553	rBV2	275	176	0.01%	0.002%
10	3.305	608	611	615	rBV	365	360	0.03%	0.003%
11	3.372	628	632	634	rVB2	245	196	0.01%	0.002%
12	3.427	646	649	653	rVB2	331	261	0.02%	0.002%
13	3.491	664	669	672	rBV2	262	218	0.02%	0.002%
14	3.543	681	685	693	rBV2	290	393	0.03%	0.004%
15	3.581	693	697	701	rVB	246	213	0.02%	0.002%
16	3.700	731	734	737	rVB2	243	172	0.01%	0.002%
17	3.784	758	760	764	rVB	260	171	0.01%	0.002%
18	4.006	825	829	833	rVV	171	216	0.02%	0.002%
19	4.208	889	892	895	rBV3	252	176	0.01%	0.002%
20	4.337	929	932	935	rBV	255	176	0.01%	0.002%
21	4.404	946	953	954	rBV	194	202	0.01%	0.002%
22	4.456	966	969	971	rBV	284	197	0.01%	0.002%
23	4.629	1009	1023	1070	rBV	129676	337527	24.84%	3.140%
24	4.989	1132	1135	1138	rBV2	263	200	0.01%	0.002%
25	5.067	1142	1159	1188	rVV	246181	536169	39.45%	4.988%
26	5.279	1223	1225	1226	rBV	449	209	0.02%	0.002%
27	5.420	1262	1269	1277	rVB2	290	528	0.04%	0.005%
28	5.485	1284	1289	1292	rBV2	197	190	0.01%	0.002%
29	5.607	1322	1327	1328	rBV2	338	233	0.02%	0.002%
30	5.729	1341	1365	1395	rBV2	503728	1358973	100.00%	12.641%
31	5.874	1407	1410	1412	rBV2	439	272	0.02%	0.003%
32	5.928	1424	1427	1431	rBV3	432	350	0.03%	0.003%
33	6.115	1481	1485	1489	rVV3	392	402	0.03%	0.004%
34	6.250	1511	1527	1560	rVV	396500	759325	55.87%	7.063%
35	6.436	1580	1585	1587	rBV3	343	281	0.02%	0.003%
36	6.504	1604	1606	1608	rBV2	403	212	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047949.D
 Acq On : 12 Apr 2022 12:46
 Operator : SY/MD
 Sample : N2343-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.530	1608	1614	1626	rVB5	1407	2642	0.19%	0.025%
38	6.623	1642	1643	1650	rVB2	275	214	0.02%	0.002%
39	6.694	1650	1665	1686	rBV	309313	608274	44.76%	5.658%
40	7.050	1772	1776	1784	rVV3	558	742	0.05%	0.007%
41	7.182	1808	1817	1828	rBV4	3197	5733	0.42%	0.053%
42	7.224	1828	1830	1835	rVB2	304	230	0.02%	0.002%
43	7.250	1835	1838	1843	rBV2	309	189	0.01%	0.002%
44	7.362	1869	1873	1876	rBV2	261	223	0.02%	0.002%
45	7.472	1904	1907	1910	rBV	245	196	0.01%	0.002%
46	7.568	1922	1937	1959	rBV	159295	284372	20.93%	2.645%
47	7.690	1968	1975	1983	rBV5	1949	3258	0.24%	0.030%
48	7.851	2021	2025	2026	rBV2	290	190	0.01%	0.002%
49	7.899	2027	2040	2055	rBV	618735	1073500	78.99%	9.986%
50	8.179	2114	2127	2144	rBV2	112212	193402	14.23%	1.799%
51	8.298	2161	2164	2167	rBV3	385	317	0.02%	0.003%
52	8.407	2196	2198	2202	rVB	413	278	0.02%	0.003%
53	8.443	2207	2209	2211	rBV	269	173	0.01%	0.002%
54	8.465	2213	2216	2218	rBV2	863	562	0.04%	0.005%
55	8.546	2236	2241	2244	rBV4	451	379	0.03%	0.004%
56	8.565	2244	2247	2250	rVB2	315	194	0.01%	0.002%
57	8.636	2255	2269	2298	rBV	429758	794552	58.47%	7.391%
58	8.883	2344	2346	2350	rVB3	569	347	0.03%	0.003%
59	8.919	2355	2357	2361	rVV2	247	202	0.01%	0.002%
60	8.996	2377	2381	2383	rVV	250	205	0.02%	0.002%
61	9.063	2400	2402	2405	rBV2	347	239	0.02%	0.002%
62	9.118	2415	2419	2422	rBV2	566	562	0.04%	0.005%
63	9.156	2427	2431	2442	rBV4	571	882	0.06%	0.008%
64	9.201	2442	2445	2448	rBV3	266	223	0.02%	0.002%
65	9.417	2498	2512	2533	rBV	607886	1023458	75.31%	9.520%
66	9.571	2554	2560	2562	rBV3	533	661	0.05%	0.006%
67	9.587	2562	2565	2567	rVV3	296	216	0.02%	0.002%
68	9.697	2590	2599	2607	rBV6	1177	1736	0.13%	0.016%
69	9.761	2615	2619	2622	rBV	250	196	0.01%	0.002%
70	9.787	2624	2627	2632	rVB2	396	312	0.02%	0.003%
71	9.841	2641	2644	2648	rVB2	293	199	0.01%	0.002%
72	9.864	2648	2651	2655	rVB2	232	173	0.01%	0.002%
73	9.893	2655	2660	2662	rBV	261	233	0.02%	0.002%
74	9.944	2673	2676	2678	rBV	304	221	0.02%	0.002%
75	10.227	2761	2764	2767	rVB2	293	170	0.01%	0.002%
76	10.671	2894	2902	2911	rVB4	2989	4205	0.31%	0.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047949.D
 Acq On : 12 Apr 2022 12:46
 Operator : SY/MD
 Sample : N2343-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.758	2913	2929	2956	rVB	456764	747153	54.98%	6.950%
78	10.861	2957	2961	2963	rBV3	707	495	0.04%	0.005%
79	10.896	2968	2972	2977	rVB3	1573	1569	0.12%	0.015%
80	11.002	3001	3005	3009	rVB3	422	369	0.03%	0.003%
81	11.034	3009	3015	3017	rBV2	518	477	0.04%	0.004%
82	11.095	3031	3034	3036	rBV	365	246	0.02%	0.002%
83	11.459	3140	3147	3159	rVB5	1826	3334	0.25%	0.031%
84	11.574	3181	3183	3188	rBV2	362	263	0.02%	0.002%
85	11.632	3197	3201	3206	rBV3	341	333	0.02%	0.003%
86	11.697	3215	3221	3228	rVB4	1324	1786	0.13%	0.017%
87	11.738	3228	3234	3235	rBV3	750	579	0.04%	0.005%
88	11.812	3241	3257	3283	rBV	658735	1054424	77.59%	9.808%
89	11.944	3293	3298	3302	rBV6	991	1302	0.10%	0.012%
90	11.976	3303	3308	3315	rVV4	1702	2341	0.17%	0.022%
91	12.018	3319	3321	3327	rVB2	543	565	0.04%	0.005%
92	12.086	3338	3342	3344	rBV2	278	213	0.02%	0.002%
93	12.195	3358	3376	3398	rBV	632294	1036211	76.25%	9.639%
94	12.324	3413	3416	3428	rVB7	770	1250	0.09%	0.012%
95	12.443	3451	3453	3456	rBV2	303	200	0.01%	0.002%
96	12.465	3456	3460	3464	rVV2	417	346	0.03%	0.003%
97	12.635	3508	3513	3514	rBV	462	389	0.03%	0.004%
98	12.764	3550	3553	3554	rBV2	363	221	0.02%	0.002%
99	13.221	3693	3695	3698	rBV2	360	273	0.02%	0.003%
100	13.848	3884	3890	3898	rVB6	1308	1544	0.11%	0.014%




Sum of corrected areas: 10750147

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047949.D
Acq On : 12 Apr 2022 12:46
Operator : SY/MD
Sample : N2343-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

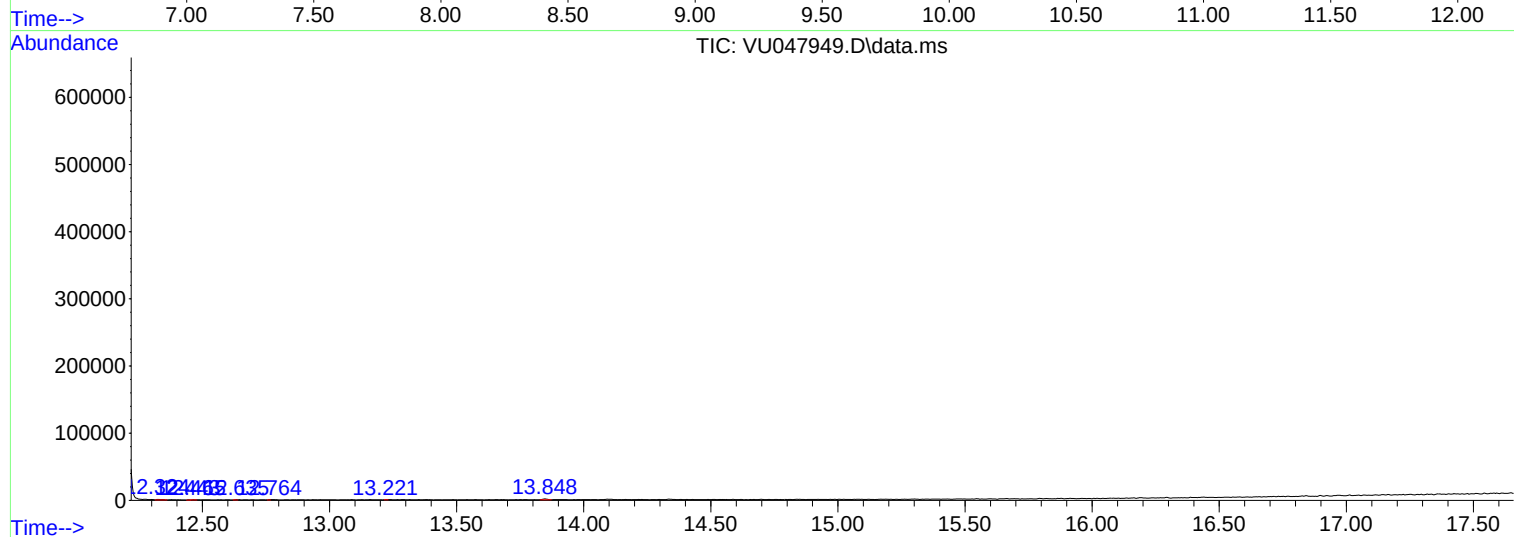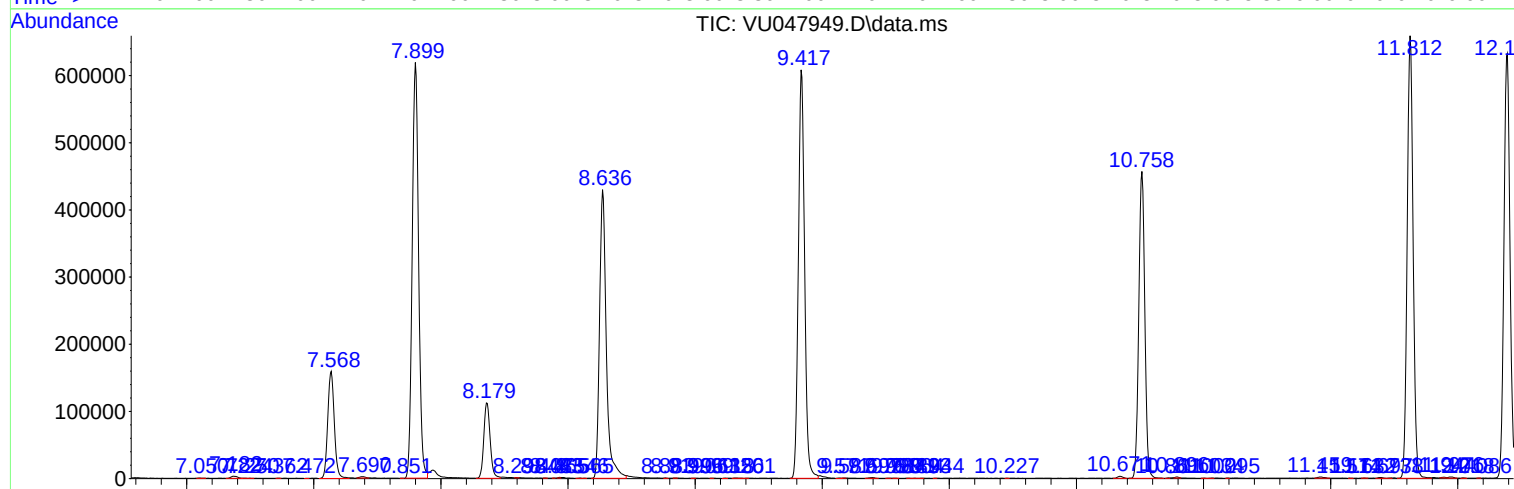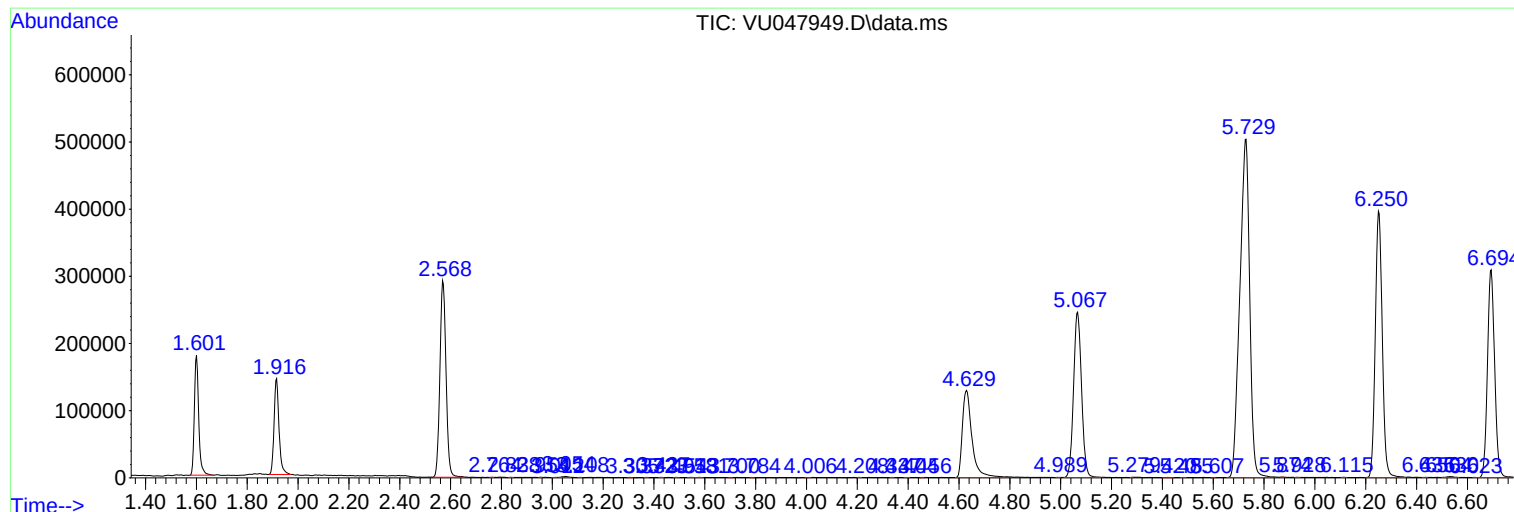

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047949.D
Acq On : 12 Apr 2022 12:46
Operator : SY/MD
Sample : N2343-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047949.D
Acq On : 12 Apr 2022 12:46
Operator : SY/MD
Sample : N2343-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------