

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047962.D
 Acq On : 12 Apr 2022 17:41
 Operator : SY/MD
 Sample : N2345-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	101	rVB	169532	198560	15.29%	1.988%
2	1.774	128	135	142	rVB5	9246	11622	0.89%	0.116%
3	1.912	170	178	198	rBV	125964	182283	14.03%	1.825%
4	2.568	369	382	395	rBV	277156	452404	34.83%	4.531%
5	2.668	411	413	417	rVB3	408	280	0.02%	0.003%
6	2.739	431	435	437	rBV	494	386	0.03%	0.004%
7	2.781	445	448	449	rBV2	428	234	0.02%	0.002%
8	2.893	476	483	486	rBV3	411	574	0.04%	0.006%
9	3.044	526	530	532	rBV2	643	456	0.04%	0.005%
10	3.118	546	553	556	rBV2	373	524	0.04%	0.005%
11	3.189	562	575	591	rVB	3399	7728	0.59%	0.077%
12	3.250	591	594	596	rBV	380	270	0.02%	0.003%
13	3.285	602	605	608	rBV3	233	211	0.02%	0.002%
14	3.324	612	617	621	rBV2	400	404	0.03%	0.004%
15	3.359	621	628	634	rBV4	561	675	0.05%	0.007%
16	3.382	634	635	639	rVB	474	218	0.02%	0.002%
17	3.408	639	643	649	rBV2	453	595	0.05%	0.006%
18	3.607	698	705	707	rBV2	342	341	0.03%	0.003%
19	3.623	707	710	715	rVV2	275	265	0.02%	0.003%
20	3.871	784	787	792	rBV2	356	303	0.02%	0.003%
21	3.977	816	820	824	rBV3	376	430	0.03%	0.004%
22	4.022	830	834	838	rVB2	444	283	0.02%	0.003%
23	4.620	1006	1020	1055	rBV	132058	317528	24.45%	3.180%
24	4.986	1128	1134	1136	rBV3	314	224	0.02%	0.002%
25	5.067	1143	1159	1184	rBV	226692	499136	38.43%	4.999%
26	5.327	1237	1240	1242	rBV2	360	248	0.02%	0.002%
27	5.391	1256	1260	1267	rVB4	335	369	0.03%	0.004%
28	5.533	1300	1304	1307	rVV3	343	250	0.02%	0.003%
29	5.726	1342	1364	1374	rBV2	472046	1298945	100.00%	13.008%
30	6.047	1460	1464	1465	rBV2	328	222	0.02%	0.002%
31	6.092	1476	1478	1482	rVB3	337	224	0.02%	0.002%
32	6.115	1482	1485	1487	rBV3	431	270	0.02%	0.003%
33	6.173	1500	1503	1509	rVB3	296	261	0.02%	0.003%
34	6.198	1509	1511	1513	rBV3	428	273	0.02%	0.003%
35	6.250	1513	1527	1551	rBV	248739	475152	36.58%	4.758%
36	6.481	1594	1599	1601	rBV2	354	303	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047962.D
 Acq On : 12 Apr 2022 17:41
 Operator : SY/MD
 Sample : N2345-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.526	1608	1613	1616	rBV3	1132	1354	0.10%	0.014%
38	6.607	1635	1638	1640	rVB2	399	225	0.02%	0.002%
39	6.694	1649	1665	1688	rBV	291895	569054	43.81%	5.699%
40	6.806	1698	1700	1706	rVB2	742	435	0.03%	0.004%
41	7.044	1769	1774	1775	rBV3	254	232	0.02%	0.002%
42	7.128	1795	1800	1805	rVV4	354	438	0.03%	0.004%
43	7.182	1808	1817	1829	rBV4	3337	6154	0.47%	0.062%
44	7.333	1860	1864	1867	rBV	318	232	0.02%	0.002%
45	7.568	1924	1937	1963	rBV	148393	263294	20.27%	2.637%
46	7.658	1963	1965	1968	rVV2	549	401	0.03%	0.004%
47	7.687	1968	1974	1987	rVB7	2216	3939	0.30%	0.039%
48	7.899	2026	2040	2056	rBV	586834	1009174	77.69%	10.106%
49	8.179	2116	2127	2145	rBV	104278	179269	13.80%	1.795%
50	8.401	2192	2196	2198	rVB4	458	344	0.03%	0.003%
51	8.462	2211	2215	2216	rBV	1209	749	0.06%	0.008%
52	8.632	2255	2268	2301	rBV	384425	710352	54.69%	7.114%
53	8.925	2354	2359	2362	rBV4	604	519	0.04%	0.005%
54	9.137	2420	2425	2429	rBV3	371	318	0.02%	0.003%
55	9.176	2433	2437	2440	rBV4	304	266	0.02%	0.003%
56	9.311	2477	2479	2485	rVB3	246	213	0.02%	0.002%
57	9.420	2498	2513	2515	rBV	403669	556193	42.82%	5.570%
58	9.565	2555	2558	2568	rVB5	1287	1837	0.14%	0.018%
59	9.607	2568	2571	2575	rVB2	338	302	0.02%	0.003%
60	9.697	2590	2599	2604	rBV5	1274	2023	0.16%	0.020%
61	9.719	2604	2606	2610	rVB2	435	237	0.02%	0.002%
62	9.880	2654	2656	2664	rVB2	185	214	0.02%	0.002%
63	10.047	2705	2708	2714	rVV2	378	301	0.02%	0.003%
64	10.095	2720	2723	2726	rBV	814	732	0.06%	0.007%
65	10.111	2726	2728	2735	rVB4	1022	816	0.06%	0.008%
66	10.484	2841	2844	2848	rVB2	393	250	0.02%	0.003%
67	10.603	2877	2881	2887	rVB	281	244	0.02%	0.002%
68	10.671	2894	2902	2910	rVB3	2495	3674	0.28%	0.037%
69	10.758	2916	2929	2949	rVV	430408	697295	53.68%	6.983%
70	10.854	2954	2959	2961	rBV3	323	257	0.02%	0.003%
71	10.893	2961	2971	2979	rBV3	3086	5297	0.41%	0.053%
72	11.089	3030	3032	3034	rBV2	345	242	0.02%	0.002%
73	11.176	3056	3059	3061	rBV	311	221	0.02%	0.002%
74	11.256	3081	3084	3087	rVB3	319	221	0.02%	0.002%
75	11.420	3129	3135	3139	rBV2	421	595	0.05%	0.006%
76	11.465	3141	3149	3162	rVV9	1948	3819	0.29%	0.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047962.D
 Acq On : 12 Apr 2022 17:41
 Operator : SY/MD
 Sample : N2345-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.690	3213	3219	3221	rBV4	1099	971	0.07%	0.010%
78	11.748	3226	3237	3246	rBV	18497	28497	2.19%	0.285%
79	11.812	3246	3257	3281	rVV2	442558	1153255	88.78%	11.549%
80	11.941	3294	3297	3299	rBV3	909	626	0.05%	0.006%
81	11.957	3299	3302	3305	rBV3	928	722	0.06%	0.007%
82	12.070	3324	3337	3352	rBV7	4660	9722	0.75%	0.097%
83	12.195	3362	3376	3398	rBV2	635413	1241382	95.57%	12.432%
84	12.369	3427	3430	3434	rBV2	393	419	0.03%	0.004%
85	12.414	3441	3444	3448	rBV3	520	502	0.04%	0.005%
86	12.587	3495	3498	3500	rBV2	310	211	0.02%	0.002%
87	12.684	3524	3528	3532	rBV3	349	401	0.03%	0.004%
88	12.774	3550	3556	3567	rVB5	1048	1672	0.13%	0.017%
89	12.973	3611	3618	3628	rBV3	3317	5037	0.39%	0.050%
90	13.024	3630	3634	3639	rBV3	299	276	0.02%	0.003%
91	13.047	3639	3641	3645	rBV	290	226	0.02%	0.002%
92	13.330	3723	3729	3735	rBV4	1740	2424	0.19%	0.024%
93	13.378	3737	3744	3755	rVB4	5975	8351	0.64%	0.084%
94	13.555	3796	3799	3802	rBV	326	223	0.02%	0.002%
95	13.844	3882	3889	3898	rVB5	4462	7102	0.55%	0.071%
96	14.098	3965	3968	3970	rBV	673	519	0.04%	0.005%
97	14.362	4046	4050	4061	rVB4	3563	4360	0.34%	0.044%
98	15.420	4377	4379	4383	rBV3	760	501	0.04%	0.005%
99	15.545	4410	4418	4428	rVB3	16252	24232	1.87%	0.243%
100	16.391	4674	4681	4688	rBV5	14435	19651	1.51%	0.197%

Sum of corrected areas: 9985465




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047962.D
Acq On : 12 Apr 2022 17:41
Operator : SY/MD
Sample : N2345-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

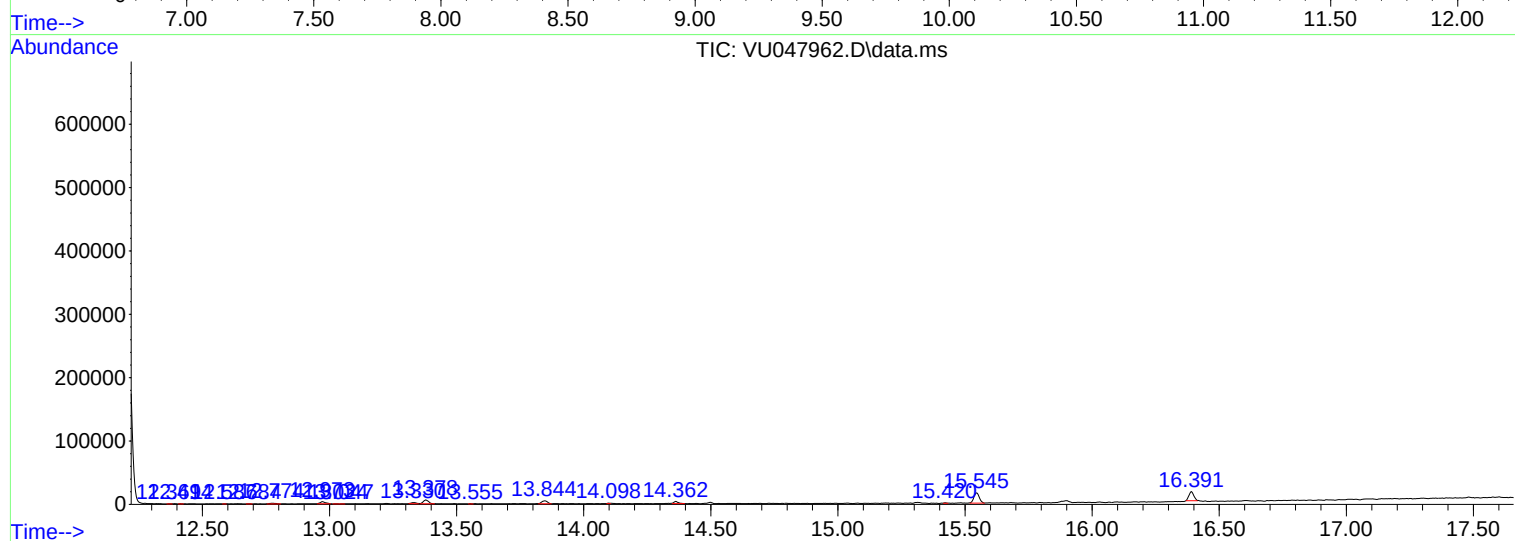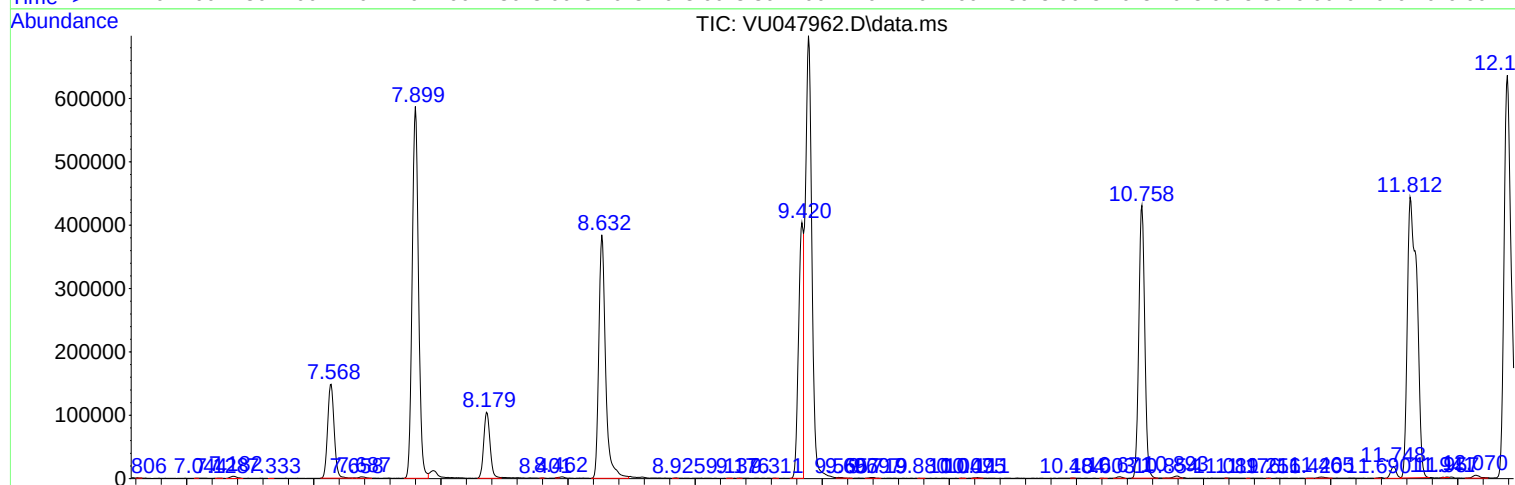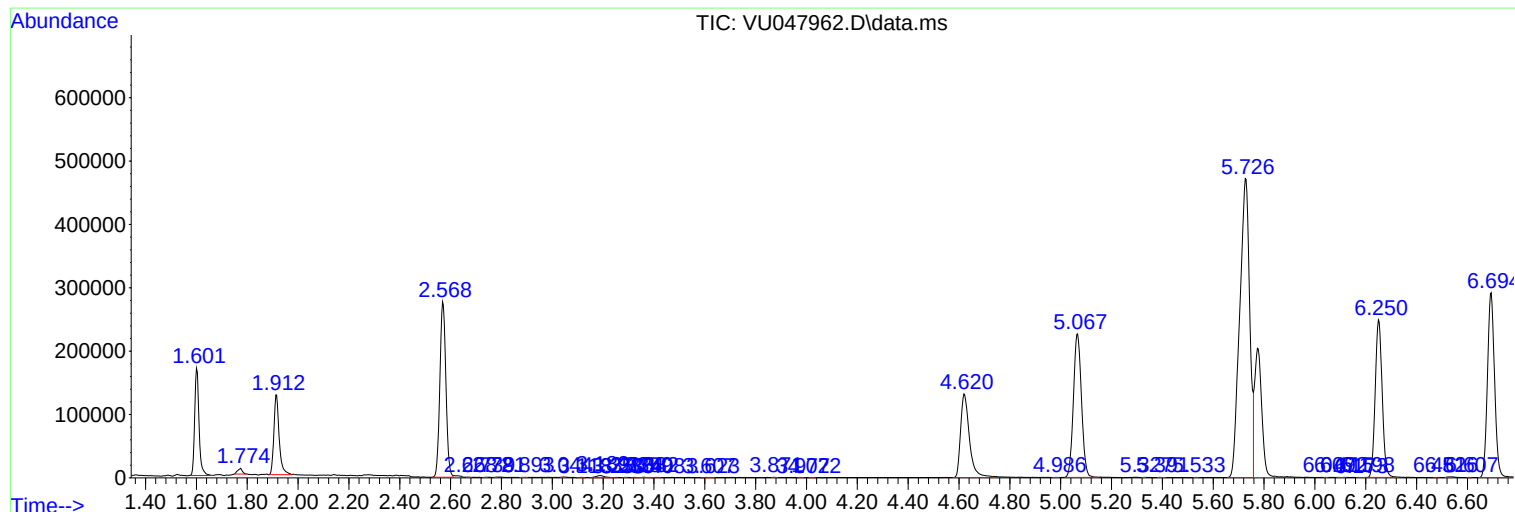

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047962.D
Acq On : 12 Apr 2022 17:41
Operator : SY/MD
Sample : N2345-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047962.D
Acq On : 12 Apr 2022 17:41
Operator : SY/MD
Sample : N2345-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------