

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047972.D
 Acq On : 12 Apr 2022 21:43
 Operator : SY/MD
 Sample : VU0412WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK087

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	101	rVB	176629	204768	15.18%	1.896%
2	1.915	170	179	197	rBV	137926	191953	14.23%	1.778%
3	2.571	370	383	404	rVB	291156	479369	35.53%	4.439%
4	2.700	420	423	427	rVB3	387	328	0.02%	0.003%
5	2.723	427	430	433	rVV3	338	253	0.02%	0.002%
6	2.761	436	442	444	rBV2	484	578	0.04%	0.005%
7	2.796	447	453	461	rVB3	1094	1679	0.12%	0.016%
8	3.054	524	533	541	rBV5	1943	3689	0.27%	0.034%
9	3.160	562	566	567	rBV2	378	321	0.02%	0.003%
10	3.189	571	575	579	rVV2	420	482	0.04%	0.004%
11	3.218	581	584	590	rVV2	264	253	0.02%	0.002%
12	3.359	623	628	632	rBV3	376	387	0.03%	0.004%
13	3.391	636	638	645	rVB	426	355	0.03%	0.003%
14	3.449	652	656	662	rVB2	342	325	0.02%	0.003%
15	3.513	670	676	680	rBV2	391	511	0.04%	0.005%
16	3.578	691	696	700	rBV3	214	288	0.02%	0.003%
17	3.665	719	723	726	rVB3	406	299	0.02%	0.003%
18	3.767	751	755	763	rVB2	326	318	0.02%	0.003%
19	3.880	786	790	792	rBV2	277	269	0.02%	0.002%
20	3.951	806	812	815	rBV3	301	290	0.02%	0.003%
21	4.208	888	892	894	rBV	358	274	0.02%	0.003%
22	4.276	908	913	918	rBV2	256	308	0.02%	0.003%
23	4.433	959	962	970	rVV3	296	419	0.03%	0.004%
24	4.620	1007	1020	1056	rBV	137881	338228	25.07%	3.132%
25	4.957	1122	1125	1132	rVB4	523	435	0.03%	0.004%
26	5.066	1142	1159	1185	rBV	240166	528515	39.18%	4.894%
27	5.288	1222	1228	1232	rBV3	435	503	0.04%	0.005%
28	5.468	1278	1284	1288	rBV2	213	261	0.02%	0.002%
29	5.526	1300	1302	1309	rVB3	388	397	0.03%	0.004%
30	5.558	1309	1312	1316	rBV2	253	270	0.02%	0.003%
31	5.729	1341	1365	1394	rBV2	497399	1349070	100.00%	12.493%
32	5.896	1415	1417	1421	rBV3	438	308	0.02%	0.003%
33	6.047	1460	1464	1470	rVB3	704	597	0.04%	0.006%
34	6.250	1512	1527	1550	rBV	406530	776804	57.58%	7.193%
35	6.533	1607	1615	1622	rBV4	1908	3075	0.23%	0.028%
36	6.693	1650	1665	1694	rBV	309013	607068	45.00%	5.622%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047972.D
 Acq On : 12 Apr 2022 21:43
 Operator : SY/MD
 Sample : VU0412WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK087

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.906	1728	1731	1734	rBV2	415	287	0.02%	0.003%
38	7.047	1772	1775	1778	rVB3	381	253	0.02%	0.002%
39	7.185	1809	1818	1833	rVV3	3882	6386	0.47%	0.059%
40	7.330	1859	1863	1865	rBV2	376	267	0.02%	0.002%
41	7.365	1869	1874	1876	rBV2	325	339	0.03%	0.003%
42	7.468	1900	1906	1912	rBV3	280	369	0.03%	0.003%
43	7.568	1924	1937	1963	rBV	156299	276553	20.50%	2.561%
44	7.687	1968	1974	1980	rBV4	2130	2593	0.19%	0.024%
45	7.732	1986	1988	1992	rVB3	446	305	0.02%	0.003%
46	7.767	1992	1999	2000	rBV2	352	299	0.02%	0.003%
47	7.796	2004	2008	2016	rVV4	1356	1778	0.13%	0.016%
48	7.899	2026	2040	2056	rBV	616525	1075023	79.69%	9.955%
49	8.179	2116	2127	2146	rBV	109217	187970	13.93%	1.741%
50	8.398	2190	2195	2198	rBV4	429	495	0.04%	0.005%
51	8.465	2214	2216	2222	rVB3	354	258	0.02%	0.002%
52	8.552	2239	2243	2250	rBV4	755	759	0.06%	0.007%
53	8.632	2255	2268	2315	rBV	397596	769475	57.04%	7.126%
54	9.008	2379	2385	2386	rBV2	475	366	0.03%	0.003%
55	9.243	2453	2458	2462	rBV3	290	308	0.02%	0.003%
56	9.417	2499	2512	2551	rBV	613708	1044924	77.46%	9.676%
57	9.574	2556	2561	2568	rVB3	861	1117	0.08%	0.010%
58	9.655	2582	2586	2589	rBV3	341	254	0.02%	0.002%
59	9.693	2592	2598	2606	rVV4	1386	2002	0.15%	0.019%
60	9.819	2634	2637	2644	rVB3	318	350	0.03%	0.003%
61	9.870	2651	2653	2662	rVB2	299	265	0.02%	0.002%
62	9.992	2688	2691	2694	rVV2	377	258	0.02%	0.002%
63	10.111	2718	2728	2730	rBV4	958	1387	0.10%	0.013%
64	10.314	2782	2791	2792	rBV	294	311	0.02%	0.003%
65	10.478	2837	2842	2844	rBV2	351	317	0.02%	0.003%
66	10.494	2844	2847	2855	rVB3	746	707	0.05%	0.007%
67	10.671	2894	2902	2910	rBV3	2278	3123	0.23%	0.029%
68	10.758	2916	2929	2947	rBV	445291	728830	54.02%	6.749%
69	10.867	2958	2963	2966	rBV	395	454	0.03%	0.004%
70	11.050	3016	3020	3024	rVB3	358	311	0.02%	0.003%
71	11.092	3027	3033	3036	rBV2	883	1043	0.08%	0.010%
72	11.211	3065	3070	3072	rBV4	329	292	0.02%	0.003%
73	11.359	3113	3116	3119	rBV2	408	317	0.02%	0.003%
74	11.468	3138	3150	3161	rBV7	2474	4766	0.35%	0.044%
75	11.693	3215	3220	3224	rBV5	1038	1057	0.08%	0.010%
76	11.751	3230	3238	3243	rBV3	1416	1756	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047972.D
 Acq On : 12 Apr 2022 21:43
 Operator : SY/MD
 Sample : VU0412WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK087

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.812	3244	3257	3274	rBV	672132	1078623	79.95%	9.988%
78	11.973	3303	3307	3318	rVB6	2049	2588	0.19%	0.024%
79	12.105	3346	3348	3352	rVV3	300	250	0.02%	0.002%
80	12.195	3362	3376	3395	rBV	623218	1030886	76.41%	9.546%
81	12.397	3436	3439	3442	rVB2	541	326	0.02%	0.003%
82	12.455	3454	3457	3462	rBV3	257	248	0.02%	0.002%
83	12.532	3474	3481	3486	rBV4	517	684	0.05%	0.006%
84	12.574	3489	3494	3499	rBB2	340	372	0.03%	0.003%
85	12.976	3613	3619	3627	rBV3	1742	2369	0.18%	0.022%
86	13.063	3643	3646	3649	rBV2	413	300	0.02%	0.003%
87	13.227	3689	3697	3703	rVB5	1920	2809	0.21%	0.026%
88	13.333	3724	3730	3735	rVB4	745	953	0.07%	0.009%
89	13.378	3740	3744	3745	rBV3	1185	835	0.06%	0.008%
90	13.847	3882	3890	3898	rBV4	3975	5523	0.41%	0.051%
91	14.092	3956	3966	3979	rBV	11904	19006	1.41%	0.176%
92	14.333	4033	4041	4050	rBV5	4197	7322	0.54%	0.068%
93	14.442	4073	4075	4080	rVB3	466	300	0.02%	0.003%
94	14.500	4089	4093	4100	rVB3	1011	1060	0.08%	0.010%
95	14.536	4100	4104	4107	rBV2	645	513	0.04%	0.005%
96	14.661	4141	4143	4151	rVB4	542	485	0.04%	0.004%
97	14.979	4240	4242	4247	rBV2	523	342	0.03%	0.003%
98	15.053	4263	4265	4267	rBV2	546	295	0.02%	0.003%
99	15.545	4411	4418	4430	rBV9	6132	9598	0.71%	0.089%
100	15.892	4515	4526	4541	rVB4	8845	21890	1.62%	0.203%



Sum of corrected areas: 10798748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047972.D
Acq On : 12 Apr 2022 21:43
Operator : SY/MD
Sample : VU0412WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK087

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

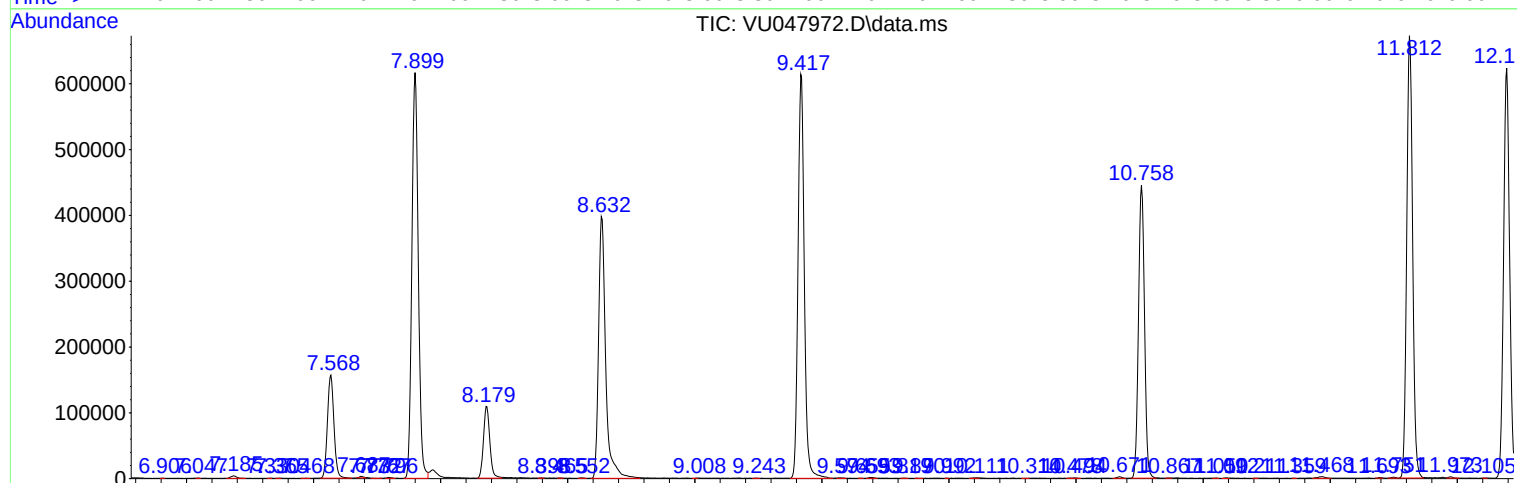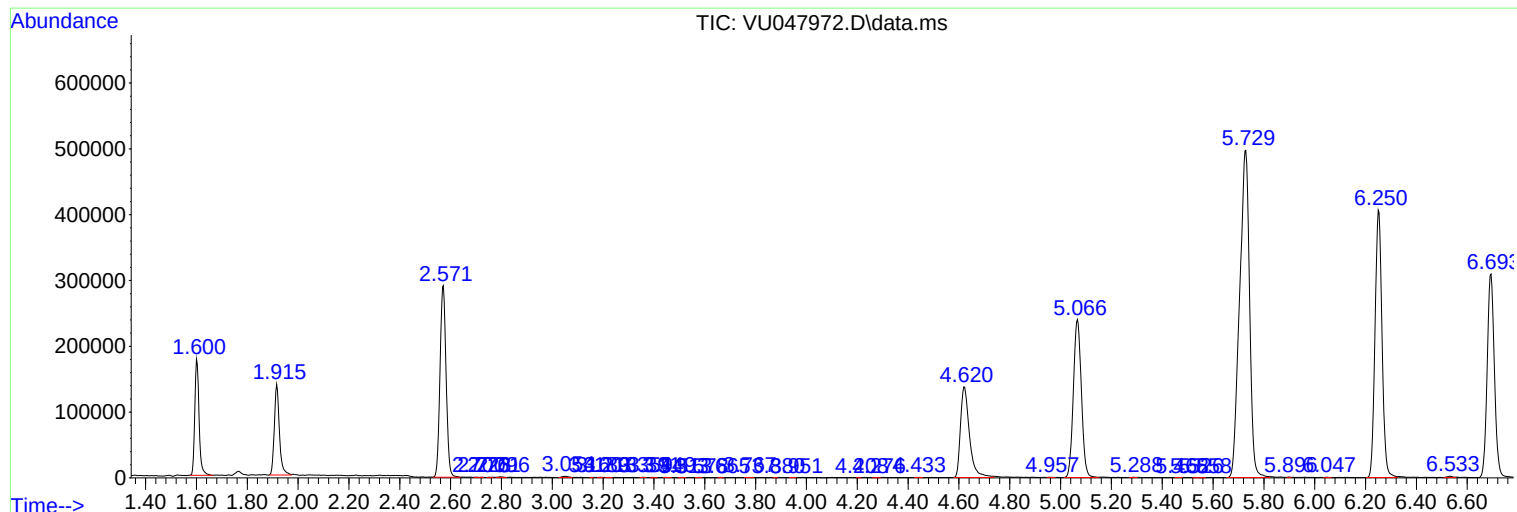

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047972.D
Acq On : 12 Apr 2022 21:43
Operator : SY/MD
Sample : VU0412WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK087

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047972.D
Acq On : 12 Apr 2022 21:43
Operator : SY/MD
Sample : VU0412WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK087

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc