

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047977.D
 Acq On : 12 Apr 2022 23:38
 Operator : SY/MD
 Sample : N2345-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	97	rBV	168519	196914	14.07%	1.800%
2	1.916	171	179	193	rBV	140063	185068	13.22%	1.692%
3	2.498	354	360	366	rVB3	747	789	0.06%	0.007%
4	2.571	370	383	401	rBV	278004	466535	33.32%	4.264%
5	3.176	559	571	574	rBV3	870	1215	0.09%	0.011%
6	3.350	619	625	628	rBV2	290	326	0.02%	0.003%
7	3.401	639	641	647	rVB2	334	318	0.02%	0.003%
8	3.523	677	679	684	rBV	458	401	0.03%	0.004%
9	3.655	716	720	725	rVB2	356	274	0.02%	0.003%
10	3.681	725	728	730	rBV2	403	278	0.02%	0.003%
11	3.716	736	739	742	rBV2	340	247	0.02%	0.002%
12	3.774	754	757	761	rBV2	447	389	0.03%	0.004%
13	3.842	774	778	782	rVV3	478	467	0.03%	0.004%
14	3.896	789	795	798	rBV3	241	239	0.02%	0.002%
15	3.912	798	800	804	rVB2	324	260	0.02%	0.002%
16	4.269	908	911	917	rVV2	246	266	0.02%	0.002%
17	4.333	924	931	935	rBB2	252	291	0.02%	0.003%
18	4.414	952	956	958	rBV2	293	262	0.02%	0.002%
19	4.629	1009	1023	1056	rBV	130690	346338	24.74%	3.166%
20	4.925	1109	1115	1119	rBV	388	360	0.03%	0.003%
21	4.983	1130	1133	1138	rVB3	310	277	0.02%	0.003%
22	5.067	1142	1159	1185	rBV2	237886	521876	37.28%	4.770%
23	5.192	1195	1198	1200	rVB2	524	286	0.02%	0.003%
24	5.208	1200	1203	1206	rVV3	370	253	0.02%	0.002%
25	5.288	1223	1228	1231	rBV2	738	679	0.05%	0.006%
26	5.530	1300	1303	1309	rVV2	338	351	0.03%	0.003%
27	5.636	1331	1336	1342	rVB	285	363	0.03%	0.003%
28	5.729	1342	1365	1400	rBV2	489154	1399996	100.00%	12.797%
29	5.931	1422	1428	1433	rBV4	492	620	0.04%	0.006%
30	5.977	1438	1442	1444	rBV2	430	299	0.02%	0.003%
31	6.041	1459	1462	1468	rVB4	444	442	0.03%	0.004%
32	6.185	1502	1507	1513	rVB3	332	453	0.03%	0.004%
33	6.250	1513	1527	1555	rBV	404935	777354	55.53%	7.106%
34	6.481	1597	1599	1604	rVB2	336	238	0.02%	0.002%
35	6.530	1607	1614	1622	rBV4	1296	2200	0.16%	0.020%
36	6.587	1628	1632	1637	rVB3	588	487	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047977.D
 Acq On : 12 Apr 2022 23:38
 Operator : SY/MD
 Sample : N2345-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1650	1665	1695	rBV	302587	597048	42.65%	5.457%
38	6.938	1736	1741	1746	rBV3	328	411	0.03%	0.004%
39	7.047	1767	1775	1777	rBV4	641	711	0.05%	0.006%
40	7.185	1807	1818	1830	rVV4	3519	6894	0.49%	0.063%
41	7.230	1830	1832	1836	rVB3	487	354	0.03%	0.003%
42	7.427	1888	1893	1897	rBV2	354	317	0.02%	0.003%
43	7.446	1897	1899	1903	rBV3	339	273	0.02%	0.002%
44	7.484	1908	1911	1915	rBV3	358	339	0.02%	0.003%
45	7.568	1922	1937	1959	rBV	153072	271758	19.41%	2.484%
46	7.687	1968	1974	1983	rBV4	2053	3317	0.24%	0.030%
47	7.822	2014	2016	2023	rBV2	237	268	0.02%	0.002%
48	7.899	2023	2040	2056	rBV	600592	1047460	74.82%	9.574%
49	8.089	2095	2099	2109	rVB5	705	986	0.07%	0.009%
50	8.182	2115	2128	2147	rBV	104631	183388	13.10%	1.676%
51	8.436	2203	2207	2209	rBV2	286	263	0.02%	0.002%
52	8.468	2210	2217	2229	rVB3	2651	5371	0.38%	0.049%
53	8.536	2235	2238	2243	rVB3	419	459	0.03%	0.004%
54	8.636	2256	2269	2301	rBV	430327	800676	57.19%	7.319%
55	9.163	2430	2433	2437	rBV	561	518	0.04%	0.005%
56	9.234	2451	2455	2458	rVB3	393	333	0.02%	0.003%
57	9.263	2458	2464	2467	rVB2	319	285	0.02%	0.003%
58	9.295	2472	2474	2481	rVB3	295	285	0.02%	0.003%
59	9.340	2484	2488	2491	rBV3	352	267	0.02%	0.002%
60	9.417	2499	2512	2551	rBV2	612131	1192165	85.15%	10.897%
61	9.639	2578	2581	2592	rVB3	682	875	0.06%	0.008%
62	9.697	2592	2599	2606	rBV3	1276	1891	0.14%	0.017%
63	9.906	2662	2664	2670	rBV2	321	339	0.02%	0.003%
64	9.973	2680	2685	2689	rBV2	305	318	0.02%	0.003%
65	10.095	2721	2723	2725	rVV2	446	263	0.02%	0.002%
66	10.115	2727	2729	2732	rVB2	451	257	0.02%	0.002%
67	10.401	2815	2818	2821	rBV2	379	310	0.02%	0.003%
68	10.478	2836	2842	2851	rVB4	574	1105	0.08%	0.010%
69	10.562	2864	2868	2873	rBV2	303	246	0.02%	0.002%
70	10.590	2873	2877	2880	rBV2	556	532	0.04%	0.005%
71	10.674	2896	2903	2910	rBV4	2187	3142	0.22%	0.029%
72	10.758	2916	2929	2949	rBV	450311	736499	52.61%	6.732%
73	10.896	2959	2972	2979	rBV2	5233	9122	0.65%	0.083%
74	10.967	2990	2994	2996	rBV2	285	255	0.02%	0.002%
75	11.005	3002	3006	3011	rVB2	485	509	0.04%	0.005%
76	11.070	3022	3026	3030	rVV2	393	448	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047977.D
 Acq On : 12 Apr 2022 23:38
 Operator : SY/MD
 Sample : N2345-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.092	3030	3033	3039	rVB3	370	358	0.03%	0.003%
78	11.201	3062	3067	3071	rBV2	272	269	0.02%	0.002%
79	11.253	3076	3083	3092	rBV2	739	1195	0.09%	0.011%
80	11.459	3140	3147	3159	rVB7	1669	3090	0.22%	0.028%
81	11.574	3180	3183	3185	rBV2	502	360	0.03%	0.003%
82	11.700	3217	3222	3227	rVB4	767	788	0.06%	0.007%
83	11.745	3230	3236	3240	rBV3	915	1165	0.08%	0.011%
84	11.812	3244	3257	3281	rBV	660038	1099804	78.56%	10.053%
85	11.922	3288	3291	3293	rBV4	471	255	0.02%	0.002%
86	11.944	3295	3298	3300	rBV2	643	364	0.03%	0.003%
87	12.066	3326	3336	3346	rBV3	10606	18936	1.35%	0.173%
88	12.147	3359	3361	3363	rBV4	542	338	0.02%	0.003%
89	12.195	3363	3376	3395	rVB	623057	1024835	73.20%	9.368%
90	12.491	3464	3468	3471	rBV2	343	336	0.02%	0.003%
91	12.770	3549	3555	3557	rBV4	879	923	0.07%	0.008%
92	12.976	3614	3619	3626	rVB5	1253	1357	0.10%	0.012%
93	13.224	3692	3696	3700	rBV3	677	597	0.04%	0.005%
94	13.378	3738	3744	3748	rBV5	1220	1293	0.09%	0.012%
95	13.848	3884	3890	3896	rVB3	1201	1600	0.11%	0.015%
96	14.085	3961	3964	3965	rBV	461	274	0.02%	0.003%
97	14.359	4047	4049	4055	rVB4	828	639	0.05%	0.006%
98	14.757	4170	4173	4174	rBV2	588	321	0.02%	0.003%
99	15.159	4296	4298	4300	rBV2	505	338	0.02%	0.003%
100	15.545	4413	4418	4425	rBV6	2310	3038	0.22%	0.028%




Sum of corrected areas: 10940141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047977.D
Acq On : 12 Apr 2022 23:38
Operator : SY/MD
Sample : N2345-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

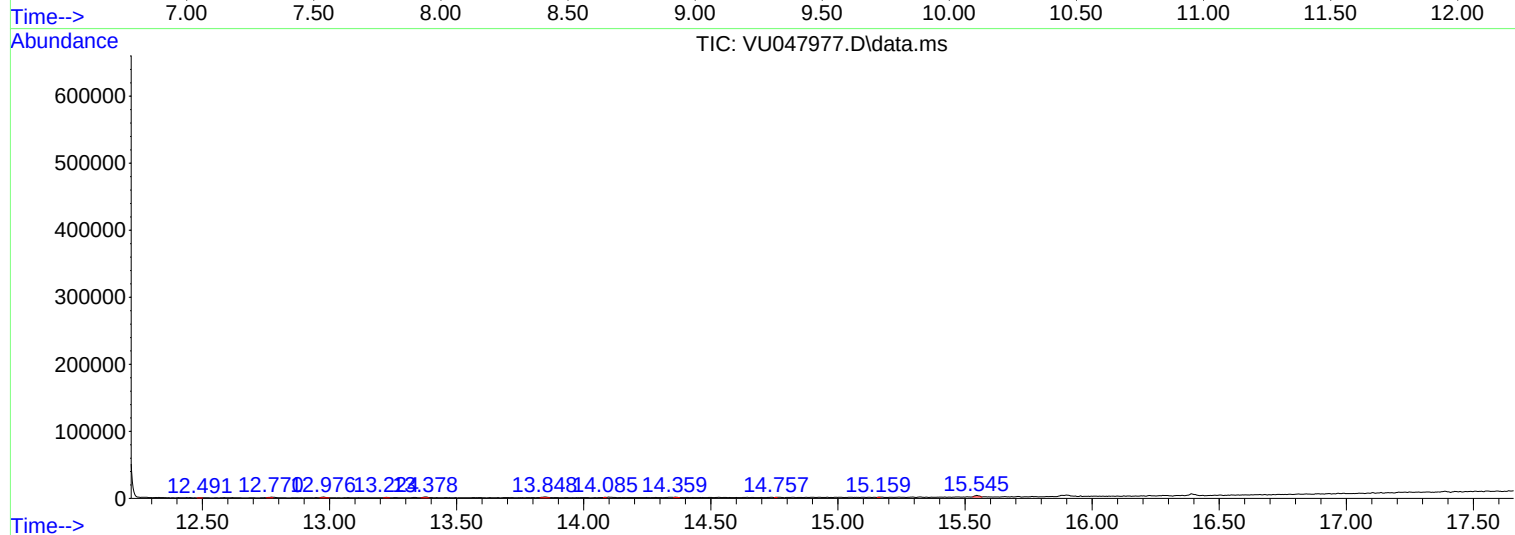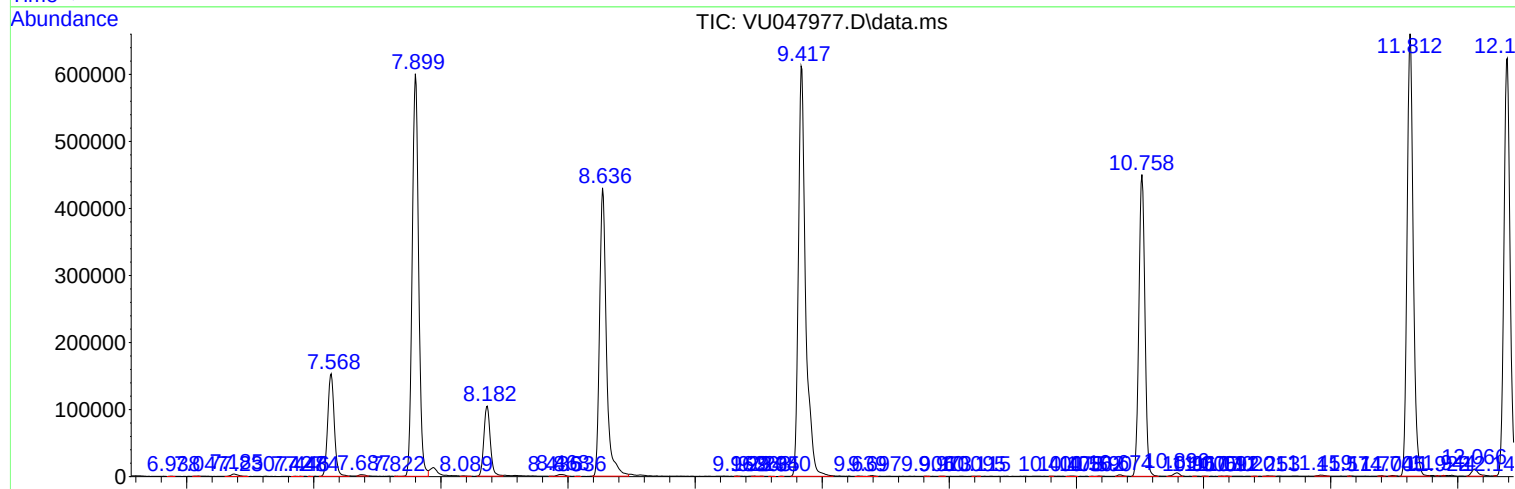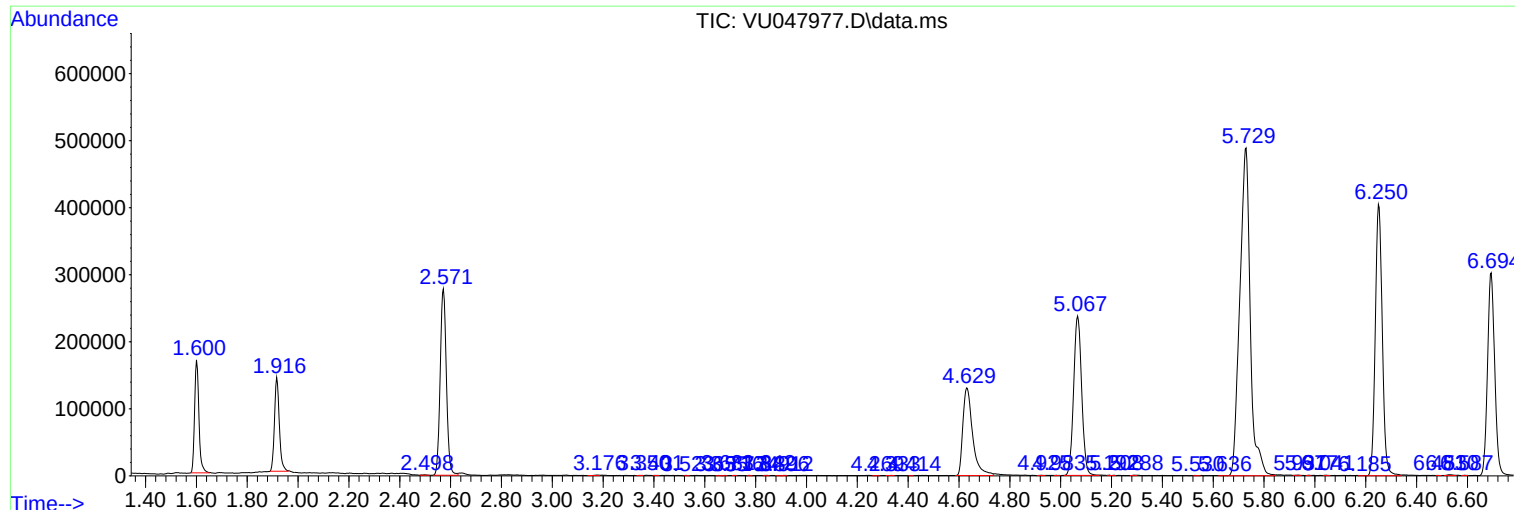

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047977.D
Acq On : 12 Apr 2022 23:38
Operator : SY/MD
Sample : N2345-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047977.D
Acq On : 12 Apr 2022 23:38
Operator : SY/MD
Sample : N2345-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc