

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047978.D
 Acq On : 13 Apr 2022 00:01
 Operator : SY/MD
 Sample : N2345-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	100	rVB	177239	206976	14.99%	1.919%
2	1.916	170	179	202	rVB	137152	192125	13.91%	1.781%
3	2.514	362	365	369	rBV3	353	238	0.02%	0.002%
4	2.572	370	383	396	rBV	286926	469289	33.98%	4.350%
5	2.707	423	425	429	rVB4	347	253	0.02%	0.002%
6	2.803	453	455	458	rVB	527	331	0.02%	0.003%
7	2.928	490	494	497	rBV2	324	261	0.02%	0.002%
8	2.977	507	509	513	rVB2	524	377	0.03%	0.003%
9	2.999	513	516	520	rVB2	337	248	0.02%	0.002%
10	3.044	527	530	532	rBV	386	291	0.02%	0.003%
11	3.192	561	576	586	rBV2	2483	5754	0.42%	0.053%
12	3.308	607	612	616	rVB2	379	405	0.03%	0.004%
13	3.359	625	628	629	rVV2	376	262	0.02%	0.002%
14	3.372	629	632	642	rVB4	762	912	0.07%	0.008%
15	3.652	714	719	721	rBV2	257	278	0.02%	0.003%
16	3.893	791	794	798	rVB2	400	296	0.02%	0.003%
17	3.928	801	805	813	rVB3	402	476	0.03%	0.004%
18	4.044	838	841	847	rVB2	422	456	0.03%	0.004%
19	4.080	847	852	855	rBV2	234	257	0.02%	0.002%
20	4.314	916	925	928	rBV2	259	375	0.03%	0.003%
21	4.411	950	955	960	rVB	379	331	0.02%	0.003%
22	4.620	1007	1020	1046	rBV	138852	336934	24.40%	3.123%
23	5.067	1142	1159	1190	rBV	241151	527177	38.18%	4.887%
24	5.285	1223	1227	1232	rBV4	528	632	0.05%	0.006%
25	5.436	1271	1274	1277	rVB	386	212	0.02%	0.002%
26	5.459	1277	1281	1283	rBV2	273	212	0.02%	0.002%
27	5.475	1283	1286	1291	rVV2	294	247	0.02%	0.002%
28	5.729	1343	1365	1395	rBV2	494929	1380879	100.00%	12.800%
29	6.041	1458	1462	1466	rVB2	419	342	0.02%	0.003%
30	6.102	1476	1481	1483	rBV3	264	222	0.02%	0.002%
31	6.118	1483	1486	1490	rVB	385	286	0.02%	0.003%
32	6.137	1490	1492	1497	rBV3	307	244	0.02%	0.002%
33	6.250	1511	1527	1551	rBV	404208	765971	55.47%	7.100%
34	6.533	1607	1615	1622	rVV4	1236	2187	0.16%	0.020%
35	6.575	1625	1628	1630	rVB2	552	289	0.02%	0.003%
36	6.636	1644	1647	1649	rBV	376	215	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047978.D
 Acq On : 13 Apr 2022 00:01
 Operator : SY/MD
 Sample : N2345-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1690	rBV	308227	602060	43.60%	5.581%
38	6.806	1696	1700	1707	rVB3	1292	1681	0.12%	0.016%
39	6.877	1717	1722	1724	rBV3	413	387	0.03%	0.004%
40	7.012	1759	1764	1769	rVB3	276	231	0.02%	0.002%
41	7.047	1769	1775	1781	rVB3	467	520	0.04%	0.005%
42	7.083	1781	1786	1790	rVB3	472	404	0.03%	0.004%
43	7.182	1806	1817	1828	rBV3	3826	7070	0.51%	0.066%
44	7.404	1882	1886	1889	rBV2	346	303	0.02%	0.003%
45	7.459	1901	1903	1907	rBV2	326	243	0.02%	0.002%
46	7.510	1912	1919	1922	rBV3	289	332	0.02%	0.003%
47	7.568	1924	1937	1957	rBV	154697	272686	19.75%	2.528%
48	7.687	1966	1974	1984	rBV6	2508	4502	0.33%	0.042%
49	7.768	1995	1999	2003	rBV2	418	350	0.03%	0.003%
50	7.796	2003	2008	2012	rBV3	620	486	0.04%	0.005%
51	7.899	2025	2040	2056	rBV	608166	1057154	76.56%	9.800%
52	8.179	2116	2127	2146	rVV	106846	184842	13.39%	1.713%
53	8.433	2203	2206	2208	rBV2	389	282	0.02%	0.003%
54	8.475	2212	2219	2229	rVB3	1831	2961	0.21%	0.027%
55	8.513	2229	2231	2238	rVB3	567	503	0.04%	0.005%
56	8.575	2246	2250	2255	rVB2	297	275	0.02%	0.003%
57	8.632	2255	2268	2307	rBV	406168	779687	56.46%	7.228%
58	8.909	2351	2354	2357	rBV3	339	226	0.02%	0.002%
59	9.272	2464	2467	2471	rBV2	253	221	0.02%	0.002%
60	9.320	2479	2482	2487	rVB	278	252	0.02%	0.002%
61	9.353	2487	2492	2497	rVB3	562	484	0.04%	0.004%
62	9.417	2497	2512	2553	rBV	604056	1109217	80.33%	10.282%
63	9.565	2554	2558	2561	rBV4	514	371	0.03%	0.003%
64	9.648	2581	2584	2588	rVB3	459	327	0.02%	0.003%
65	9.693	2592	2598	2606	rBV2	1314	1761	0.13%	0.016%
66	9.925	2667	2670	2674	rBV	327	211	0.02%	0.002%
67	10.182	2747	2750	2755	rBV2	319	240	0.02%	0.002%
68	10.472	2837	2840	2842	rBV	342	225	0.02%	0.002%
69	10.619	2881	2886	2889	rVB3	319	314	0.02%	0.003%
70	10.668	2896	2901	2903	rBV4	1732	1694	0.12%	0.016%
71	10.758	2915	2929	2953	rBV	463966	745150	53.96%	6.907%
72	10.896	2961	2972	2983	rBV	3556	6166	0.45%	0.057%
73	11.005	3003	3006	3009	rVV3	372	234	0.02%	0.002%
74	11.121	3036	3042	3045	rBV2	445	513	0.04%	0.005%
75	11.198	3064	3066	3070	rVB	312	227	0.02%	0.002%
76	11.388	3119	3125	3127	rBV2	318	339	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047978.D
 Acq On : 13 Apr 2022 00:01
 Operator : SY/MD
 Sample : N2345-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.462	3139	3148	3150	rBV4	1425	1952	0.14%	0.018%
78	11.697	3217	3221	3225	rBV2	641	644	0.05%	0.006%
79	11.812	3244	3257	3277	rBV	653025	1061471	76.87%	9.840%
80	11.970	3302	3306	3307	rBV2	798	583	0.04%	0.005%
81	12.073	3329	3338	3353	rBV5	2723	5349	0.39%	0.050%
82	12.195	3361	3376	3393	rBV	620297	1026106	74.31%	9.512%
83	12.410	3440	3443	3446	rBV3	397	342	0.02%	0.003%
84	12.459	3454	3458	3461	rBV2	417	371	0.03%	0.003%
85	12.616	3503	3507	3510	rBV	384	323	0.02%	0.003%
86	12.771	3550	3555	3556	rBV2	666	529	0.04%	0.005%
87	12.819	3566	3570	3574	rBV2	436	402	0.03%	0.004%
88	12.854	3578	3581	3586	rVB	332	298	0.02%	0.003%
89	12.934	3603	3606	3613	rBV3	414	560	0.04%	0.005%
90	12.970	3613	3617	3621	rBV4	781	873	0.06%	0.008%
91	13.156	3670	3675	3677	rBV2	429	444	0.03%	0.004%
92	13.227	3695	3697	3703	rVB4	331	226	0.02%	0.002%
93	13.381	3740	3745	3751	rVB5	996	995	0.07%	0.009%
94	14.024	3942	3945	3947	rBV3	498	298	0.02%	0.003%
95	14.333	4038	4041	4044	rBV4	386	339	0.02%	0.003%
96	14.796	4181	4185	4188	rBV	629	469	0.03%	0.004%
97	14.851	4200	4202	4206	rVB2	725	310	0.02%	0.003%
98	15.330	4349	4351	4353	rBV2	546	254	0.02%	0.002%
99	15.549	4415	4419	4428	rVB7	2196	2720	0.20%	0.025%
100	16.053	4574	4576	4577	rBV	992	490	0.04%	0.005%




Sum of corrected areas: 10787719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047978.D
Acq On : 13 Apr 2022 00:01
Operator : SY/MD
Sample : N2345-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

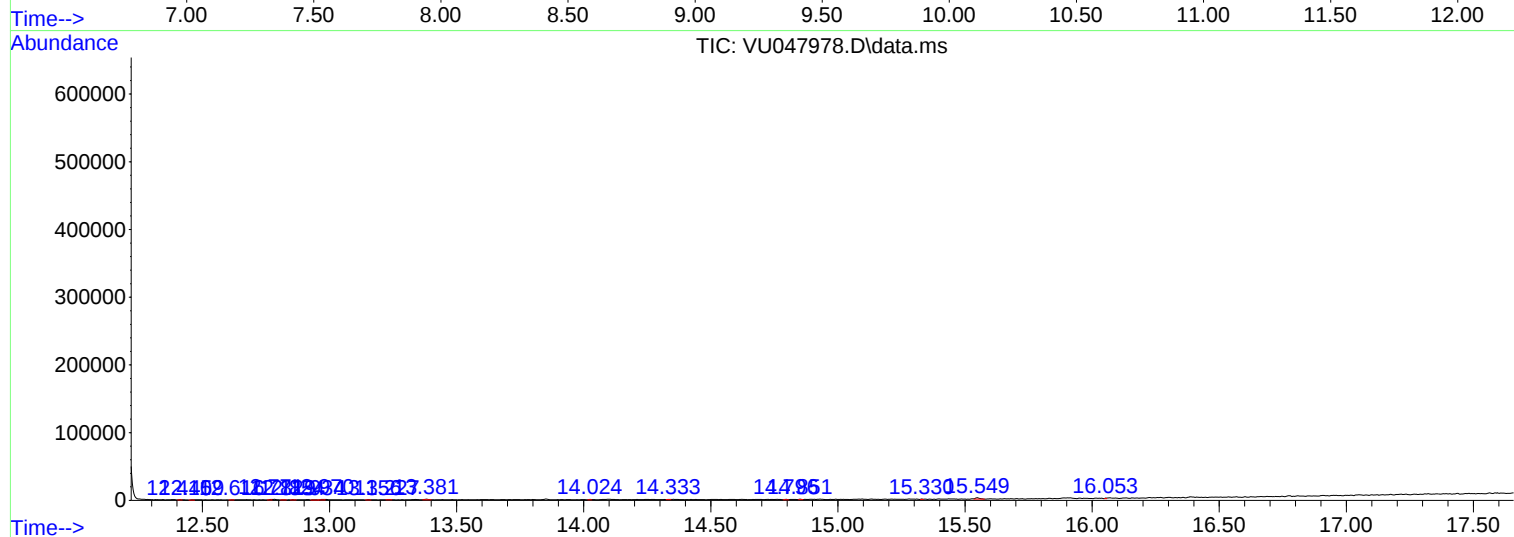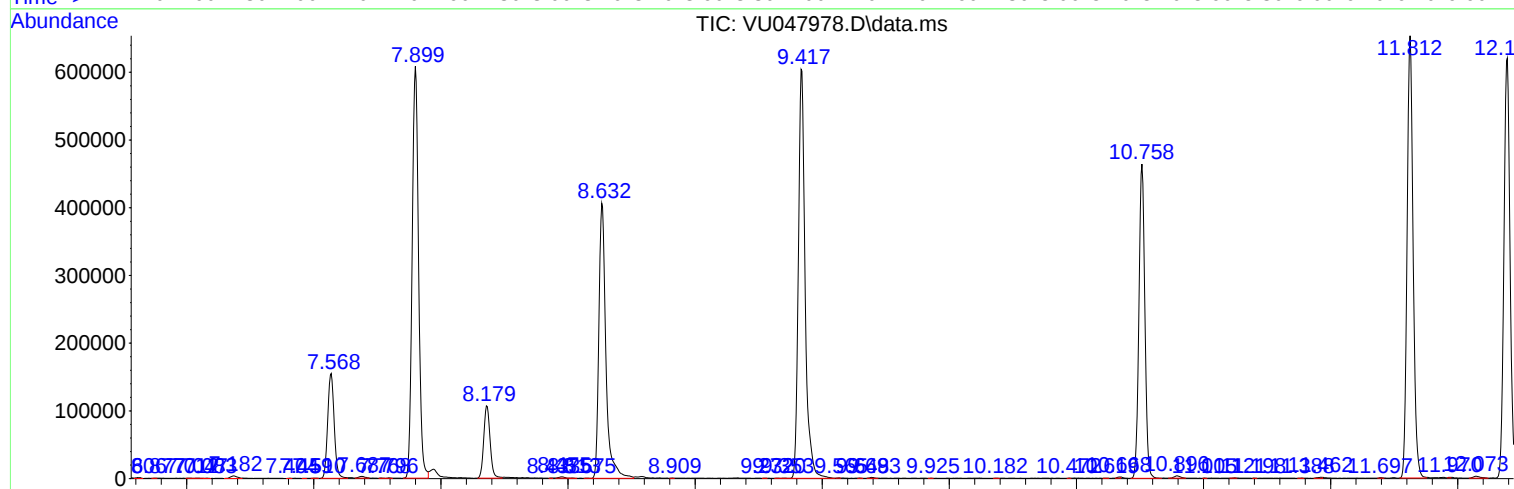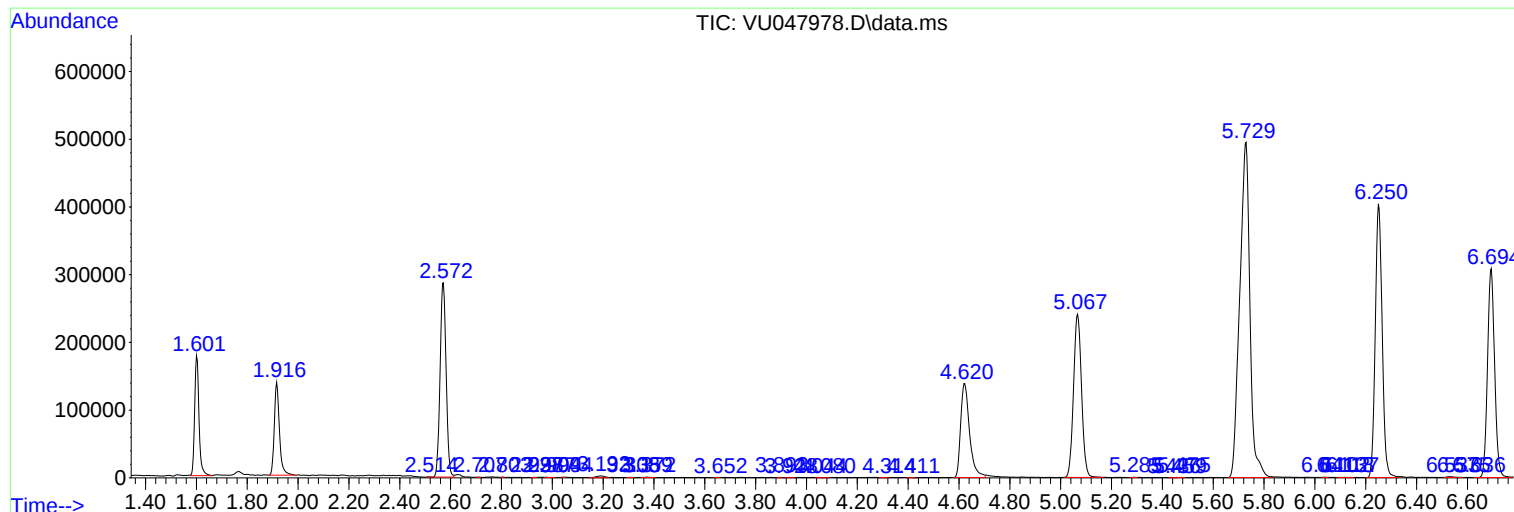

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047978.D
Acq On : 13 Apr 2022 00:01
Operator : SY/MD
Sample : N2345-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047978.D
Acq On : 13 Apr 2022 00:01
Operator : SY/MD
Sample : N2345-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc