

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047979.D
 Acq On : 13 Apr 2022 00:24
 Operator : SY/MD
 Sample : N2345-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047979.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	99	rBV	176510	202134	14.77%	1.883%
2	1.916	170	179	200	rBV	135974	189674	13.86%	1.767%
3	2.571	370	383	396	rBV	287587	472785	34.54%	4.405%
4	2.684	414	418	421	rBV	456	378	0.03%	0.004%
5	2.906	483	487	489	rBV2	330	290	0.02%	0.003%
6	3.002	514	517	521	rBV2	325	252	0.02%	0.002%
7	3.051	525	532	539	rBV5	644	1030	0.08%	0.010%
8	3.182	564	573	575	rBV3	2953	3921	0.29%	0.037%
9	3.314	610	614	619	rVB4	338	345	0.03%	0.003%
10	3.356	623	627	631	rVB2	513	450	0.03%	0.004%
11	3.395	635	639	644	rVV3	277	295	0.02%	0.003%
12	3.504	668	673	675	rVV2	206	199	0.01%	0.002%
13	3.661	719	722	725	rBV2	294	214	0.02%	0.002%
14	3.700	731	734	739	rVB2	255	233	0.02%	0.002%
15	3.726	739	742	747	rVB2	369	300	0.02%	0.003%
16	3.761	747	753	755	rVB	359	273	0.02%	0.003%
17	3.816	767	770	773	rBV2	260	225	0.02%	0.002%
18	3.848	777	780	785	rVB3	271	239	0.02%	0.002%
19	4.121	863	865	868	rVB2	351	199	0.01%	0.002%
20	4.144	868	872	876	rBV2	332	297	0.02%	0.003%
21	4.182	878	884	887	rBV2	232	225	0.02%	0.002%
22	4.224	891	897	899	rBV2	293	263	0.02%	0.002%
23	4.321	922	927	929	rBV2	257	213	0.02%	0.002%
24	4.620	1007	1020	1054	rBV	142516	347281	25.37%	3.235%
25	5.009	1137	1141	1142	rBV2	345	211	0.02%	0.002%
26	5.067	1142	1159	1180	rVV2	240472	524913	38.34%	4.890%
27	5.259	1215	1219	1223	rVB2	301	274	0.02%	0.003%
28	5.292	1223	1229	1231	rBV3	695	752	0.05%	0.007%
29	5.340	1240	1244	1247	rBV	341	288	0.02%	0.003%
30	5.562	1310	1313	1316	rBV	370	316	0.02%	0.003%
31	5.632	1327	1335	1338	rBV2	235	216	0.02%	0.002%
32	5.726	1343	1364	1397	rBV2	494368	1368949	100.00%	12.754%
33	6.092	1474	1478	1479	rBV	297	207	0.02%	0.002%
34	6.150	1491	1496	1498	rBV2	340	371	0.03%	0.003%
35	6.250	1509	1527	1547	rBV	390269	753159	55.02%	7.017%
36	6.484	1597	1600	1605	rBV2	308	278	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047979.D
 Acq On : 13 Apr 2022 00:24
 Operator : SY/MD
 Sample : N2345-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.529	1609	1614	1622	rBV4	1539	2554	0.19%	0.024%
38	6.632	1641	1646	1650	rBV2	157	206	0.02%	0.002%
39	6.693	1650	1665	1694	rBV	307304	603320	44.07%	5.621%
40	6.809	1696	1701	1707	rVV4	1012	1424	0.10%	0.013%
41	6.854	1711	1715	1718	rVB2	458	348	0.03%	0.003%
42	6.886	1723	1725	1728	rVB	385	218	0.02%	0.002%
43	7.028	1766	1769	1770	rBV	372	231	0.02%	0.002%
44	7.044	1772	1774	1778	rVV2	421	372	0.03%	0.003%
45	7.066	1778	1781	1784	rVV2	351	272	0.02%	0.003%
46	7.150	1803	1807	1809	rBV2	299	236	0.02%	0.002%
47	7.182	1809	1817	1831	rVV4	3748	6930	0.51%	0.065%
48	7.240	1831	1835	1838	rVB2	387	269	0.02%	0.003%
49	7.279	1844	1847	1850	rBV	300	209	0.02%	0.002%
50	7.504	1914	1917	1922	rVB3	269	238	0.02%	0.002%
51	7.568	1922	1937	1958	rBV	154286	273896	20.01%	2.552%
52	7.687	1969	1974	1989	rVB3	2710	4927	0.36%	0.046%
53	7.790	2001	2006	2009	rBV3	299	238	0.02%	0.002%
54	7.899	2025	2040	2056	rBV	608497	1059365	77.39%	9.869%
55	8.179	2116	2127	2143	rBV	107824	183596	13.41%	1.710%
56	8.394	2193	2194	2198	rVB	412	228	0.02%	0.002%
57	8.472	2212	2218	2231	rVB3	1726	3049	0.22%	0.028%
58	8.552	2237	2243	2251	rBV7	2995	4751	0.35%	0.044%
59	8.632	2256	2268	2307	rBV	408403	784719	57.32%	7.311%
60	8.841	2331	2333	2340	rVB3	555	293	0.02%	0.003%
61	8.877	2340	2344	2346	rVV2	395	279	0.02%	0.003%
62	8.906	2350	2353	2357	rVB2	511	449	0.03%	0.004%
63	8.928	2357	2360	2367	rBV3	455	638	0.05%	0.006%
64	8.986	2376	2378	2382	rVB	371	220	0.02%	0.002%
65	9.111	2412	2417	2423	rVV3	361	532	0.04%	0.005%
66	9.288	2468	2472	2475	rBV3	249	196	0.01%	0.002%
67	9.420	2499	2513	2547	rVV	597742	1064051	77.73%	9.913%
68	9.645	2580	2583	2588	rVB3	403	392	0.03%	0.004%
69	9.693	2591	2598	2605	rBV2	945	1472	0.11%	0.014%
70	9.812	2632	2635	2639	rBV2	274	211	0.02%	0.002%
71	9.979	2681	2687	2689	rBV	338	292	0.02%	0.003%
72	10.253	2768	2772	2777	rBV3	276	341	0.02%	0.003%
73	10.491	2842	2846	2851	rVB2	549	466	0.03%	0.004%
74	10.594	2875	2878	2882	rBV	447	341	0.02%	0.003%
75	10.616	2882	2885	2889	rVV2	460	386	0.03%	0.004%
76	10.642	2889	2893	2896	rVV3	348	331	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047979.D
 Acq On : 13 Apr 2022 00:24
 Operator : SY/MD
 Sample : N2345-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.668	2896	2901	2911	rVB6	1697	2661	0.19%	0.025%
78	10.758	2916	2929	2949	rBV	458849	745592	54.46%	6.946%
79	10.864	2959	2962	2965	rBV3	757	594	0.04%	0.006%
80	10.896	2966	2972	2983	rVB4	2584	3887	0.28%	0.036%
81	11.336	3106	3109	3112	rVB2	263	199	0.01%	0.002%
82	11.455	3143	3146	3148	rBV2	943	668	0.05%	0.006%
83	11.532	3167	3170	3175	rBV	269	207	0.02%	0.002%
84	11.574	3179	3183	3185	rVB2	303	230	0.02%	0.002%
85	11.693	3218	3220	3229	rVB4	651	563	0.04%	0.005%
86	11.751	3232	3238	3243	rVB4	902	1101	0.08%	0.010%
87	11.812	3244	3257	3277	rBV	642646	1047949	76.55%	9.763%
88	11.944	3296	3298	3302	rVB4	602	335	0.02%	0.003%
89	11.970	3302	3306	3307	rBV3	767	555	0.04%	0.005%
90	12.069	3328	3337	3348	rBV4	6175	11866	0.87%	0.111%
91	12.195	3362	3376	3397	rBV	634830	1035472	75.64%	9.647%
92	12.494	3464	3469	3472	rBV2	458	467	0.03%	0.004%
93	12.526	3476	3479	3482	rVV2	329	287	0.02%	0.003%
94	12.889	3589	3592	3595	rBV	285	225	0.02%	0.002%
95	12.973	3615	3618	3626	rVB4	775	781	0.06%	0.007%
96	13.227	3694	3697	3701	rBV2	511	328	0.02%	0.003%
97	13.330	3726	3729	3733	rBV3	556	442	0.03%	0.004%
98	13.378	3741	3744	3751	rBV5	960	1151	0.08%	0.011%
99	13.848	3884	3890	3898	rVB5	2512	3759	0.27%	0.035%
100	14.327	4036	4039	4041	rBV2	574	409	0.03%	0.004%




Sum of corrected areas: 10733863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047979.D
Acq On : 13 Apr 2022 00:24
Operator : SY/MD
Sample : N2345-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

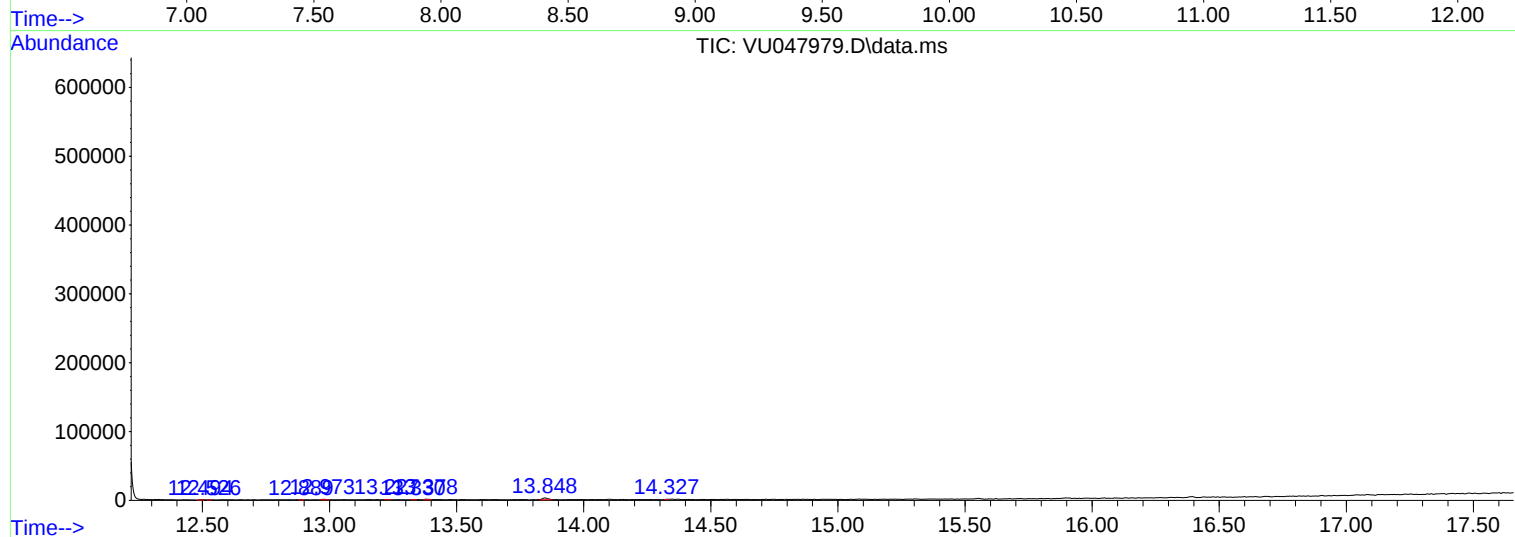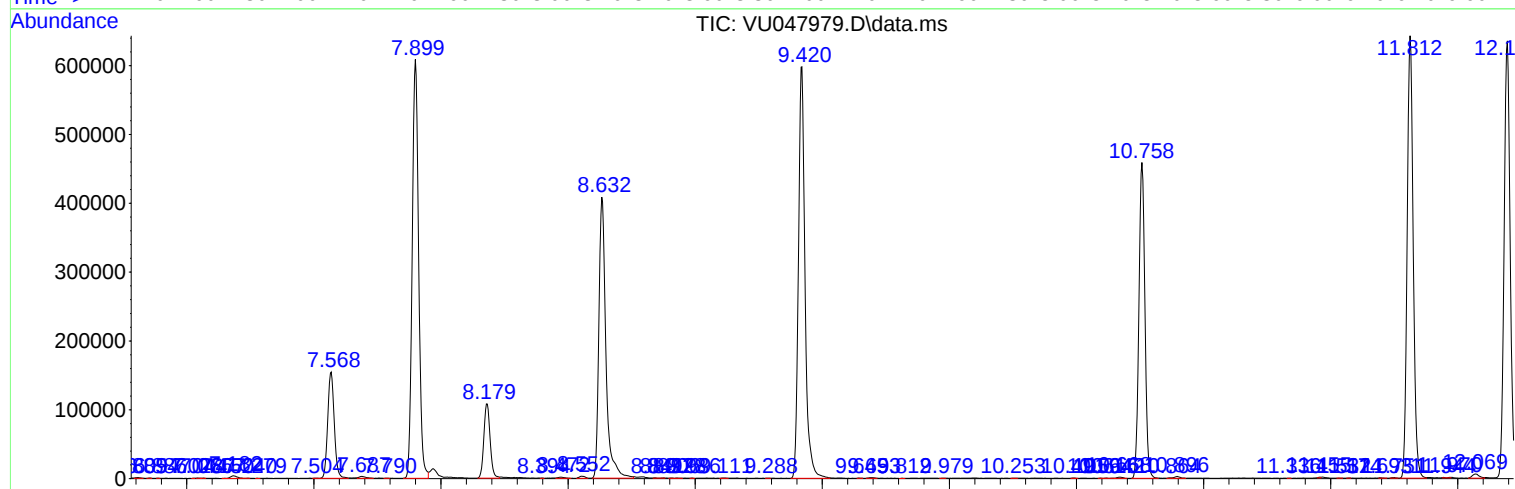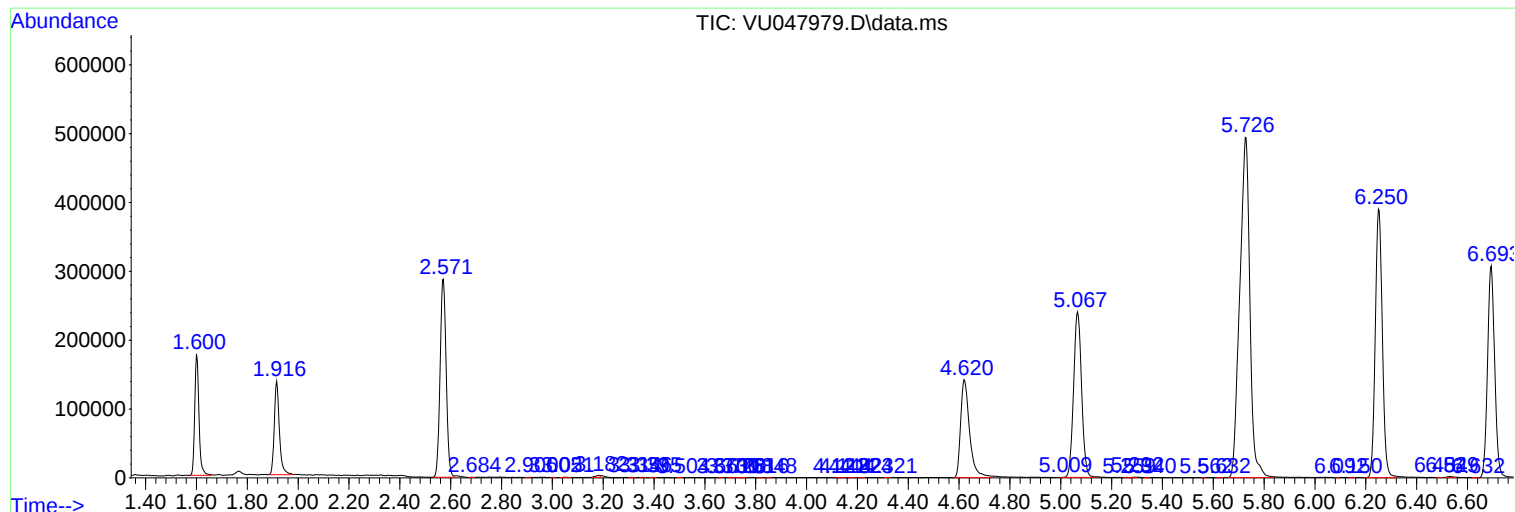

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047979.D
Acq On : 13 Apr 2022 00:24
Operator : SY/MD
Sample : N2345-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047979.D
Acq On : 13 Apr 2022 00:24
Operator : SY/MD
Sample : N2345-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------