

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047980.D
 Acq On : 13 Apr 2022 00:47
 Operator : SY/MD
 Sample : N2345-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rBV	166481	190140	14.63%	1.829%
2	1.916	170	179	199	rBV	131123	181220	13.95%	1.743%
3	2.568	370	382	398	rBV	273944	449801	34.62%	4.326%
4	2.761	438	442	445	rBV4	414	312	0.02%	0.003%
5	2.787	448	450	453	rBV2	268	199	0.02%	0.002%
6	2.848	466	469	473	rBV3	264	289	0.02%	0.003%
7	2.951	498	501	503	rBV3	378	260	0.02%	0.003%
8	3.044	525	530	534	rVV4	692	825	0.06%	0.008%
9	3.118	550	553	558	rVB3	326	219	0.02%	0.002%
10	3.189	562	575	586	rBV3	1993	4682	0.36%	0.045%
11	3.269	597	600	605	rBV2	304	313	0.02%	0.003%
12	3.295	605	608	612	rVB2	338	287	0.02%	0.003%
13	3.321	612	616	618	rBV	332	285	0.02%	0.003%
14	3.549	683	687	691	rBV2	244	271	0.02%	0.003%
15	3.626	706	711	717	rVB3	361	489	0.04%	0.005%
16	3.671	723	725	728	rVB3	333	211	0.02%	0.002%
17	4.076	846	851	854	rBV2	190	209	0.02%	0.002%
18	4.234	896	900	904	rBV2	327	229	0.02%	0.002%
19	4.279	909	914	918	rBV2	377	421	0.03%	0.004%
20	4.346	933	935	940	rVB3	234	199	0.02%	0.002%
21	4.436	961	963	967	rVB2	349	243	0.02%	0.002%
22	4.472	972	974	981	rBV2	191	228	0.02%	0.002%
23	4.620	1007	1020	1053	rBV	133181	323391	24.89%	3.110%
24	5.067	1142	1159	1185	rBV	230886	504059	38.80%	4.848%
25	5.298	1224	1231	1238	rVB5	935	1343	0.10%	0.013%
26	5.334	1238	1242	1245	rBV2	471	426	0.03%	0.004%
27	5.375	1251	1255	1257	rBV2	528	328	0.03%	0.003%
28	5.424	1265	1270	1275	rBV2	386	314	0.02%	0.003%
29	5.459	1277	1281	1287	rVV	328	430	0.03%	0.004%
30	5.536	1303	1305	1310	rVB2	327	249	0.02%	0.002%
31	5.581	1315	1319	1322	rVB2	246	197	0.02%	0.002%
32	5.600	1322	1325	1327	rBV	382	235	0.02%	0.002%
33	5.639	1335	1337	1341	rBV2	276	239	0.02%	0.002%
34	5.729	1341	1365	1400	rVV2	467394	1299243	100.00%	12.496%
35	5.848	1400	1402	1405	rVV2	353	217	0.02%	0.002%
36	6.112	1480	1484	1488	rBV4	356	348	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047980.D
 Acq On : 13 Apr 2022 00:47
 Operator : SY/MD
 Sample : N2345-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1551	rBV	396367	750733	57.78%	7.221%
38	6.526	1608	1613	1622	rBV3	1028	1606	0.12%	0.015%
39	6.694	1650	1665	1684	rBV	293202	574891	44.25%	5.529%
40	6.803	1697	1699	1705	rVB3	744	581	0.04%	0.006%
41	7.044	1769	1774	1776	rBV	336	371	0.03%	0.004%
42	7.063	1778	1780	1785	rVV	563	290	0.02%	0.003%
43	7.182	1810	1817	1831	rVB3	3607	6437	0.50%	0.062%
44	7.240	1831	1835	1839	rVB	338	222	0.02%	0.002%
45	7.488	1907	1912	1918	rVB2	204	219	0.02%	0.002%
46	7.568	1924	1937	1953	rBV	145131	257898	19.85%	2.480%
47	7.690	1966	1975	1983	rVB6	2557	4216	0.32%	0.041%
48	7.726	1983	1986	1991	rVB3	431	383	0.03%	0.004%
49	7.758	1991	1996	1999	rBV3	485	417	0.03%	0.004%
50	7.806	2004	2011	2013	rBV2	258	331	0.03%	0.003%
51	7.899	2025	2040	2056	rBV	578452	1006405	77.46%	9.680%
52	8.179	2115	2127	2147	rBV	102395	178295	13.72%	1.715%
53	8.427	2201	2204	2207	rBV	320	229	0.02%	0.002%
54	8.475	2210	2219	2228	rVB3	1953	3361	0.26%	0.032%
55	8.552	2240	2243	2246	rVB2	544	368	0.03%	0.004%
56	8.578	2246	2251	2256	rBV2	314	312	0.02%	0.003%
57	8.632	2256	2268	2297	rBV	398682	745361	57.37%	7.169%
58	8.845	2330	2334	2337	rBV4	455	385	0.03%	0.004%
59	8.983	2373	2377	2380	rVV3	424	383	0.03%	0.004%
60	9.153	2425	2430	2434	rBV2	290	315	0.02%	0.003%
61	9.266	2462	2465	2469	rVB2	383	200	0.02%	0.002%
62	9.417	2499	2512	2547	rBV	598394	1064234	81.91%	10.236%
63	9.565	2554	2558	2562	rBV3	481	369	0.03%	0.004%
64	9.652	2579	2585	2587	rVV3	248	267	0.02%	0.003%
65	9.693	2592	2598	2599	rBV3	915	773	0.06%	0.007%
66	9.771	2617	2622	2624	rVV3	219	234	0.02%	0.002%
67	9.867	2648	2652	2659	rVB3	416	488	0.04%	0.005%
68	9.935	2670	2673	2679	rVB2	359	344	0.03%	0.003%
69	10.028	2692	2702	2703	rBV2	268	352	0.03%	0.003%
70	10.105	2723	2726	2729	rVB	467	342	0.03%	0.003%
71	10.372	2805	2809	2813	rBV2	225	253	0.02%	0.002%
72	10.443	2827	2831	2833	rBV2	370	245	0.02%	0.002%
73	10.459	2833	2836	2838	rBV3	296	200	0.02%	0.002%
74	10.594	2873	2878	2880	rBV2	232	219	0.02%	0.002%
75	10.668	2895	2901	2909	rBV5	1813	2197	0.17%	0.021%
76	10.758	2915	2929	2954	rVB	438483	715098	55.04%	6.878%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047980.D
 Acq On : 13 Apr 2022 00:47
 Operator : SY/MD
 Sample : N2345-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.896	2962	2972	2986	rVB2	3094	5309	0.41%	0.051%
78	11.050	3015	3020	3023	rBV2	373	371	0.03%	0.004%
79	11.115	3038	3040	3043	rVV4	510	304	0.02%	0.003%
80	11.221	3071	3073	3077	rBV2	413	284	0.02%	0.003%
81	11.285	3090	3093	3097	rBV2	314	284	0.02%	0.003%
82	11.308	3098	3100	3109	rVB2	331	340	0.03%	0.003%
83	11.353	3109	3114	3115	rBV2	293	262	0.02%	0.003%
84	11.427	3133	3137	3140	rBV3	437	327	0.03%	0.003%
85	11.462	3140	3148	3151	rBV5	1332	1698	0.13%	0.016%
86	11.581	3182	3185	3187	rBV3	253	198	0.02%	0.002%
87	11.745	3230	3236	3244	rBV4	2214	3065	0.24%	0.029%
88	11.812	3244	3257	3283	rBV	650681	1089770	83.88%	10.482%
89	11.970	3304	3306	3314	rVB5	1139	1090	0.08%	0.010%
90	12.070	3329	3337	3349	rBV5	3793	7028	0.54%	0.068%
91	12.115	3349	3351	3358	rVB3	577	505	0.04%	0.005%
92	12.195	3358	3376	3402	rBV	602718	995563	76.63%	9.575%
93	12.285	3402	3404	3408	rBV2	547	311	0.02%	0.003%
94	12.336	3415	3420	3424	rBV2	563	586	0.05%	0.006%
95	12.381	3431	3434	3438	rBV	253	236	0.02%	0.002%
96	12.594	3496	3500	3504	rBV3	376	312	0.02%	0.003%
97	12.774	3552	3556	3558	rBV3	505	440	0.03%	0.004%
98	12.980	3614	3620	3625	rVB4	847	1007	0.08%	0.010%
99	13.163	3674	3677	3684	rVB4	523	424	0.03%	0.004%
100	13.844	3883	3889	3900	rVB3	3371	5147	0.40%	0.050%




Sum of corrected areas: 10397036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047980.D
Acq On : 13 Apr 2022 00:47
Operator : SY/MD
Sample : N2345-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

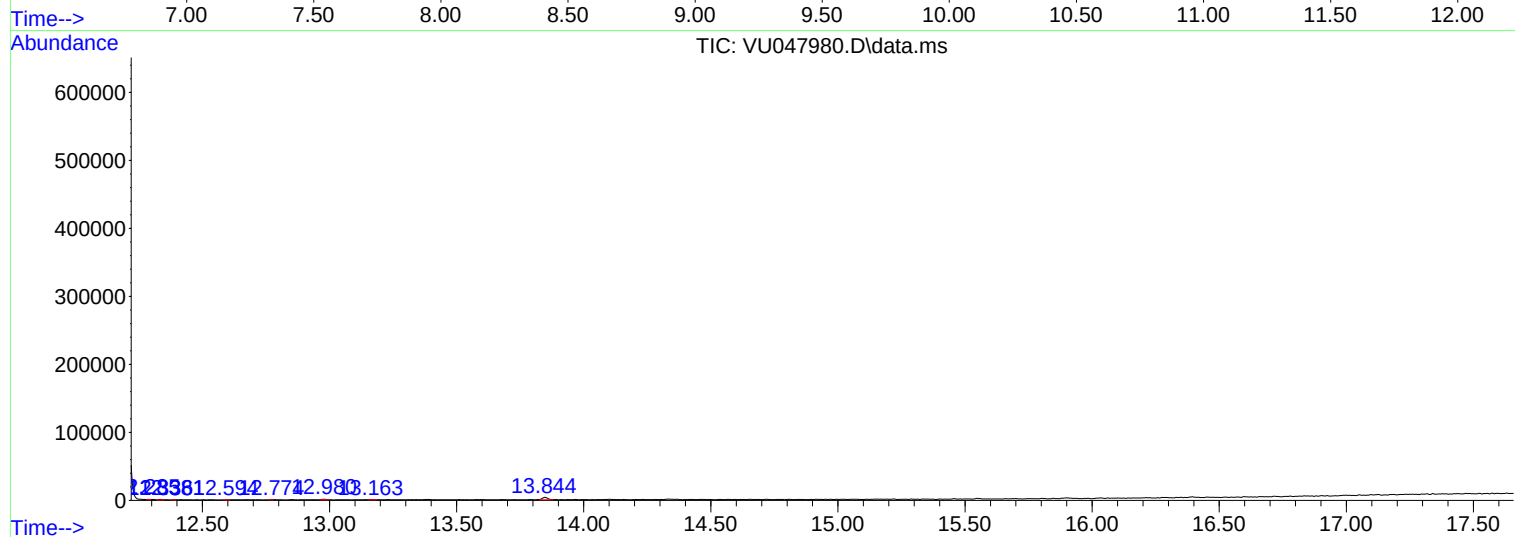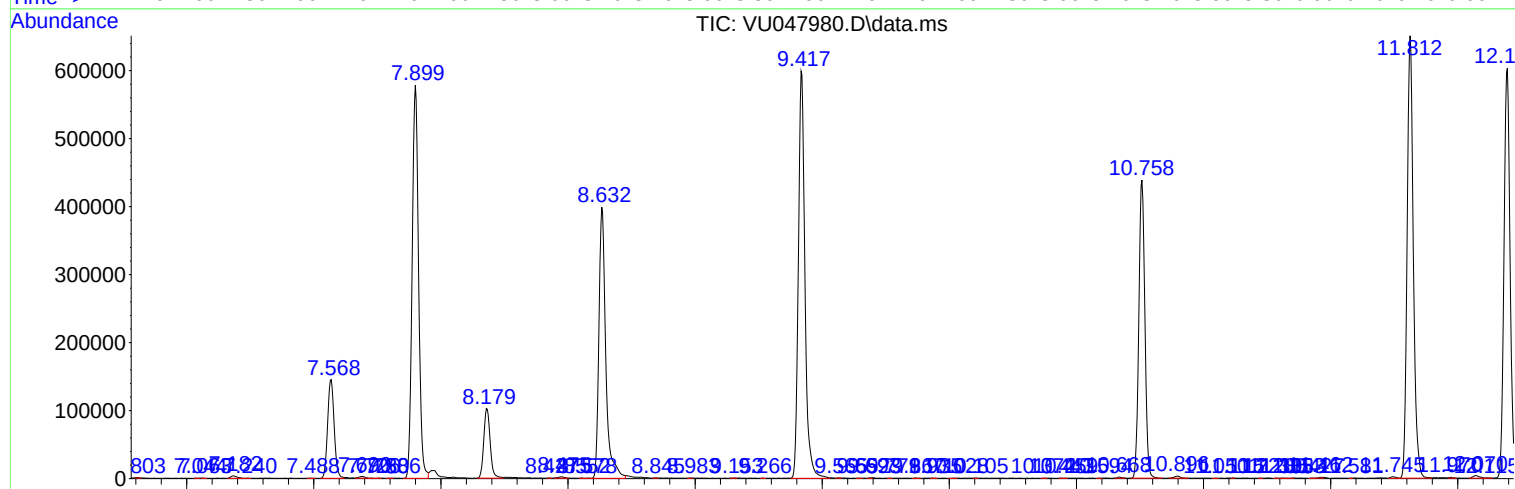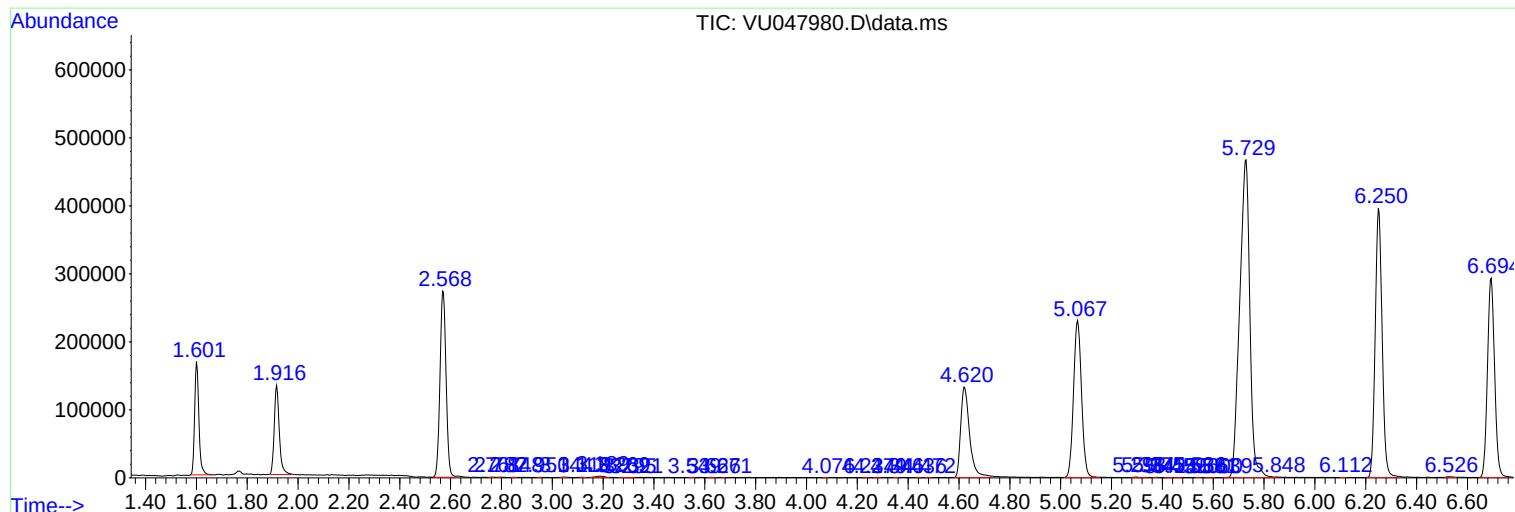

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047980.D
Acq On : 13 Apr 2022 00:47
Operator : SY/MD
Sample : N2345-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047980.D
Acq On : 13 Apr 2022 00:47
Operator : SY/MD
Sample : N2345-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc