

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047983.D
 Acq On : 13 Apr 2022 01:56
 Operator : SY/MD
 Sample : N2345-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	103	rVB	181841	212355	7.72%	1.555%
2	1.916	171	179	204	rVB	142379	198602	7.22%	1.454%
3	2.571	370	383	400	rBV	294708	481883	17.53%	3.529%
4	2.784	446	449	451	rBV3	509	308	0.01%	0.002%
5	3.051	525	532	541	rBV5	2284	4037	0.15%	0.030%
6	3.173	566	570	571	rBV3	524	339	0.01%	0.002%
7	3.182	571	573	576	rBV3	471	326	0.01%	0.002%
8	3.243	589	592	595	rBV3	310	232	0.01%	0.002%
9	3.430	644	650	652	rBV4	414	366	0.01%	0.003%
10	3.446	652	655	661	rVB2	315	350	0.01%	0.003%
11	3.546	683	686	688	rBV2	551	422	0.02%	0.003%
12	3.629	708	712	719	rBV3	322	432	0.02%	0.003%
13	3.790	757	762	764	rBV2	416	405	0.01%	0.003%
14	3.886	787	792	797	rBV3	282	296	0.01%	0.002%
15	3.993	816	825	829	rBV3	465	641	0.02%	0.005%
16	4.044	835	841	845	rVB4	211	249	0.01%	0.002%
17	4.067	845	848	851	rBV2	452	274	0.01%	0.002%
18	4.240	898	902	905	rBV3	306	306	0.01%	0.002%
19	4.327	926	929	930	rBV	404	250	0.01%	0.002%
20	4.340	930	933	940	rVV3	508	615	0.02%	0.005%
21	4.620	1006	1020	1052	rBV	145795	352108	12.81%	2.579%
22	5.067	1142	1159	1182	rVV	244650	538375	19.58%	3.943%
23	5.214	1199	1205	1210	rVB3	541	665	0.02%	0.005%
24	5.282	1221	1226	1227	rBV2	339	274	0.01%	0.002%
25	5.420	1266	1269	1274	rBV3	311	346	0.01%	0.003%
26	5.729	1343	1365	1373	rBV2	512003	1392815	50.65%	10.201%
27	6.250	1512	1527	1547	rBV	435391	825389	30.02%	6.045%
28	6.513	1605	1609	1610	rBV3	543	303	0.01%	0.002%
29	6.526	1610	1613	1614	rBV2	655	417	0.02%	0.003%
30	6.597	1631	1635	1637	rVV3	556	344	0.01%	0.003%
31	6.693	1650	1665	1687	rBV	315222	617238	22.45%	4.520%
32	6.800	1694	1698	1701	rBV3	542	590	0.02%	0.004%
33	6.854	1712	1715	1719	rVB2	349	232	0.01%	0.002%
34	6.947	1741	1744	1749	rVB3	317	296	0.01%	0.002%
35	6.983	1753	1755	1760	rVB3	258	227	0.01%	0.002%
36	7.018	1762	1766	1768	rBV3	257	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047983.D
 Acq On : 13 Apr 2022 01:56
 Operator : SY/MD
 Sample : N2345-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.182	1809	1817	1830	rVV3	4054	7015	0.26%	0.051%
38	7.234	1830	1833	1839	rVB2	471	354	0.01%	0.003%
39	7.459	1898	1903	1907	rVB3	314	307	0.01%	0.002%
40	7.565	1924	1936	1955	rBV	158618	283899	10.32%	2.079%
41	7.687	1967	1974	1983	rBV5	3068	4424	0.16%	0.032%
42	7.771	1994	2000	2003	rBV4	494	546	0.02%	0.004%
43	7.790	2003	2006	2009	rVB	368	230	0.01%	0.002%
44	7.899	2023	2040	2056	rBV	631115	1100772	40.03%	8.062%
45	8.182	2116	2128	2144	rBV	109750	190781	6.94%	1.397%
46	8.558	2242	2245	2250	rVB4	530	436	0.02%	0.003%
47	8.581	2250	2252	2256	rBV3	370	369	0.01%	0.003%
48	8.632	2256	2268	2309	rBV	426029	802804	29.20%	5.879%
49	8.944	2362	2365	2367	rBV3	354	233	0.01%	0.002%
50	8.970	2370	2373	2377	rBV	438	387	0.01%	0.003%
51	9.008	2381	2385	2387	rBV2	351	318	0.01%	0.002%
52	9.166	2431	2434	2437	rVB3	689	405	0.01%	0.003%
53	9.185	2437	2440	2444	rVB	385	309	0.01%	0.002%
54	9.208	2444	2447	2450	rBV2	389	339	0.01%	0.002%
55	9.304	2475	2477	2479	rVB2	662	279	0.01%	0.002%
56	9.320	2479	2482	2484	rBV	495	296	0.01%	0.002%
57	9.336	2484	2487	2491	rVB4	425	367	0.01%	0.003%
58	9.420	2498	2513	2514	rBV	680145	793292	28.85%	5.810%
59	9.639	2578	2581	2584	rBV2	547	381	0.01%	0.003%
60	9.816	2633	2636	2640	rVB2	611	424	0.02%	0.003%
61	9.838	2640	2643	2645	rBV5	488	345	0.01%	0.003%
62	9.976	2682	2686	2687	rBV2	477	323	0.01%	0.002%
63	10.041	2704	2706	2712	rVV3	425	360	0.01%	0.003%
64	10.098	2720	2724	2727	rBV3	801	632	0.02%	0.005%
65	10.179	2745	2749	2753	rVV4	360	268	0.01%	0.002%
66	10.234	2763	2766	2772	rVB2	665	612	0.02%	0.004%
67	10.298	2783	2786	2790	rVB2	429	258	0.01%	0.002%
68	10.362	2801	2806	2808	rBV3	447	356	0.01%	0.003%
69	10.632	2888	2890	2894	rBV	361	269	0.01%	0.002%
70	10.671	2894	2902	2909	rVV7	1899	2791	0.10%	0.020%
71	10.758	2916	2929	2949	rBV	464569	748541	27.22%	5.482%
72	10.893	2964	2971	2979	rBV4	1417	2197	0.08%	0.016%
73	10.922	2979	2980	2986	rVB4	513	249	0.01%	0.002%
74	10.951	2986	2989	2995	rVB3	368	324	0.01%	0.002%
75	11.008	3000	3007	3011	rBV4	494	606	0.02%	0.004%
76	11.118	3036	3041	3042	rBV2	463	329	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047983.D
 Acq On : 13 Apr 2022 01:56
 Operator : SY/MD
 Sample : N2345-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.160	3053	3054	3059	rVB	537	303	0.01%	0.002%
78	11.185	3059	3062	3064	rBV	475	323	0.01%	0.002%
79	11.468	3138	3150	3154	rBV7	1757	2879	0.10%	0.021%
80	11.571	3178	3182	3187	rBV5	572	625	0.02%	0.005%
81	11.635	3197	3202	3203	rBV2	373	305	0.01%	0.002%
82	11.684	3213	3217	3218	rBV3	881	615	0.02%	0.005%
83	11.748	3226	3237	3245	rBV2	37682	61463	2.24%	0.450%
84	11.835	3245	3264	3287	rVB2	1122291	2749644	100.00%	20.137%
85	12.076	3335	3339	3341	rBV4	701	653	0.02%	0.005%
86	12.198	3362	3377	3398	rBV2	784699	1894573	68.90%	13.875%
87	12.722	3537	3540	3543	rBV3	414	326	0.01%	0.002%
88	12.761	3549	3552	3555	rBV3	450	391	0.01%	0.003%
89	12.831	3571	3574	3580	rVB3	493	444	0.02%	0.003%
90	12.864	3580	3584	3585	rBV3	429	290	0.01%	0.002%
91	12.976	3610	3619	3627	rBV6	1933	3539	0.13%	0.026%
92	13.243	3699	3702	3710	rBV3	610	560	0.02%	0.004%
93	13.307	3720	3722	3725	rBV	311	235	0.01%	0.002%
94	13.330	3726	3729	3730	rBV3	560	322	0.01%	0.002%
95	13.381	3740	3745	3750	rVV5	934	1036	0.04%	0.008%
96	13.417	3753	3756	3761	rBV	338	234	0.01%	0.002%
97	13.706	3843	3846	3849	rVB2	387	230	0.01%	0.002%
98	13.841	3875	3888	3907	rBV	208254	331053	12.04%	2.425%
99	14.092	3963	3966	3970	rBV2	828	725	0.03%	0.005%
100	14.333	4031	4041	4054	rBV2	14939	23643	0.86%	0.173%




Sum of corrected areas: 13654372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047983.D
Acq On : 13 Apr 2022 01:56
Operator : SY/MD
Sample : N2345-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

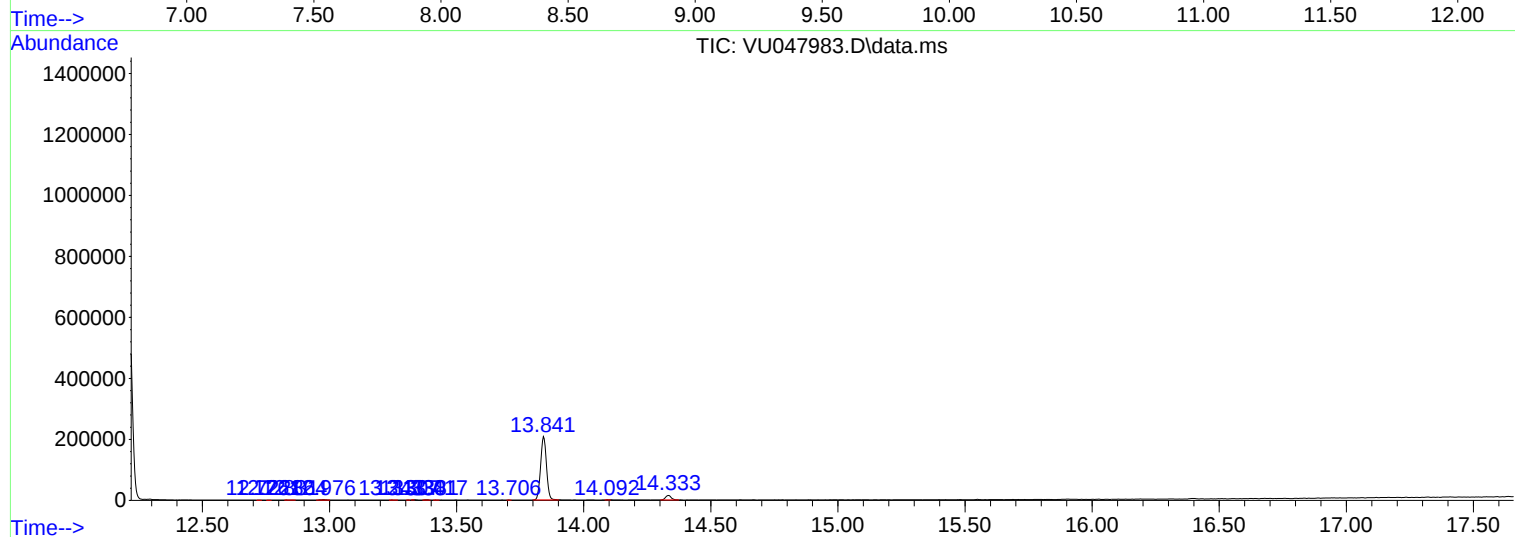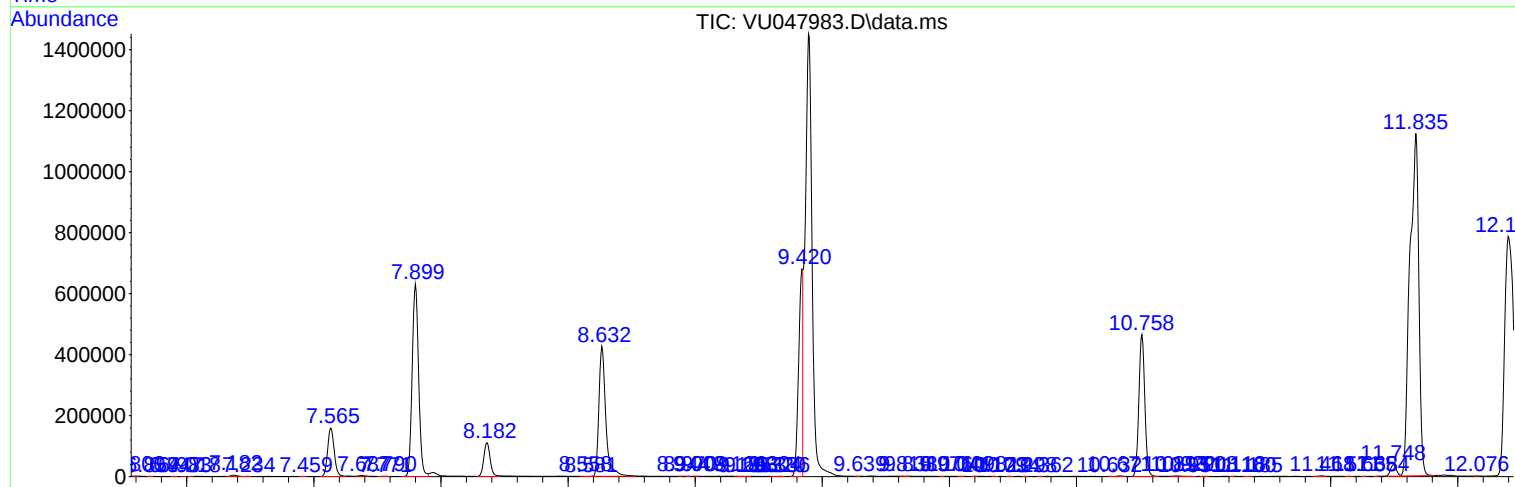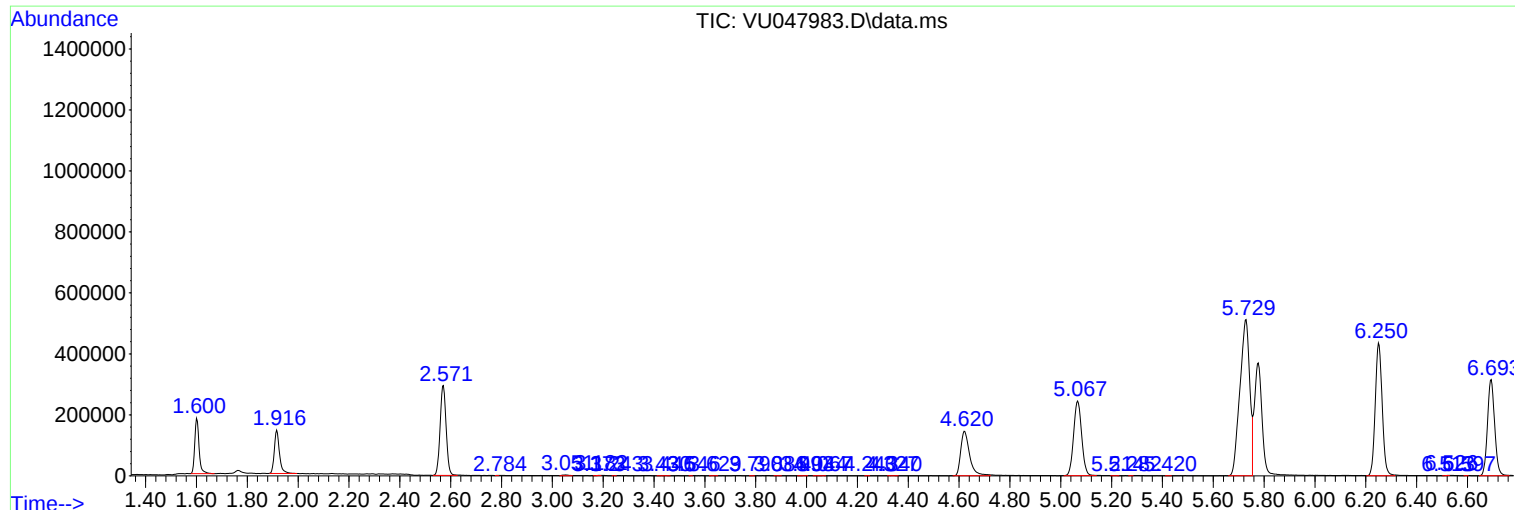

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047983.D
Acq On : 13 Apr 2022 01:56
Operator : SY/MD
Sample : N2345-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047983.D
Acq On : 13 Apr 2022 01:56
Operator : SY/MD
Sample : N2345-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------