

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047984.D
 Acq On : 13 Apr 2022 02:19
 Operator : SY/MD
 Sample : N2345-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	101	rBB	176788	206218	12.98%	1.749%
2	1.768	127	133	145	rVB7	7548	11202	0.71%	0.095%
3	1.916	170	179	195	rBV	140050	194881	12.27%	1.653%
4	2.571	370	383	398	rBV	292047	476163	29.98%	4.039%
5	2.854	467	471	474	rVB3	439	333	0.02%	0.003%
6	2.887	477	481	485	rBV4	317	329	0.02%	0.003%
7	3.009	516	519	523	rBV3	366	248	0.02%	0.002%
8	3.051	523	532	541	rVB6	2509	4902	0.31%	0.042%
9	3.096	541	546	553	rBV2	418	638	0.04%	0.005%
10	3.189	572	575	585	rVB4	939	1118	0.07%	0.009%
11	3.449	651	656	658	rBV3	268	285	0.02%	0.002%
12	3.549	682	687	690	rBV3	352	278	0.02%	0.002%
13	3.578	693	696	699	rVB2	345	244	0.02%	0.002%
14	3.700	731	734	735	rBV2	366	252	0.02%	0.002%
15	3.761	750	753	756	rBV3	408	381	0.02%	0.003%
16	4.025	831	835	838	rBV	360	361	0.02%	0.003%
17	4.070	846	849	852	rBV	397	274	0.02%	0.002%
18	4.096	855	857	859	rVV2	404	238	0.01%	0.002%
19	4.121	862	865	873	rVB3	423	491	0.03%	0.004%
20	4.186	880	885	886	rBV	350	262	0.02%	0.002%
21	4.198	886	889	895	rVB3	434	501	0.03%	0.004%
22	4.305	918	922	927	rBV3	318	345	0.02%	0.003%
23	4.623	1007	1021	1062	rBV	145117	357103	22.49%	3.029%
24	4.867	1095	1097	1102	rBV2	305	257	0.02%	0.002%
25	4.925	1112	1115	1121	rVB5	428	404	0.03%	0.003%
26	5.067	1143	1159	1183	rVV	244315	534472	33.65%	4.533%
27	5.231	1207	1210	1213	rBV	376	267	0.02%	0.002%
28	5.288	1221	1228	1229	rBV2	636	541	0.03%	0.005%
29	5.343	1239	1245	1248	rVB3	601	533	0.03%	0.005%
30	5.391	1254	1260	1262	rVB4	351	336	0.02%	0.003%
31	5.729	1339	1365	1375	rBV2	506492	1376661	86.68%	11.676%
32	6.031	1456	1459	1460	rBV	524	273	0.02%	0.002%
33	6.057	1465	1467	1473	rVV3	415	402	0.03%	0.003%
34	6.099	1478	1480	1483	rBV3	400	258	0.02%	0.002%
35	6.118	1483	1486	1489	rVB3	664	448	0.03%	0.004%
36	6.250	1509	1527	1561	rVV	413332	790892	49.80%	6.708%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047984.D
 Acq On : 13 Apr 2022 02:19
 Operator : SY/MD
 Sample : N2345-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.530	1610	1614	1617	rVV3	918	818	0.05%	0.007%
38	6.600	1633	1636	1640	rVV2	353	327	0.02%	0.003%
39	6.623	1642	1643	1648	rVB2	464	273	0.02%	0.002%
40	6.694	1648	1665	1691	rBV	313916	615391	38.75%	5.219%
41	6.948	1741	1744	1746	rBV2	314	238	0.01%	0.002%
42	7.034	1768	1771	1773	rBV	466	267	0.02%	0.002%
43	7.092	1785	1789	1792	rBV	298	239	0.02%	0.002%
44	7.108	1792	1794	1800	rVB2	464	357	0.02%	0.003%
45	7.182	1805	1817	1828	rBV3	3995	7736	0.49%	0.066%
46	7.488	1905	1912	1916	rBV3	287	342	0.02%	0.003%
47	7.568	1922	1937	1958	rBV	157124	276683	17.42%	2.347%
48	7.690	1967	1975	1983	rBV5	2561	4212	0.27%	0.036%
49	7.793	2001	2007	2009	rBV3	375	458	0.03%	0.004%
50	7.899	2020	2040	2056	rBV	630449	1079989	68.00%	9.160%
51	8.182	2115	2128	2148	rBV	110355	190647	12.00%	1.617%
52	8.256	2148	2151	2154	rVV3	587	465	0.03%	0.004%
53	8.546	2237	2241	2245	rVB3	369	264	0.02%	0.002%
54	8.571	2245	2249	2252	rBV3	365	333	0.02%	0.003%
55	8.632	2252	2268	2312	rBV	424670	807117	50.82%	6.846%
56	8.857	2332	2338	2343	rVB4	576	636	0.04%	0.005%
57	8.906	2346	2353	2355	rBV3	262	252	0.02%	0.002%
58	9.050	2395	2398	2401	rBV4	334	246	0.02%	0.002%
59	9.266	2461	2465	2469	rBV	265	323	0.02%	0.003%
60	9.349	2487	2491	2496	rBV3	205	249	0.02%	0.002%
61	9.417	2499	2512	2518	rBV	623639	1099745	69.25%	9.327%
62	9.700	2591	2600	2605	rVB3	1070	1569	0.10%	0.013%
63	9.751	2610	2616	2617	rBV2	307	237	0.01%	0.002%
64	9.944	2673	2676	2679	rVB2	322	246	0.02%	0.002%
65	9.970	2679	2684	2690	rBV2	398	540	0.03%	0.005%
66	9.999	2690	2693	2698	rVV2	347	252	0.02%	0.002%
67	10.099	2721	2724	2728	rBV3	383	403	0.03%	0.003%
68	10.147	2737	2739	2742	rVB2	510	262	0.02%	0.002%
69	10.179	2747	2749	2753	rVV2	376	375	0.02%	0.003%
70	10.359	2802	2805	2809	rBV	332	285	0.02%	0.002%
71	10.385	2810	2813	2817	rVV2	375	276	0.02%	0.002%
72	10.668	2893	2901	2914	rBV4	2444	3733	0.24%	0.032%
73	10.758	2916	2929	2954	rVV	462745	748933	47.16%	6.352%
74	10.857	2957	2960	2965	rVB4	493	549	0.03%	0.005%
75	10.886	2965	2969	2970	rBV	416	261	0.02%	0.002%
76	10.918	2977	2979	2984	rVB3	364	296	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047984.D
 Acq On : 13 Apr 2022 02:19
 Operator : SY/MD
 Sample : N2345-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.028	3011	3013	3020	rVB2	324	276	0.02%	0.002%
78	11.089	3029	3032	3038	rVB4	462	423	0.03%	0.004%
79	11.192	3057	3064	3067	rBV2	258	336	0.02%	0.003%
80	11.272	3085	3089	3090	rBV	381	239	0.02%	0.002%
81	11.365	3114	3118	3121	rBV3	435	358	0.02%	0.003%
82	11.455	3142	3146	3148	rBV3	1549	1321	0.08%	0.011%
83	11.639	3200	3203	3207	rBV2	324	321	0.02%	0.003%
84	11.687	3216	3218	3226	rVB2	637	741	0.05%	0.006%
85	11.748	3228	3237	3245	rBV2	11676	17813	1.12%	0.151%
86	11.812	3245	3257	3282	rVV2	691155	1588134	100.00%	13.470%
87	11.973	3304	3307	3315	rVB4	1925	2094	0.13%	0.018%
88	12.021	3320	3322	3327	rBV2	351	292	0.02%	0.002%
89	12.086	3337	3342	3345	rBV5	431	416	0.03%	0.004%
90	12.195	3360	3376	3402	rBV2	665167	1277713	80.45%	10.837%
91	12.362	3426	3428	3431	rBV	597	362	0.02%	0.003%
92	12.510	3470	3474	3478	rVB3	451	358	0.02%	0.003%
93	12.976	3616	3619	3626	rVB2	1141	1146	0.07%	0.010%
94	13.381	3742	3745	3754	rVB4	865	952	0.06%	0.008%
95	13.680	3835	3838	3841	rBV2	351	272	0.02%	0.002%
96	13.844	3878	3889	3906	rBV2	50052	80300	5.06%	0.681%
97	14.098	3965	3968	3972	rBV4	605	440	0.03%	0.004%
98	14.333	4034	4041	4052	rVB5	3770	5312	0.33%	0.045%
99	14.732	4162	4165	4171	rBV4	531	540	0.03%	0.005%
100	15.545	4415	4418	4425	rVB4	1520	1665	0.10%	0.014%

Sum of corrected areas: 11790439




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047984.D
Acq On : 13 Apr 2022 02:19
Operator : SY/MD
Sample : N2345-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

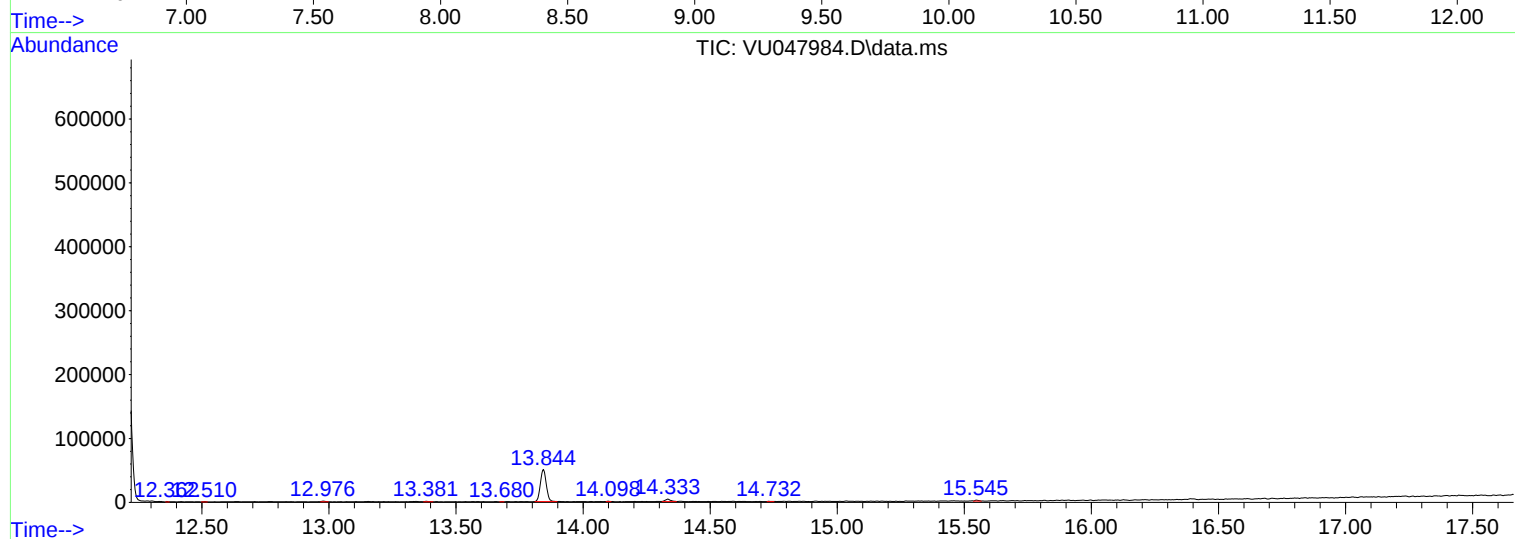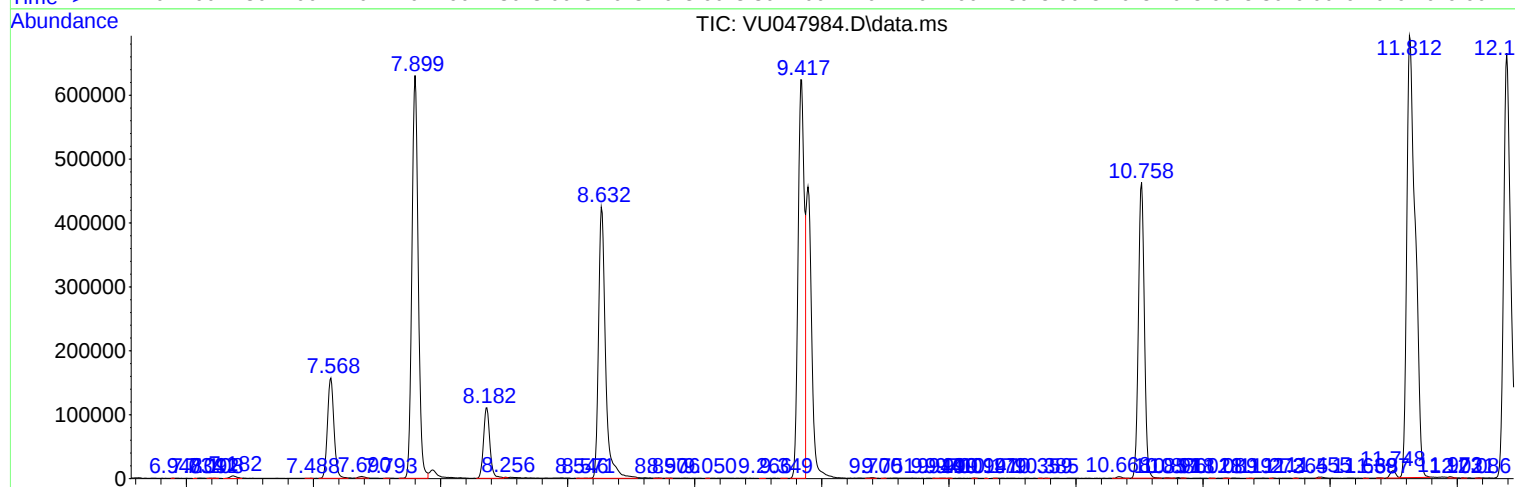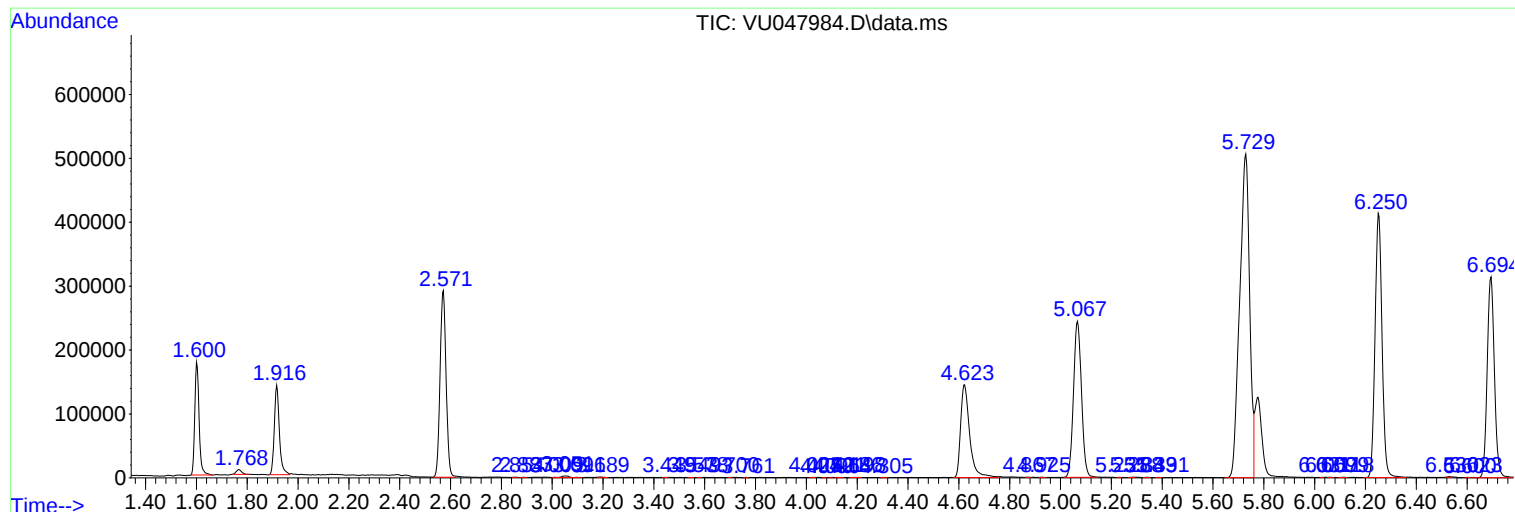

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047984.D
Acq On : 13 Apr 2022 02:19
Operator : SY/MD
Sample : N2345-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047984.D
Acq On : 13 Apr 2022 02:19
Operator : SY/MD
Sample : N2345-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc