


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047940.D
Acq On : 12 Apr 2022 08:59
Operator : SY/MD
Sample : BFB062
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB062

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Title : VOC Analysis
Last Update : Sat Apr 16 00:34:16 2022

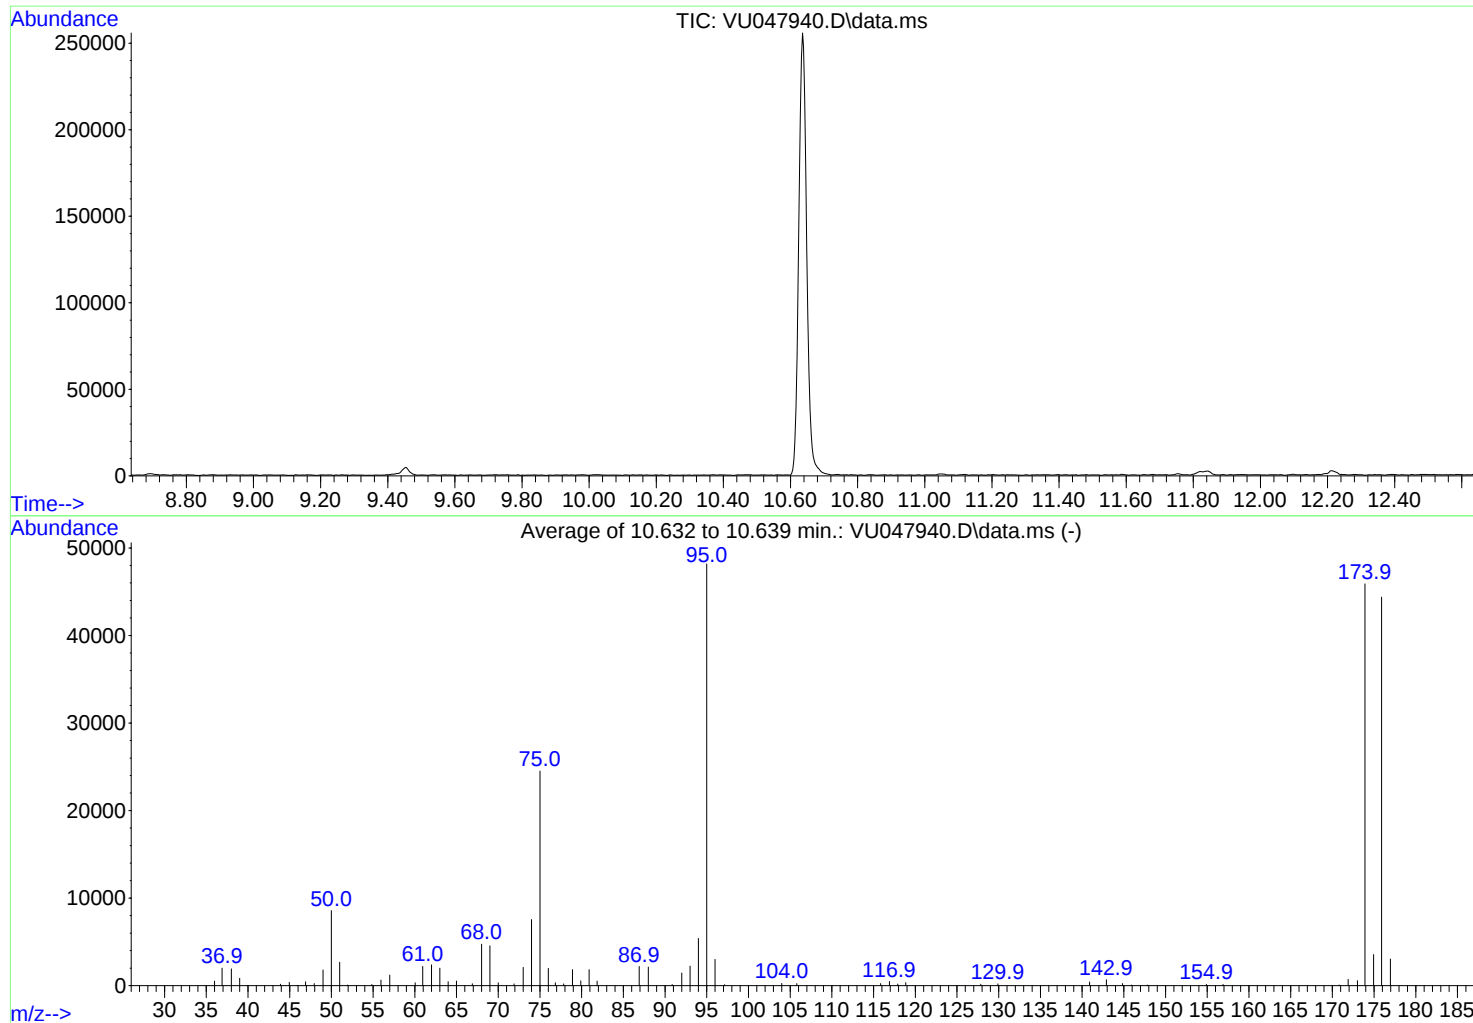

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	8572	PASS
75	95	30	80	50.9	24507	PASS
95	95	100	100	100.0	48187	PASS
96	95	5	9	6.2	2997	PASS
173	174	0.00	2	1.2	563	PASS
174	95	50	120	95.3	45901	PASS
175	174	5	9	7.7	3555	PASS
176	174	95	101	96.7	44384	PASS
177	176	5	9	6.8	3027	PASS

m/z	Abundance
40.00	125.0
43.90	449.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

m/z	Abundance
36.00	533.0
36.90	1954.0
38.00	1992.0
39.00	845.0
39.90	166.0
44.00	639.0
44.90	400.0
46.90	455.0
47.90	168.0
49.00	1810.0
50.00	8447.0
51.00	2586.0
54.90	112.0
56.00	643.0
57.00	1144.0
60.10	317.0
61.00	2249.0
62.00	2447.0
63.00	1968.0
64.00	466.0
65.00	538.0
66.90	179.0
68.00	4573.0
69.00	4397.0
70.00	327.0
71.90	225.0
73.00	2029.0
74.00	7347.0
75.00	24392.0
76.00	2001.0
76.90	352.0
77.90	177.0
78.90	1839.0
79.90	550.0
80.90	1882.0
81.80	494.0
86.90	2109.0
88.00	1998.0
90.90	136.0
92.00	1416.0
93.00	2144.0
94.00	5402.0
95.00	47360.0
96.00	3054.0
97.20	106.0
104.10	291.0
105.80	205.0
115.90	244.0
116.90	405.0
117.90	166.0
118.90	293.0
127.80	133.0
129.90	178.0
140.90	396.0
142.90	644.0
144.90	266.0
154.90	146.0
156.90	119.0
171.90	661.0
173.00	518.0
173.90	43856.0
175.00	3452.0
175.90	42088.0
177.00	3017.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

m/z	Abundance
36.00	539.0
36.90	2027.0
38.00	1925.0
39.00	858.0
39.90	159.0
44.00	616.0
45.00	400.0
46.90	454.0
48.00	227.0
49.00	1830.0
50.00	8947.0
51.00	2791.0
52.00	109.0
54.80	108.0
56.00	659.0
57.00	1202.0
60.10	334.0
61.00	2272.0
62.00	2488.0
63.00	2036.0
64.00	485.0
65.00	541.0
66.90	243.0
68.00	4897.0
69.00	4646.0
70.00	321.0
71.90	204.0
73.00	2121.0
74.00	7721.0
75.00	25280.0
76.00	2039.0
76.80	331.0
77.90	217.0
78.90	1864.0
79.90	563.0
80.90	1861.0
81.80	538.0
86.90	2246.0
88.00	2239.0
90.80	126.0
92.00	1464.0
93.00	2311.0
94.00	5514.0
95.00	49832.0
96.00	3015.0
97.10	110.0
104.00	270.0
105.80	255.0
115.90	239.0
116.90	500.0
117.90	198.0
118.80	368.0
127.90	166.0
129.90	205.0
140.90	421.0
142.90	719.0
144.90	248.0
145.90	105.0
147.80	111.0
154.90	158.0
156.90	156.0
170.80	110.0
171.90	741.0
173.00	597.0
173.90	47192.0
174.90	3617.0
175.90	45632.0
177.00	3129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

m/z	Abundance
36.00	466.0
36.90	1990.0
38.00	1828.0
39.00	825.0
39.90	158.0
43.90	584.0
45.00	355.0
45.90	102.0
46.90	426.0
48.00	307.0
49.00	1741.0
50.00	8321.0
51.00	2614.0
51.90	139.0
54.80	148.0
55.90	645.0
57.00	1282.0
60.00	317.0
60.90	2078.0
62.00	2218.0
63.00	1949.0
64.00	431.0
65.00	516.0
66.90	228.0
68.00	4732.0
69.00	4604.0
70.00	341.0
71.90	179.0
73.00	2094.0
74.00	7564.0
75.00	23848.0
76.00	1905.0
76.80	300.0
77.80	208.0
78.90	1803.0
79.90	539.0
80.90	1750.0
81.90	522.0
86.90	2214.0
88.00	2146.0
90.80	128.0
92.00	1448.0
93.00	2230.0
94.00	5266.0
95.00	47368.0
96.00	2923.0
97.10	102.0
103.90	209.0
105.80	270.0
115.80	226.0
116.90	503.0
117.90	194.0
118.80	379.0
127.90	183.0
129.90	220.0
140.90	424.0
142.90	695.0
144.80	202.0
145.90	117.0
147.80	118.0
154.90	152.0
156.90	138.0
170.80	117.0
171.90	757.0
173.00	575.0
173.90	46656.0
174.90	3596.0
175.90	45432.0
176.90	2936.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062