

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053657.D
 Acq On : 12 Apr 2023 13:22
 Operator : JC/MD
 Sample : 02251-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	109515	130750	17.03%	2.074%
2	1.909	169	177	192	rBV	83778	115930	15.10%	1.839%
3	2.562	369	380	401	rBV	160478	264091	34.40%	4.189%
4	2.729	430	432	435	rBV2	382	218	0.03%	0.003%
5	3.211	579	582	585	rBV	168	100	0.01%	0.002%
6	3.231	585	588	591	rBV	308	197	0.03%	0.003%
7	3.276	599	602	606	rBV2	234	184	0.02%	0.003%
8	3.327	616	618	622	rVB	208	91	0.01%	0.001%
9	3.890	792	793	794	rBV	137	41	0.01%	0.001%
10	4.259	906	908	915	rBV2	266	306	0.04%	0.005%
11	4.343	933	934	936	rVB2	129	46	0.01%	0.001%
12	4.430	958	961	964	rBV	139	75	0.01%	0.001%
13	4.520	986	989	993	rVB	494	250	0.03%	0.004%
14	4.613	1007	1018	1040	rBV	60207	143926	18.75%	2.283%
15	5.054	1140	1155	1182	rBV	138584	311367	40.56%	4.939%
16	5.282	1223	1226	1234	rBV2	554	500	0.07%	0.008%
17	5.324	1235	1239	1242	rBV2	347	305	0.04%	0.005%
18	5.388	1257	1259	1261	rBV	210	89	0.01%	0.001%
19	5.542	1305	1307	1310	rBV2	217	129	0.02%	0.002%
20	5.565	1312	1314	1319	rVB	274	152	0.02%	0.002%
21	5.719	1342	1362	1381	rBV2	283938	767643	100.00%	12.178%
22	5.960	1433	1437	1440	rBV3	505	535	0.07%	0.008%
23	6.041	1461	1462	1465	rBV	208	104	0.01%	0.002%
24	6.243	1511	1525	1545	rBV	287554	550706	71.74%	8.736%
25	6.465	1592	1594	1596	rBV	107	61	0.01%	0.001%
26	6.517	1605	1610	1616	rBV4	2091	3267	0.43%	0.052%
27	6.684	1649	1662	1685	rBV	176741	343622	44.76%	5.451%
28	6.800	1696	1698	1701	rBV3	632	384	0.05%	0.006%
29	6.838	1708	1710	1712	rBV2	186	114	0.01%	0.002%
30	6.864	1716	1718	1721	rBV2	223	134	0.02%	0.002%
31	7.002	1758	1761	1767	rVB2	310	272	0.04%	0.004%
32	7.025	1767	1768	1769	rBV2	123	37	0.00%	0.001%
33	7.166	1809	1812	1813	rBV	225	110	0.01%	0.002%
34	7.179	1814	1816	1820	rVV2	794	519	0.07%	0.008%
35	7.198	1820	1822	1828	rVB3	528	438	0.06%	0.007%
36	7.253	1838	1839	1840	rVB	207	40	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053657.D
 Acq On : 12 Apr 2023 13:22
 Operator : JC/MD
 Sample : 02251-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.266	1840	1843	1845	rBV2	197	126	0.02%	0.002%
38	7.388	1878	1881	1884	rVB2	263	190	0.02%	0.003%
39	7.562	1923	1935	1956	rBV	100808	176701	23.02%	2.803%
40	7.755	1993	1995	1999	rBV	207	187	0.02%	0.003%
41	7.893	2024	2038	2067	rBV	375974	645569	84.10%	10.241%
42	8.176	2114	2126	2146	rBV2	68981	119978	15.63%	1.903%
43	8.343	2175	2178	2181	rVB	265	167	0.02%	0.003%
44	8.365	2183	2185	2187	rBV	249	94	0.01%	0.001%
45	8.417	2200	2201	2202	rBV	226	74	0.01%	0.001%
46	8.626	2255	2266	2296	rBV	184750	338242	44.06%	5.366%
47	8.986	2374	2378	2380	rBV2	261	162	0.02%	0.003%
48	9.047	2394	2397	2399	rBV2	186	131	0.02%	0.002%
49	9.079	2404	2407	2410	rVV	230	135	0.02%	0.002%
50	9.124	2418	2421	2425	rBV2	232	197	0.03%	0.003%
51	9.414	2498	2511	2538	rBV	404215	682643	88.93%	10.829%
52	9.645	2579	2583	2585	rBV	357	257	0.03%	0.004%
53	9.732	2607	2610	2613	rBV	351	222	0.03%	0.004%
54	9.751	2613	2616	2617	rBV	214	95	0.01%	0.002%
55	9.790	2627	2628	2629	rBV	279	80	0.01%	0.001%
56	10.098	2722	2724	2725	rBV	192	64	0.01%	0.001%
57	10.115	2727	2729	2731	rVB	431	151	0.02%	0.002%
58	10.127	2731	2733	2735	rBV	253	113	0.01%	0.002%
59	10.330	2793	2796	2798	rBV2	298	207	0.03%	0.003%
60	10.362	2803	2806	2807	rBV2	183	82	0.01%	0.001%
61	10.751	2914	2927	2947	rBV	253272	407256	53.05%	6.461%
62	10.970	2992	2995	2997	rBV	201	144	0.02%	0.002%
63	11.053	3017	3021	3025	rVB2	249	192	0.03%	0.003%
64	11.073	3025	3027	3029	rBV	174	89	0.01%	0.001%
65	11.304	3097	3099	3102	rBV2	306	162	0.02%	0.003%
66	11.549	3170	3175	3178	rBV2	269	284	0.04%	0.005%
67	11.597	3187	3190	3194	rBV	245	146	0.02%	0.002%
68	11.745	3232	3236	3237	rBV	687	474	0.06%	0.008%
69	11.809	3243	3256	3277	rBV	427799	688447	89.68%	10.921%
70	12.188	3362	3374	3392	rBV	368781	601152	78.31%	9.536%
71	12.333	3416	3419	3422	rBV2	404	350	0.05%	0.006%
72	13.034	3635	3637	3642	rBV2	580	433	0.06%	0.007%
73	13.079	3650	3651	3655	rVB	367	139	0.02%	0.002%
74	13.819	3879	3881	3884	rBV	250	118	0.02%	0.002%
75	13.851	3886	3891	3898	rVB	1069	1374	0.18%	0.022%
76	13.921	3910	3913	3917	rBV	441	380	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053657.D
Acq On : 12 Apr 2023 13:22
Operator : JC/MD
Sample : 02251-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis




Sum of corrected areas: 6303740

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053657.D
Acq On : 12 Apr 2023 13:22
Operator : JC/MD
Sample : 02251-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

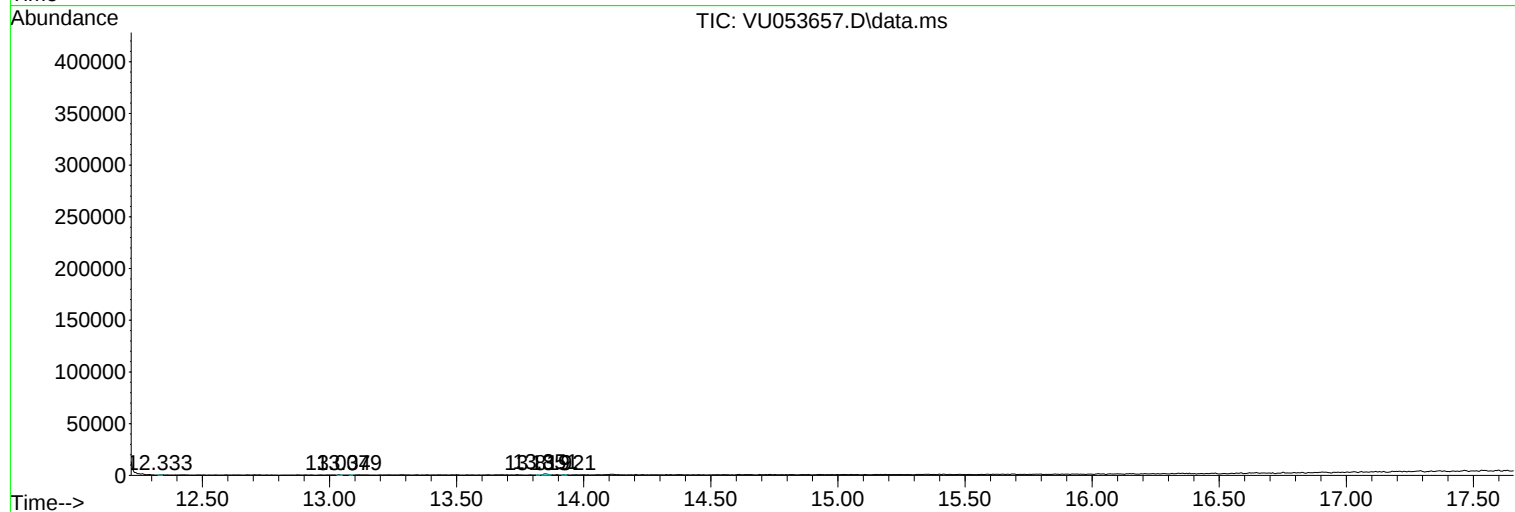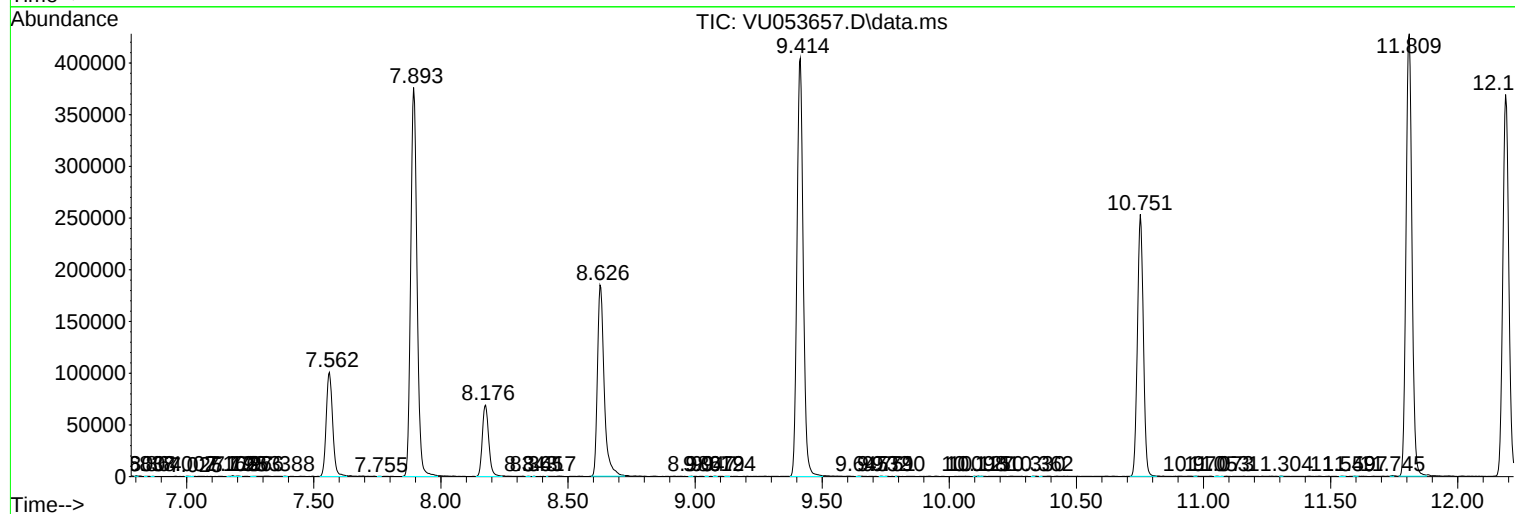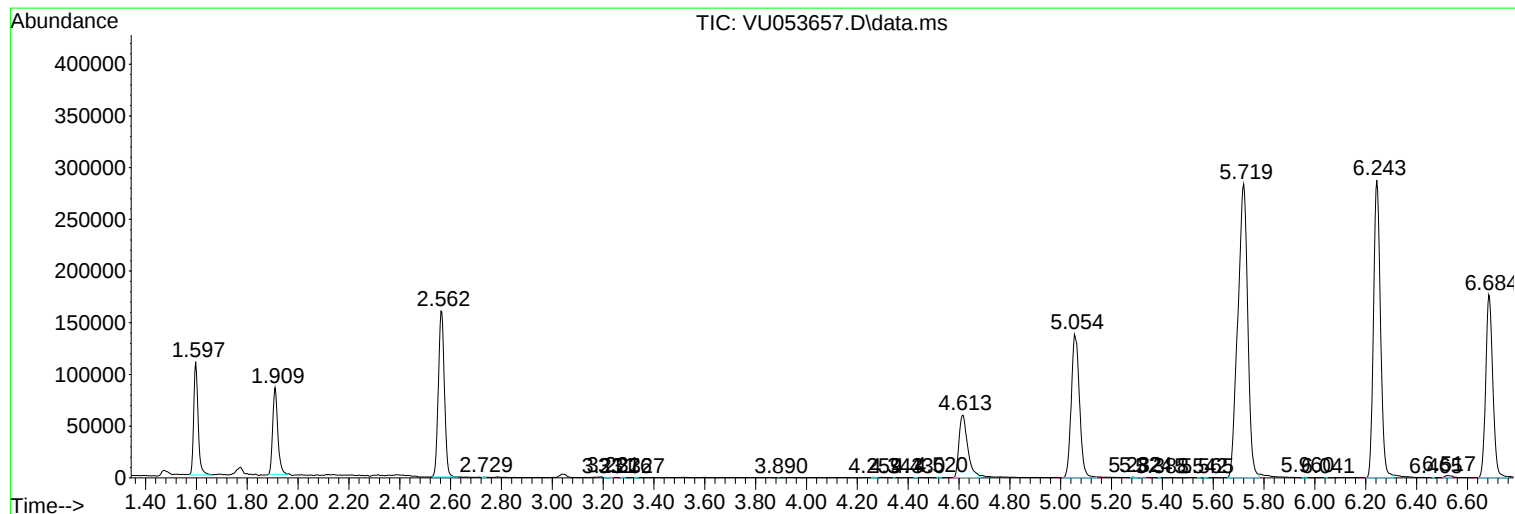

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053657.D
Acq On : 12 Apr 2023 13:22
Operator : JC/MD
Sample : 02251-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053657.D
Acq On : 12 Apr 2023 13:22
Operator : JC/MD
Sample : 02251-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------