

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053658.D
 Acq On : 12 Apr 2023 13:46
 Operator : JC/MD
 Sample : 02252-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	91455	108779	13.65%	1.737%
2	1.909	170	177	192	rVB	82534	111651	14.01%	1.783%
3	2.562	369	380	393	rBV	151813	242765	30.47%	3.878%
4	2.858	469	472	474	rBV	279	224	0.03%	0.004%
5	2.890	477	482	486	rVV4	534	574	0.07%	0.009%
6	2.909	486	488	491	rVV	275	152	0.02%	0.002%
7	2.938	491	497	501	rVB	332	329	0.04%	0.005%
8	3.044	523	530	534	rBV4	741	1064	0.13%	0.017%
9	3.160	559	566	568	rBV3	703	821	0.10%	0.013%
10	3.334	616	620	624	rBV	293	261	0.03%	0.004%
11	3.433	648	651	654	rBV2	236	157	0.02%	0.003%
12	3.456	654	658	661	rVV	323	255	0.03%	0.004%
13	3.543	681	685	691	rVB2	251	197	0.02%	0.003%
14	3.578	691	696	698	rBV2	376	274	0.03%	0.004%
15	3.883	788	791	795	rVB	285	178	0.02%	0.003%
16	4.009	827	830	832	rVV2	249	164	0.02%	0.003%
17	4.153	868	875	880	rVB2	264	343	0.04%	0.005%
18	4.186	880	885	891	rBV2	342	460	0.06%	0.007%
19	4.272	908	912	918	rVB2	245	292	0.04%	0.005%
20	4.305	918	922	924	rBV	273	198	0.02%	0.003%
21	4.369	939	942	949	rVB	187	187	0.02%	0.003%
22	4.449	963	967	975	rBV2	290	363	0.05%	0.006%
23	4.562	998	1002	1005	rBV	249	193	0.02%	0.003%
24	4.613	1005	1018	1042	rBV	74073	179662	22.55%	2.870%
25	4.951	1120	1123	1127	rVB2	334	221	0.03%	0.004%
26	5.057	1141	1156	1181	rVV	153549	333036	41.79%	5.319%
27	5.279	1222	1225	1227	rBV	276	160	0.02%	0.003%
28	5.327	1235	1240	1242	rBV	249	214	0.03%	0.003%
29	5.510	1293	1297	1298	rBV2	246	202	0.03%	0.003%
30	5.719	1341	1362	1383	rBV2	290300	796833	100.00%	12.727%
31	6.002	1446	1450	1453	rBV2	203	171	0.02%	0.003%
32	6.243	1511	1525	1550	rBV2	246189	474011	59.49%	7.571%
33	6.491	1598	1602	1604	rBV2	355	242	0.03%	0.004%
34	6.523	1604	1612	1614	rBV3	2499	3255	0.41%	0.052%
35	6.684	1649	1662	1688	rBV	185424	364421	45.73%	5.821%
36	6.973	1748	1752	1759	rVB2	278	287	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053658.D
 Acq On : 12 Apr 2023 13:46
 Operator : JC/MD
 Sample : 02252-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CMD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.182	1810	1817	1819	rBV4	1185	1184	0.15%	0.019%
38	7.276	1841	1846	1849	rBV2	242	254	0.03%	0.004%
39	7.301	1852	1854	1862	rVB2	295	237	0.03%	0.004%
40	7.346	1862	1868	1870	rVB2	208	200	0.03%	0.003%
41	7.372	1871	1876	1879	rBV2	190	175	0.02%	0.003%
42	7.398	1879	1884	1885	rBV	234	156	0.02%	0.002%
43	7.562	1923	1935	1956	rBV	101452	179999	22.59%	2.875%
44	7.674	1966	1970	1971	rBV	426	220	0.03%	0.004%
45	7.809	2010	2012	2018	rVB	237	200	0.03%	0.003%
46	7.893	2024	2038	2067	rBV	368189	642053	80.58%	10.255%
47	8.083	2093	2097	2101	rBV3	388	390	0.05%	0.006%
48	8.176	2114	2126	2140	rBV	70709	120929	15.18%	1.932%
49	8.279	2153	2158	2163	rBV3	446	494	0.06%	0.008%
50	8.523	2229	2234	2239	rBV2	250	269	0.03%	0.004%
51	8.549	2240	2242	2247	rVB2	266	186	0.02%	0.003%
52	8.626	2255	2266	2301	rBV	221236	411887	51.69%	6.579%
53	8.832	2327	2330	2335	rVB2	335	244	0.03%	0.004%
54	8.883	2343	2346	2351	rBV2	187	176	0.02%	0.003%
55	8.941	2361	2364	2371	rVB	369	279	0.04%	0.004%
56	8.980	2371	2376	2378	rBV2	217	203	0.03%	0.003%
57	9.063	2399	2402	2407	rBV2	252	256	0.03%	0.004%
58	9.115	2415	2418	2421	rVB2	279	189	0.02%	0.003%
59	9.134	2421	2424	2427	rVB2	201	145	0.02%	0.002%
60	9.189	2437	2441	2444	rBV	173	154	0.02%	0.002%
61	9.275	2462	2468	2472	rBV2	310	304	0.04%	0.005%
62	9.349	2488	2491	2493	rVB	276	150	0.02%	0.002%
63	9.414	2497	2511	2538	rBV	347052	577316	72.45%	9.221%
64	9.742	2608	2613	2616	rBV	199	188	0.02%	0.003%
65	9.796	2624	2630	2632	rBV	455	315	0.04%	0.005%
66	9.848	2642	2646	2651	rVV	243	196	0.02%	0.003%
67	9.989	2687	2690	2692	rBV	208	152	0.02%	0.002%
68	10.063	2710	2713	2716	rBV2	283	192	0.02%	0.003%
69	10.173	2741	2747	2752	rBV2	258	249	0.03%	0.004%
70	10.488	2840	2845	2848	rBV	436	321	0.04%	0.005%
71	10.661	2895	2899	2900	rBV2	236	186	0.02%	0.003%
72	10.751	2912	2927	2944	rVV	286279	462089	57.99%	7.381%
73	10.886	2962	2969	2971	rBV2	685	633	0.08%	0.010%
74	11.076	3024	3028	3030	rVV2	194	150	0.02%	0.002%
75	11.092	3030	3033	3038	rVB	450	241	0.03%	0.004%
76	11.137	3043	3047	3052	rBV2	261	256	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053658.D
 Acq On : 12 Apr 2023 13:46
 Operator : JC/MD
 Sample : 02252-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.208	3061	3069	3074	rBV	418	534	0.07%	0.009%
78	11.246	3078	3081	3084	rVB2	245	163	0.02%	0.003%
79	11.513	3161	3164	3166	rBV2	268	170	0.02%	0.003%
80	11.555	3174	3177	3180	rVB2	260	151	0.02%	0.002%
81	11.748	3228	3237	3242	rVB2	533	809	0.10%	0.013%
82	11.809	3243	3256	3276	rBV	356920	577880	72.52%	9.230%
83	11.935	3292	3295	3300	rVB2	342	268	0.03%	0.004%
84	11.960	3300	3303	3304	rBV	305	182	0.02%	0.003%
85	12.002	3314	3316	3321	rVB	366	167	0.02%	0.003%
86	12.034	3321	3326	3328	rBV	327	226	0.03%	0.004%
87	12.189	3362	3374	3392	rBV	401623	647148	81.22%	10.337%
88	12.417	3440	3445	3446	rBV	232	193	0.02%	0.003%
89	12.799	3561	3564	3569	rVB2	331	279	0.04%	0.004%
90	12.828	3570	3573	3574	rBV2	359	147	0.02%	0.002%
91	12.893	3587	3593	3600	rBV6	1056	1498	0.19%	0.024%
92	13.256	3703	3706	3708	rBV2	255	152	0.02%	0.002%
93	13.407	3749	3753	3758	rBV	322	349	0.04%	0.006%
94	13.587	3805	3809	3810	rBV	335	243	0.03%	0.004%
95	13.664	3830	3833	3835	rBV3	313	201	0.03%	0.003%
96	13.713	3846	3848	3851	rBV	389	241	0.03%	0.004%
97	13.812	3876	3879	3883	rBV2	308	192	0.02%	0.003%
98	13.841	3883	3888	3898	rVB5	1667	2389	0.30%	0.038%
99	14.008	3935	3940	3942	rBV2	426	362	0.05%	0.006%
100	14.336	4037	4042	4046	rBV3	769	811	0.10%	0.013%




Sum of corrected areas: 6260768

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053658.D
Acq On : 12 Apr 2023 13:46
Operator : JC/MD
Sample : 02252-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

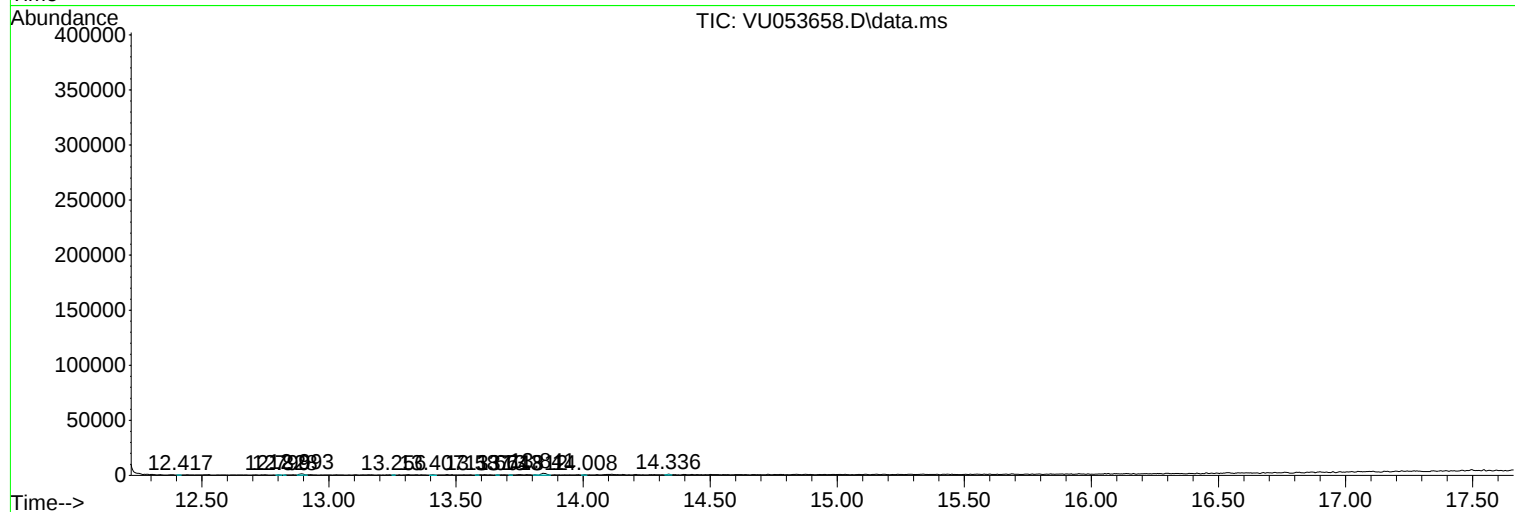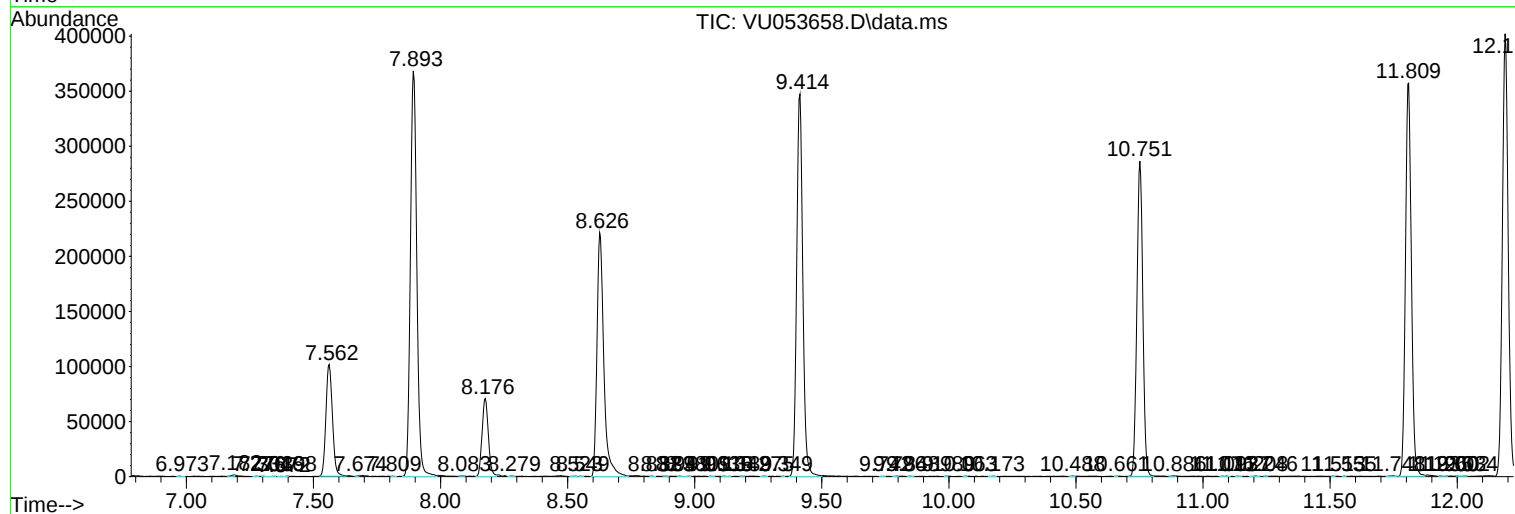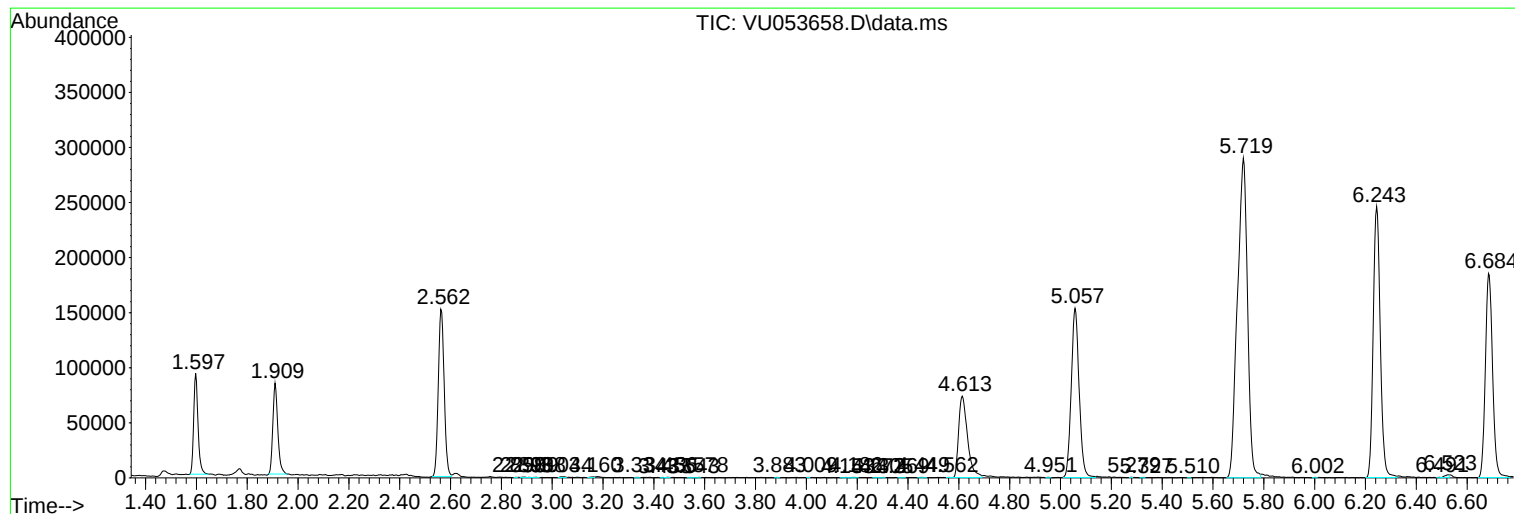

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053658.D
Acq On : 12 Apr 2023 13:46
Operator : JC/MD
Sample : 02252-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053658.D
Acq On : 12 Apr 2023 13:46
Operator : JC/MD
Sample : 02252-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------