

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053661.D
 Acq On : 12 Apr 2023 14:56
 Operator : JC/MD
 Sample : 02252-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	89520	105758	12.87%	1.551%
2	1.909	169	177	194	rBV	81318	116796	14.21%	1.713%
3	2.562	368	380	396	rBV	158022	250859	30.52%	3.678%
4	2.986	509	512	515	rBV	383	345	0.04%	0.005%
5	3.031	524	526	532	rBV2	528	537	0.07%	0.008%
6	3.308	608	612	615	rBV2	204	216	0.03%	0.003%
7	3.485	664	667	670	rBV2	246	183	0.02%	0.003%
8	3.549	685	687	691	rVB	360	235	0.03%	0.003%
9	3.617	706	708	712	rVB2	361	190	0.02%	0.003%
10	3.636	712	714	721	rVB	222	134	0.02%	0.002%
11	3.858	780	783	786	rVV2	334	209	0.03%	0.003%
12	3.877	786	789	793	rVB	302	184	0.02%	0.003%
13	4.002	822	828	829	rBV	156	167	0.02%	0.002%
14	4.160	874	877	879	rBV	279	207	0.03%	0.003%
15	4.263	904	909	911	rBV	199	184	0.02%	0.003%
16	4.337	929	932	935	rVB	278	192	0.02%	0.003%
17	4.385	944	947	950	rVB	386	192	0.02%	0.003%
18	4.462	967	971	975	rBV2	266	212	0.03%	0.003%
19	4.485	975	978	981	rVB	352	210	0.03%	0.003%
20	4.507	981	985	988	rBV2	329	316	0.04%	0.005%
21	4.555	997	1000	1003	rBV	319	186	0.02%	0.003%
22	4.613	1003	1018	1051	rBV	78912	194341	23.65%	2.850%
23	4.883	1099	1102	1104	rBV	259	198	0.02%	0.003%
24	5.057	1139	1156	1181	rBV	153175	340948	41.49%	4.999%
25	5.363	1248	1251	1254	rBV2	300	219	0.03%	0.003%
26	5.433	1267	1273	1275	rBV	298	259	0.03%	0.004%
27	5.600	1322	1325	1327	rBV2	212	138	0.02%	0.002%
28	5.719	1338	1362	1383	rBV2	297725	821829	100.00%	12.050%
29	5.964	1435	1438	1441	rVB	409	235	0.03%	0.003%
30	6.051	1462	1465	1468	rBV	299	191	0.02%	0.003%
31	6.067	1468	1470	1474	rVB2	271	167	0.02%	0.002%
32	6.189	1506	1508	1511	rBV	190	135	0.02%	0.002%
33	6.244	1511	1525	1556	rBV	309350	589483	71.73%	8.643%
34	6.494	1601	1603	1605	rBV	243	136	0.02%	0.002%
35	6.523	1605	1612	1623	rVB5	2583	4567	0.56%	0.067%
36	6.684	1648	1662	1680	rBV	196403	376945	45.87%	5.527%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053661.D
 Acq On : 12 Apr 2023 14:56
 Operator : JC/MD
 Sample : 02252-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.906	1728	1731	1735	rVB2	209	195	0.02%	0.003%
38	7.028	1766	1769	1774	rVB	271	283	0.03%	0.004%
39	7.182	1812	1817	1829	rVB4	1408	2385	0.29%	0.035%
40	7.263	1840	1842	1847	rVB2	284	200	0.02%	0.003%
41	7.298	1847	1853	1858	rBV2	301	417	0.05%	0.006%
42	7.362	1870	1873	1877	rVB2	338	246	0.03%	0.004%
43	7.388	1877	1881	1883	rBV	277	263	0.03%	0.004%
44	7.443	1894	1898	1906	rVB	342	433	0.05%	0.006%
45	7.559	1923	1934	1955	rBV	104284	185751	22.60%	2.724%
46	7.645	1959	1961	1966	rVB4	627	526	0.06%	0.008%
47	7.694	1966	1976	1979	rBV5	777	1356	0.16%	0.020%
48	7.748	1986	1993	1998	rBV2	341	411	0.05%	0.006%
49	7.777	1999	2002	2006	rBV2	239	201	0.02%	0.003%
50	7.893	2024	2038	2068	rBV	385204	662047	80.56%	9.707%
51	8.176	2114	2126	2150	rVV2	74752	127388	15.50%	1.868%
52	8.327	2170	2173	2177	rVB2	223	195	0.02%	0.003%
53	8.411	2196	2199	2200	rBV	218	134	0.02%	0.002%
54	8.520	2231	2233	2237	rVB	241	149	0.02%	0.002%
55	8.546	2237	2241	2243	rBV	456	248	0.03%	0.004%
56	8.584	2247	2253	2255	rBV2	256	269	0.03%	0.004%
57	8.626	2255	2266	2300	rBV	238306	434246	52.84%	6.367%
58	8.925	2356	2359	2367	rVB2	271	337	0.04%	0.005%
59	8.964	2367	2371	2372	rBV2	266	162	0.02%	0.002%
60	9.002	2378	2383	2388	rBV	209	266	0.03%	0.004%
61	9.070	2400	2404	2406	rBV	252	163	0.02%	0.002%
62	9.108	2406	2416	2419	rBV	289	438	0.05%	0.006%
63	9.189	2435	2441	2443	rBV2	312	312	0.04%	0.005%
64	9.266	2461	2465	2468	rBV2	325	262	0.03%	0.004%
65	9.304	2474	2477	2479	rBV2	224	145	0.02%	0.002%
66	9.356	2489	2493	2496	rBV2	328	280	0.03%	0.004%
67	9.414	2496	2511	2534	rBV	425667	711802	86.61%	10.437%
68	9.581	2561	2563	2565	rBV	283	138	0.02%	0.002%
69	9.722	2603	2607	2611	rBV	161	153	0.02%	0.002%
70	9.841	2640	2644	2648	rBV2	308	292	0.04%	0.004%
71	9.948	2673	2677	2680	rBV2	250	212	0.03%	0.003%
72	9.996	2689	2692	2696	rBV2	226	241	0.03%	0.004%
73	10.224	2761	2763	2765	rBV	296	163	0.02%	0.002%
74	10.295	2782	2785	2787	rBV	251	170	0.02%	0.002%
75	10.375	2808	2810	2816	rVV2	240	219	0.03%	0.003%
76	10.414	2820	2822	2825	rVB	376	176	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053661.D
 Acq On : 12 Apr 2023 14:56
 Operator : JC/MD
 Sample : 02252-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.497	2845	2848	2853	rBV2	237	199	0.02%	0.003%
78	10.681	2901	2905	2914	rBV	406	553	0.07%	0.008%
79	10.751	2914	2927	2944	rBV	300406	486772	59.23%	7.137%
80	10.890	2967	2970	2976	rVB2	851	702	0.09%	0.010%
81	11.002	3001	3005	3008	rBV	217	161	0.02%	0.002%
82	11.034	3008	3015	3020	rVV2	320	415	0.05%	0.006%
83	11.144	3046	3049	3051	rBV	191	143	0.02%	0.002%
84	11.253	3080	3083	3087	rVB2	363	304	0.04%	0.004%
85	11.333	3105	3108	3110	rBV	263	206	0.03%	0.003%
86	11.716	3223	3227	3231	rBV2	246	302	0.04%	0.004%
87	11.742	3232	3235	3240	rVB3	567	490	0.06%	0.007%
88	11.806	3243	3255	3274	rBV	451614	720757	87.70%	10.568%
89	12.189	3362	3374	3399	rBV	409129	665657	81.00%	9.760%
90	12.414	3441	3444	3449	rVB	238	233	0.03%	0.003%
91	12.484	3462	3466	3470	rBV	325	252	0.03%	0.004%
92	12.645	3513	3516	3520	rBV2	193	152	0.02%	0.002%
93	12.751	3546	3549	3551	rBV2	300	207	0.03%	0.003%
94	12.931	3602	3605	3610	rVB2	224	210	0.03%	0.003%
95	13.115	3656	3662	3663	rBV	312	237	0.03%	0.003%
96	13.812	3876	3879	3882	rBV	270	226	0.03%	0.003%
97	13.928	3913	3915	3918	rBV2	243	136	0.02%	0.002%
98	14.002	3934	3938	3941	rBV	418	343	0.04%	0.005%
99	14.246	4010	4014	4017	rBV	418	433	0.05%	0.006%
100	15.381	4364	4367	4372	rBV2	485	466	0.06%	0.007%


Sum of corrected areas: 6820133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053661.D
Acq On : 12 Apr 2023 14:56
Operator : JC/MD
Sample : 02252-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

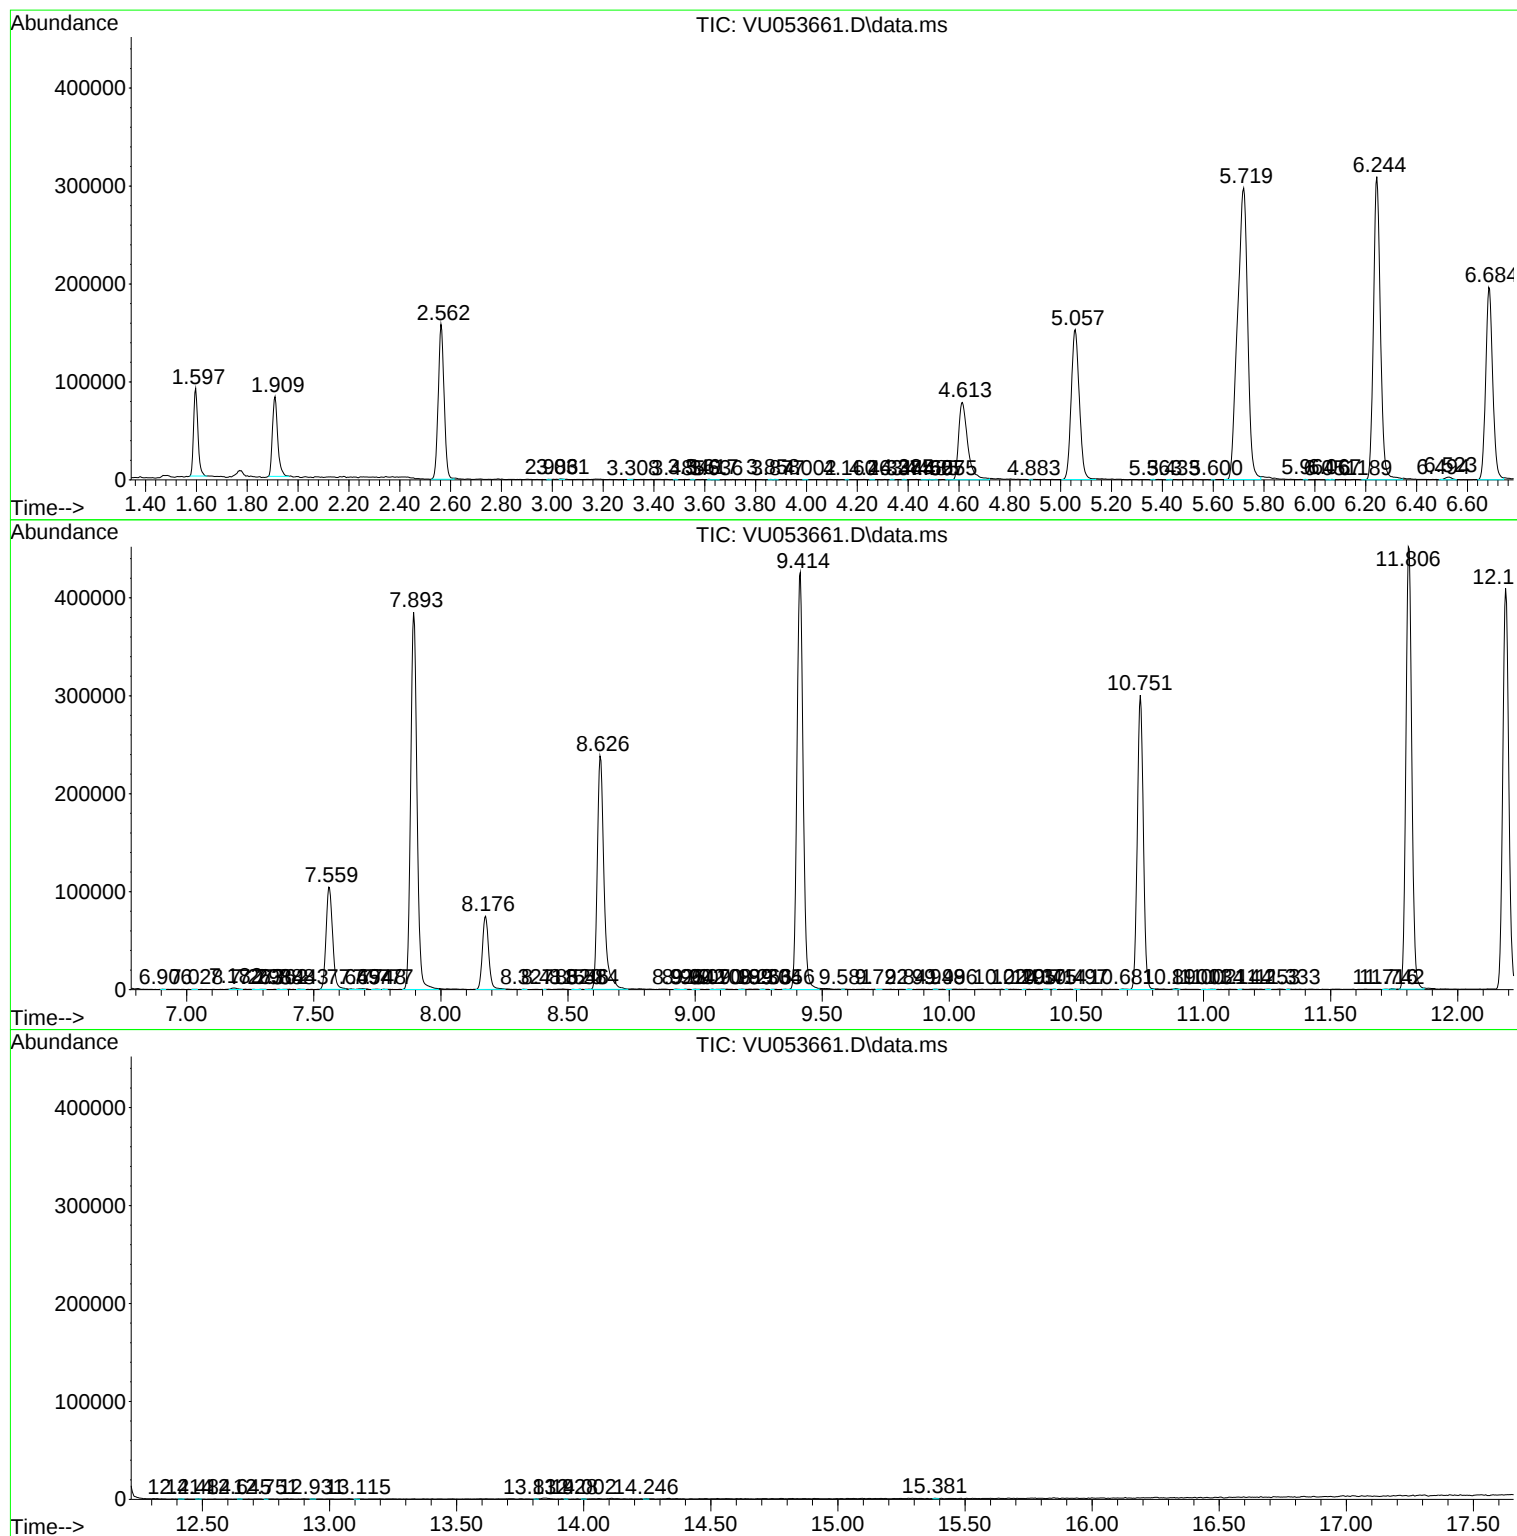

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053661.D
Acq On : 12 Apr 2023 14:56
Operator : JC/MD
Sample : 02252-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053661.D
Acq On : 12 Apr 2023 14:56
Operator : JC/MD
Sample : 02252-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------