

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053662.D
 Acq On : 12 Apr 2023 15:19
 Operator : JC/MD
 Sample : 02252-08DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	90894	104786	11.36%	1.522%
2	1.909	169	177	199	rVB	78011	112636	12.21%	1.636%
3	2.562	369	380	397	rVB	146179	234906	25.47%	3.411%
4	3.038	520	528	543	rBV4	4282	8331	0.90%	0.121%
5	3.237	587	590	592	rBV	314	260	0.03%	0.004%
6	3.697	732	733	734	rBV	154	51	0.01%	0.001%
7	4.099	856	858	859	rBV	195	93	0.01%	0.001%
8	4.308	921	923	925	rBV	163	66	0.01%	0.001%
9	4.491	977	980	982	rBV	253	146	0.02%	0.002%
10	4.613	1006	1018	1040	rBV	75577	180886	19.61%	2.627%
11	4.951	1121	1123	1124	rBV	299	126	0.01%	0.002%
12	5.057	1141	1156	1180	rBV	152101	327158	35.47%	4.751%
13	5.395	1259	1261	1265	rVB2	430	266	0.03%	0.004%
14	5.417	1265	1268	1269	rBV	193	116	0.01%	0.002%
15	5.719	1341	1362	1370	rBV2	283809	780164	84.58%	11.329%
16	6.054	1463	1466	1467	rBV	310	185	0.02%	0.003%
17	6.063	1467	1469	1471	rVB2	341	166	0.02%	0.002%
18	6.153	1493	1497	1498	rBV	296	191	0.02%	0.003%
19	6.243	1512	1525	1548	rBV	296512	567375	61.51%	8.239%
20	6.481	1597	1599	1601	rBV	200	76	0.01%	0.001%
21	6.526	1601	1613	1626	rVB4	3195	6103	0.66%	0.089%
22	6.578	1626	1629	1631	rBV2	235	165	0.02%	0.002%
23	6.684	1649	1662	1685	rBV	182566	357824	38.79%	5.196%
24	7.057	1774	1778	1780	rBV	185	188	0.02%	0.003%
25	7.076	1780	1784	1786	rVV2	191	169	0.02%	0.002%
26	7.163	1807	1811	1812	rBV	484	271	0.03%	0.004%
27	7.266	1840	1843	1846	rVB	280	143	0.02%	0.002%
28	7.311	1854	1857	1860	rBV	240	213	0.02%	0.003%
29	7.411	1886	1888	1890	rBV	240	103	0.01%	0.001%
30	7.452	1899	1901	1903	rBV	204	116	0.01%	0.002%
31	7.562	1924	1935	1952	rBV	97115	173569	18.82%	2.520%
32	7.793	2005	2007	2014	rVB	348	193	0.02%	0.003%
33	7.848	2022	2024	2025	rBV	169	70	0.01%	0.001%
34	7.893	2026	2038	2060	rVV	361811	628569	68.15%	9.127%
35	8.083	2095	2097	2100	rBV2	226	124	0.01%	0.002%
36	8.173	2114	2125	2147	rBV	71713	122634	13.30%	1.781%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053662.D
 Acq On : 12 Apr 2023 15:19
 Operator : JC/MD
 Sample : 02252-08DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ME4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	8.311	2165	2168	2172	rBV2	276	256	0.03%	0.004%
38	8.353	2179	2181	2182	rBV2	214	99	0.01%	0.001%
39	8.385	2188	2191	2193	rBV	343	230	0.02%	0.003%
40	8.542	2237	2240	2243	rVB2	325	232	0.03%	0.003%
41	8.555	2243	2244	2245	rBB2	113	22	0.00%	0.000%
42	8.571	2245	2249	2250	rBV	265	220	0.02%	0.003%
43	8.626	2255	2266	2294	rBV	230460	413844	44.87%	6.009%
44	8.854	2335	2337	2339	rBV	180	73	0.01%	0.001%
45	8.877	2339	2344	2348	rVV2	377	312	0.03%	0.005%
46	9.414	2498	2511	2515	rBV	427993	699217	75.81%	10.153%
47	9.623	2574	2576	2579	rBV	314	149	0.02%	0.002%
48	9.703	2598	2601	2604	rBV	392	190	0.02%	0.003%
49	9.796	2626	2630	2633	rBV2	276	281	0.03%	0.004%
50	9.902	2660	2663	2666	rBV	269	230	0.02%	0.003%
51	10.343	2797	2800	2802	rBV	327	201	0.02%	0.003%
52	10.468	2833	2839	2844	rVB2	367	396	0.04%	0.006%
53	10.751	2913	2927	2943	rBV	287619	458147	49.67%	6.653%
54	11.041	3013	3017	3018	rBV	205	124	0.01%	0.002%
55	11.745	3229	3236	3243	rBV5	4196	6884	0.75%	0.100%
56	11.809	3244	3256	3280	rVV2	461235	922351	100.00%	13.393%
57	12.189	3361	3374	3397	rBV2	414120	767654	83.23%	11.147%
58	12.545	3482	3485	3487	rBV	361	229	0.02%	0.003%
59	12.635	3509	3513	3514	rBV	474	292	0.03%	0.004%
60	13.053	3640	3643	3645	rBV	285	183	0.02%	0.003%
61	13.844	3881	3889	3897	rBV5	4134	6363	0.69%	0.092%




Sum of corrected areas: 6886617

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053662.D
Acq On : 12 Apr 2023 15:19
Operator : JC/MD
Sample : 02252-08DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

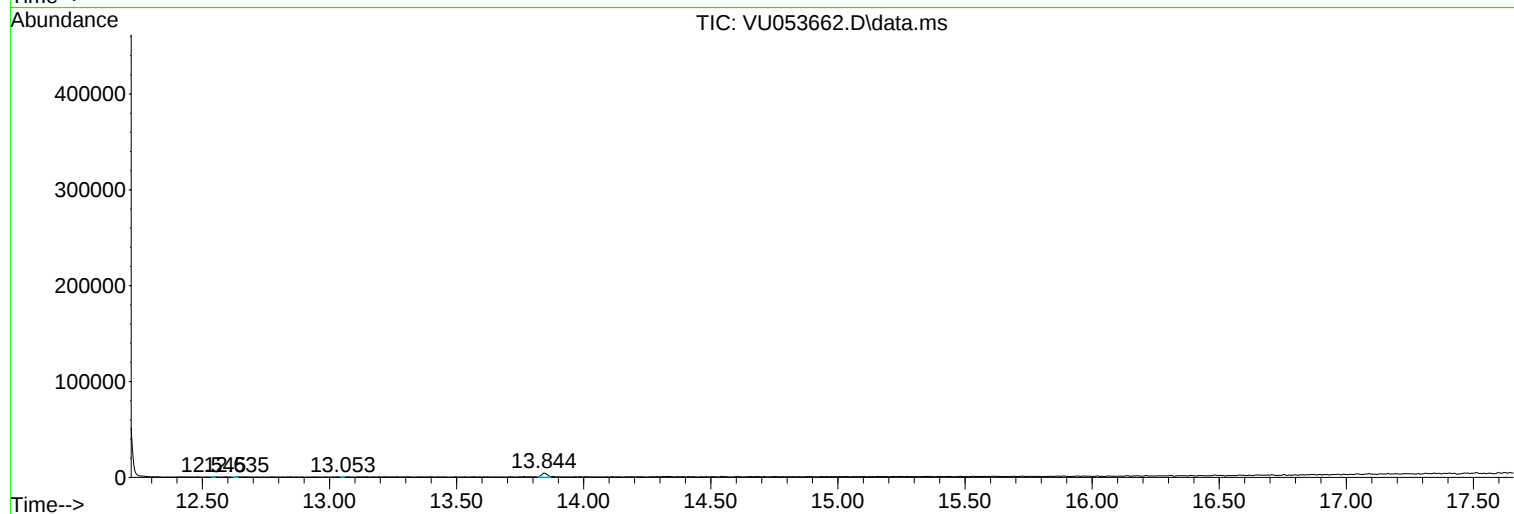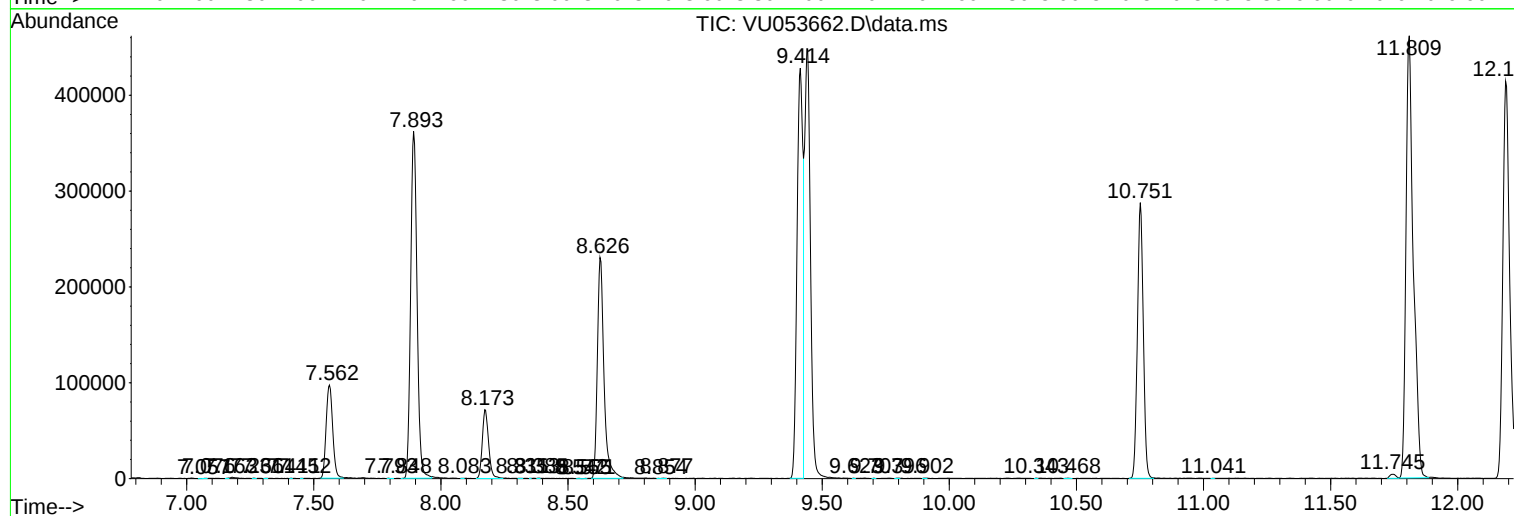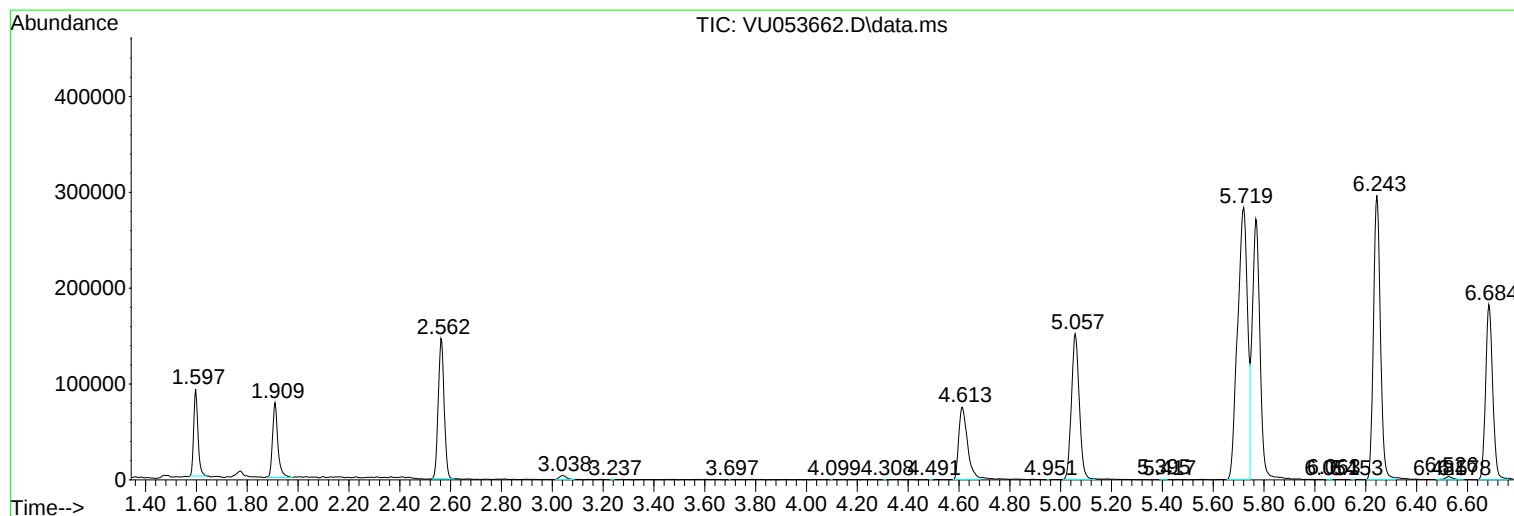

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053662.D
Acq On : 12 Apr 2023 15:19
Operator : JC/MD
Sample : 02252-08DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053662.D
Acq On : 12 Apr 2023 15:19
Operator : JC/MD
Sample : 02252-08DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc