

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053664.D
 Acq On : 12 Apr 2023 16:06
 Operator : JC/MD
 Sample : 02252-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	85478	102144	12.93%	1.625%
2	1.906	169	176	196	rVB	76551	114048	14.44%	1.814%
3	2.562	369	380	398	rVB	144481	233130	29.52%	3.708%
4	2.732	430	433	434	rBV	625	309	0.04%	0.005%
5	3.038	523	528	536	rVB2	1095	1207	0.15%	0.019%
6	3.080	538	541	545	rVB2	263	231	0.03%	0.004%
7	3.186	567	574	578	rVB3	712	921	0.12%	0.015%
8	3.340	620	622	625	rVB	260	140	0.02%	0.002%
9	3.372	628	632	636	rVV2	330	272	0.03%	0.004%
10	3.398	637	640	644	rVB2	216	188	0.02%	0.003%
11	3.530	679	681	685	rVB	338	194	0.02%	0.003%
12	3.565	689	692	694	rBV	241	158	0.02%	0.003%
13	3.919	797	802	809	rVB2	350	368	0.05%	0.006%
14	4.105	855	860	863	rVB	238	197	0.02%	0.003%
15	4.305	919	922	924	rBV	212	168	0.02%	0.003%
16	4.359	936	939	942	rBV	284	214	0.03%	0.003%
17	4.404	949	953	956	rVB	208	188	0.02%	0.003%
18	4.440	960	964	969	rVV	232	244	0.03%	0.004%
19	4.613	1005	1018	1040	rBV	79218	189722	24.02%	3.018%
20	4.845	1087	1090	1093	rVB3	374	271	0.03%	0.004%
21	4.903	1106	1108	1115	rVB3	312	301	0.04%	0.005%
22	4.951	1119	1123	1126	rBB2	425	331	0.04%	0.005%
23	4.980	1126	1132	1135	rBV2	517	370	0.05%	0.006%
24	5.054	1139	1155	1175	rBV	146665	324627	41.11%	5.164%
25	5.282	1224	1226	1230	rBV2	289	230	0.03%	0.004%
26	5.440	1265	1275	1281	rVB2	225	374	0.05%	0.006%
27	5.485	1285	1289	1296	rBV2	315	259	0.03%	0.004%
28	5.584	1316	1320	1327	rVB2	273	260	0.03%	0.004%
29	5.719	1342	1362	1388	rBV2	286639	789726	100.00%	12.561%
30	5.989	1443	1446	1448	rBV	320	201	0.03%	0.003%
31	6.018	1453	1455	1460	rVB	202	140	0.02%	0.002%
32	6.121	1485	1487	1494	rVB2	354	267	0.03%	0.004%
33	6.243	1511	1525	1541	rBV	252684	481925	61.02%	7.666%
34	6.462	1588	1593	1597	rVB2	447	429	0.05%	0.007%
35	6.526	1604	1613	1623	rBV3	2712	4994	0.63%	0.079%
36	6.684	1649	1662	1691	rVV	183882	365253	46.25%	5.810%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053664.D
 Acq On : 12 Apr 2023 16:06
 Operator : JC/MD
 Sample : 02252-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.012	1758	1764	1768	rVB2	217	207	0.03%	0.003%
38	7.095	1784	1790	1793	rBV2	272	354	0.04%	0.006%
39	7.124	1797	1799	1804	rVB2	383	185	0.02%	0.003%
40	7.179	1812	1816	1817	rBV	1426	882	0.11%	0.014%
41	7.231	1828	1832	1835	rVB2	241	181	0.02%	0.003%
42	7.247	1835	1837	1841	rBV	231	159	0.02%	0.003%
43	7.276	1843	1846	1850	rVB2	249	185	0.02%	0.003%
44	7.513	1915	1920	1923	rBV2	213	207	0.03%	0.003%
45	7.562	1923	1935	1952	rBV	100566	178738	22.63%	2.843%
46	7.687	1971	1974	1983	rVV3	1045	1136	0.14%	0.018%
47	7.893	2024	2038	2062	rBV	359636	627104	79.41%	9.975%
48	8.176	2115	2126	2151	rVB2	69916	120788	15.29%	1.921%
49	8.266	2151	2154	2155	rBV2	293	153	0.02%	0.002%
50	8.462	2213	2215	2219	rBV2	263	199	0.03%	0.003%
51	8.520	2228	2233	2236	rBV2	253	244	0.03%	0.004%
52	8.546	2236	2241	2246	rVB2	501	572	0.07%	0.009%
53	8.575	2246	2250	2253	rBV	184	186	0.02%	0.003%
54	8.626	2255	2266	2298	rVV	233042	423403	53.61%	6.735%
55	8.841	2330	2333	2335	rBV2	454	290	0.04%	0.005%
56	8.864	2338	2340	2343	rVV2	252	144	0.02%	0.002%
57	8.883	2343	2346	2349	rVV	200	144	0.02%	0.002%
58	8.912	2353	2355	2360	rVB	267	209	0.03%	0.003%
59	9.083	2403	2408	2411	rBV2	296	328	0.04%	0.005%
60	9.234	2449	2455	2457	rBV2	179	169	0.02%	0.003%
61	9.356	2490	2493	2496	rBV	311	319	0.04%	0.005%
62	9.414	2498	2511	2538	rVV	354204	602716	76.32%	9.587%
63	9.613	2570	2573	2576	rBV2	188	141	0.02%	0.002%
64	9.771	2619	2622	2625	rBV2	201	163	0.02%	0.003%
65	9.822	2630	2638	2640	rBV2	291	340	0.04%	0.005%
66	9.861	2646	2650	2653	rBV	252	209	0.03%	0.003%
67	9.964	2680	2682	2687	rVB2	303	219	0.03%	0.003%
68	9.992	2687	2691	2694	rBV2	225	173	0.02%	0.003%
69	10.012	2694	2697	2705	rBV2	226	301	0.04%	0.005%
70	10.240	2762	2768	2771	rBV2	239	235	0.03%	0.004%
71	10.308	2785	2789	2792	rBV	202	193	0.02%	0.003%
72	10.327	2792	2795	2801	rVB	286	235	0.03%	0.004%
73	10.523	2854	2856	2859	rVB2	223	140	0.02%	0.002%
74	10.751	2915	2927	2947	rVB	294164	470809	59.62%	7.489%
75	10.870	2958	2964	2965	rBV	246	227	0.03%	0.004%
76	10.967	2991	2994	2999	rBV	204	205	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053664.D
 Acq On : 12 Apr 2023 16:06
 Operator : JC/MD
 Sample : 02252-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.996	2999	3003	3006	rVB2	282	252	0.03%	0.004%
78	11.060	3021	3023	3029	rVB2	285	259	0.03%	0.004%
79	11.259	3082	3085	3088	rBV2	228	156	0.02%	0.002%
80	11.385	3120	3124	3128	rBV2	297	258	0.03%	0.004%
81	11.594	3186	3189	3191	rBV2	238	176	0.02%	0.003%
82	11.742	3233	3235	3236	rBV	360	181	0.02%	0.003%
83	11.809	3244	3256	3279	rVV	375131	601866	76.21%	9.573%
84	12.118	3347	3352	3357	rBV2	356	518	0.07%	0.008%
85	12.189	3362	3374	3394	rBV	388754	631646	79.98%	10.047%
86	12.443	3451	3453	3456	rBV	224	138	0.02%	0.002%
87	12.481	3462	3465	3468	rBV2	271	216	0.03%	0.003%
88	12.578	3492	3495	3497	rBV2	243	152	0.02%	0.002%
89	12.767	3551	3554	3558	rVB2	440	281	0.04%	0.004%
90	12.790	3558	3561	3563	rBV2	301	185	0.02%	0.003%
91	12.938	3601	3607	3610	rBV	332	263	0.03%	0.004%
92	13.275	3709	3712	3716	rVV	265	157	0.02%	0.002%
93	13.317	3720	3725	3731	rVB3	480	582	0.07%	0.009%
94	13.365	3737	3740	3742	rBV	268	173	0.02%	0.003%
95	13.452	3762	3767	3770	rBV2	445	459	0.06%	0.007%
96	13.510	3783	3785	3788	rBV2	324	253	0.03%	0.004%
97	13.552	3795	3798	3802	rBV	306	198	0.03%	0.003%
98	13.848	3886	3890	3894	rBV3	1175	1102	0.14%	0.018%
99	14.102	3966	3969	3974	rBV	396	432	0.05%	0.007%
100	14.336	4040	4042	4045	rVB2	456	183	0.02%	0.003%




Sum of corrected areas: 6286879

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053664.D
Acq On : 12 Apr 2023 16:06
Operator : JC/MD
Sample : 02252-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

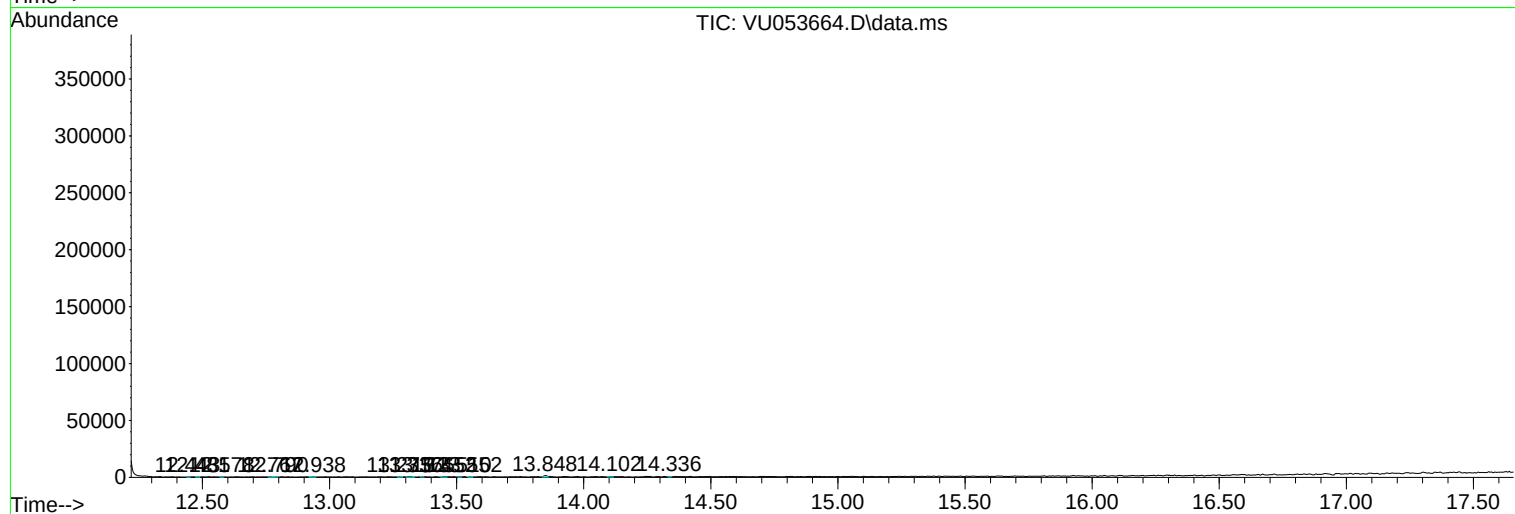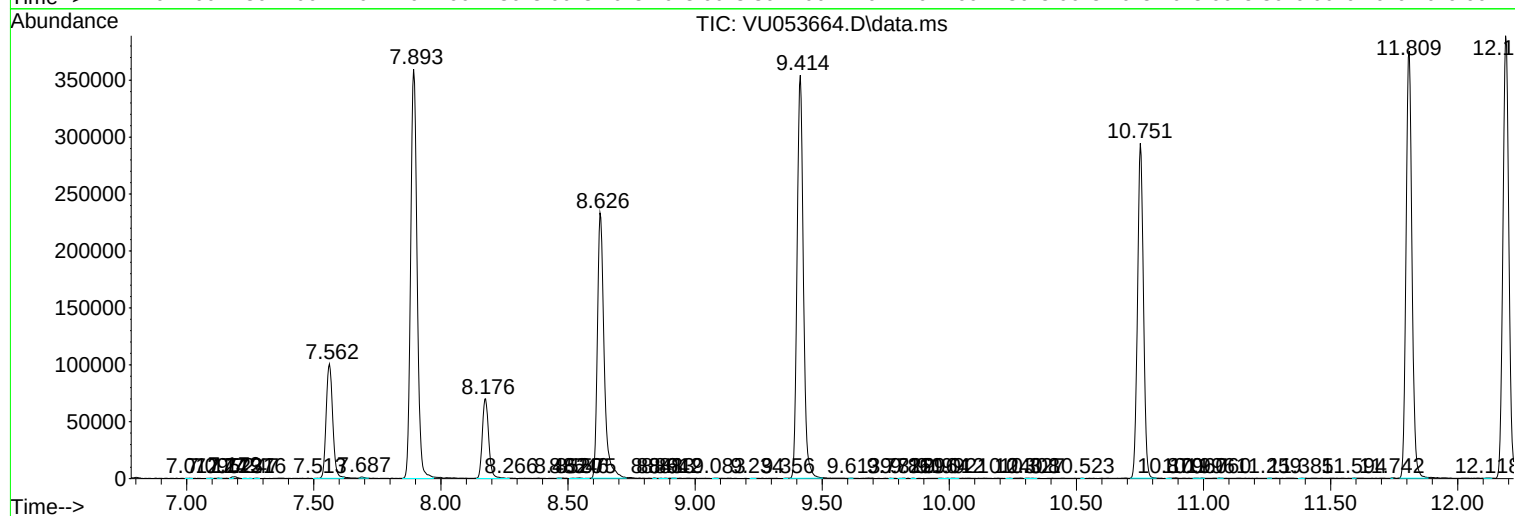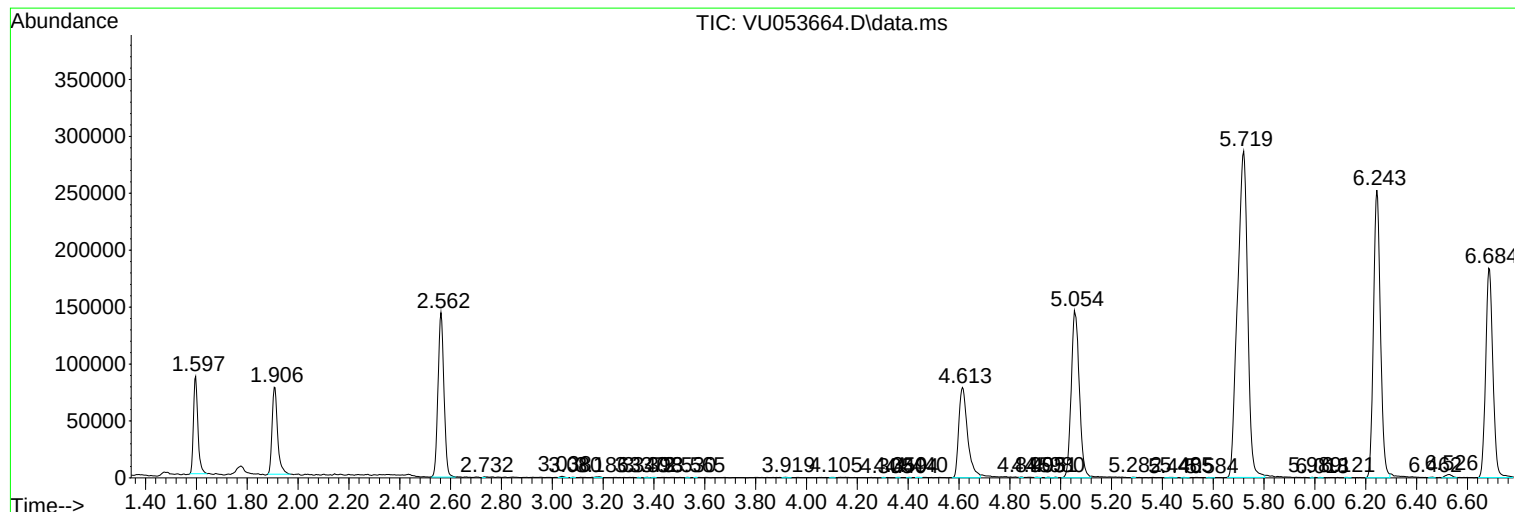

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053664.D
Acq On : 12 Apr 2023 16:06
Operator : JC/MD
Sample : 02252-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053664.D
Acq On : 12 Apr 2023 16:06
Operator : JC/MD
Sample : 02252-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------