

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053670.D
 Acq On : 12 Apr 2023 18:29
 Operator : JC/MD
 Sample : 02252-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	95	rBV	86357	103967	13.65%	1.621%
2	1.909	169	177	196	rVB	73699	108408	14.23%	1.690%
3	2.562	368	380	393	rBV	138870	223915	29.39%	3.491%
4	3.086	539	543	546	rBV2	321	328	0.04%	0.005%
5	3.224	584	586	589	rBV	266	151	0.02%	0.002%
6	3.366	624	630	632	rBV2	240	220	0.03%	0.003%
7	3.382	632	635	638	rBV	266	203	0.03%	0.003%
8	3.433	646	651	654	rBV	288	243	0.03%	0.004%
9	3.533	680	682	686	rVB	228	158	0.02%	0.002%
10	3.604	700	704	709	rBV	248	245	0.03%	0.004%
11	3.694	729	732	735	rBV	429	199	0.03%	0.003%
12	3.813	766	769	778	rBV	360	367	0.05%	0.006%
13	3.851	778	781	783	rBV	187	141	0.02%	0.002%
14	3.989	819	824	827	rBV	272	247	0.03%	0.004%
15	4.118	860	864	866	rBV	210	172	0.02%	0.003%
16	4.208	889	892	895	rBV	228	145	0.02%	0.002%
17	4.231	896	899	901	rVB2	277	145	0.02%	0.002%
18	4.295	915	919	921	rBV2	333	265	0.03%	0.004%
19	4.443	961	965	967	rBV2	285	195	0.03%	0.003%
20	4.475	973	975	977	rBV	507	273	0.04%	0.004%
21	4.523	988	990	993	rBV	323	184	0.02%	0.003%
22	4.613	1006	1018	1044	rBV	77685	188073	24.69%	2.933%
23	4.861	1091	1095	1099	rBV2	433	457	0.06%	0.007%
24	4.893	1103	1105	1108	rBV2	258	158	0.02%	0.002%
25	4.967	1124	1128	1130	rVB2	338	234	0.03%	0.004%
26	4.983	1130	1133	1135	rBV	240	143	0.02%	0.002%
27	5.057	1140	1156	1181	rVV2	148106	319747	41.97%	4.986%
28	5.285	1225	1227	1229	rVV	325	147	0.02%	0.002%
29	5.427	1267	1271	1274	rBV	228	155	0.02%	0.002%
30	5.491	1284	1291	1293	rVB2	237	180	0.02%	0.003%
31	5.510	1293	1297	1301	rBV	303	219	0.03%	0.003%
32	5.597	1321	1324	1331	rVB2	219	160	0.02%	0.002%
33	5.642	1335	1338	1341	rVB	308	193	0.03%	0.003%
34	5.719	1341	1362	1393	rBV2	277045	761872	100.00%	11.880%
35	6.002	1445	1450	1453	rBV2	259	258	0.03%	0.004%
36	6.105	1478	1482	1485	rBV	364	330	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053670.D
 Acq On : 12 Apr 2023 18:29
 Operator : JC/MD
 Sample : 02252-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.243	1512	1525	1546	rBV	293656	558033	73.24%	8.701%
38	6.456	1589	1591	1594	rVV	298	192	0.03%	0.003%
39	6.523	1604	1612	1622	rBV3	2622	4563	0.60%	0.071%
40	6.684	1646	1662	1681	rBV	180891	352373	46.25%	5.494%
41	6.886	1720	1725	1731	rBV3	808	625	0.08%	0.010%
42	6.912	1731	1733	1739	rVB2	217	197	0.03%	0.003%
43	6.944	1739	1743	1746	rVB2	248	212	0.03%	0.003%
44	6.980	1752	1754	1757	rVB	301	146	0.02%	0.002%
45	7.009	1757	1763	1765	rBV	238	208	0.03%	0.003%
46	7.047	1771	1775	1778	rBV	266	183	0.02%	0.003%
47	7.185	1808	1818	1821	rBV4	1390	1860	0.24%	0.029%
48	7.507	1914	1918	1921	rBV	310	240	0.03%	0.004%
49	7.562	1923	1935	1955	rBV	98238	170067	22.32%	2.652%
50	7.645	1960	1961	1969	rVB3	575	428	0.06%	0.007%
51	7.687	1969	1974	1980	rBV4	1130	1436	0.19%	0.022%
52	7.812	2007	2013	2015	rBV2	176	187	0.02%	0.003%
53	7.893	2024	2038	2057	rBV	346812	605369	79.46%	9.439%
54	8.083	2095	2097	2102	rVB	264	181	0.02%	0.003%
55	8.176	2115	2126	2144	rVV	68154	114605	15.04%	1.787%
56	8.320	2168	2171	2173	rBV	206	149	0.02%	0.002%
57	8.353	2176	2181	2183	rVV2	281	202	0.03%	0.003%
58	8.385	2184	2191	2197	rVB2	395	518	0.07%	0.008%
59	8.462	2211	2215	2216	rBV3	292	222	0.03%	0.003%
60	8.513	2229	2231	2237	rBV	232	155	0.02%	0.002%
61	8.575	2247	2250	2253	rBV2	254	204	0.03%	0.003%
62	8.626	2254	2266	2298	rVV	229813	421351	55.30%	6.570%
63	8.790	2312	2317	2319	rBV2	1003	899	0.12%	0.014%
64	8.832	2328	2330	2335	rVB	249	222	0.03%	0.003%
65	8.886	2343	2347	2349	rBV	274	195	0.03%	0.003%
66	9.031	2389	2392	2398	rBV	289	228	0.03%	0.004%
67	9.089	2408	2410	2415	rVB2	256	160	0.02%	0.002%
68	9.169	2432	2435	2439	rVB	289	172	0.02%	0.003%
69	9.208	2444	2447	2449	rVV2	292	183	0.02%	0.003%
70	9.272	2463	2467	2471	rBV	335	219	0.03%	0.003%
71	9.304	2473	2477	2480	rBV2	215	200	0.03%	0.003%
72	9.414	2498	2511	2533	rBV	413043	685549	89.98%	10.690%
73	9.664	2585	2589	2593	rBV2	344	266	0.03%	0.004%
74	9.957	2677	2680	2683	rBV2	277	261	0.03%	0.004%
75	10.015	2694	2698	2707	rVV	313	434	0.06%	0.007%
76	10.073	2713	2716	2718	rBV	403	225	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053670.D
 Acq On : 12 Apr 2023 18:29
 Operator : JC/MD
 Sample : 02252-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.137	2732	2736	2744	rVB2	550	567	0.07%	0.009%
78	10.304	2785	2788	2795	rBV2	281	305	0.04%	0.005%
79	10.664	2898	2900	2906	rVB2	285	213	0.03%	0.003%
80	10.751	2915	2927	2944	rBV	281637	456311	59.89%	7.115%
81	10.854	2956	2959	2965	rVB	254	221	0.03%	0.003%
82	10.886	2965	2969	2970	rBV	439	285	0.04%	0.004%
83	10.915	2975	2978	2982	rBV2	197	158	0.02%	0.002%
84	10.944	2982	2987	2988	rBV	218	185	0.02%	0.003%
85	11.240	3075	3079	3086	rVB2	362	460	0.06%	0.007%
86	11.275	3086	3090	3093	rBV	174	141	0.02%	0.002%
87	11.330	3104	3107	3112	rBV	236	260	0.03%	0.004%
88	11.375	3118	3121	3127	rVB	232	173	0.02%	0.003%
89	11.410	3127	3132	3135	rBV2	362	333	0.04%	0.005%
90	11.713	3223	3226	3227	rBV	296	158	0.02%	0.002%
91	11.748	3232	3237	3242	rVB3	590	588	0.08%	0.009%
92	11.809	3243	3256	3276	rBV	427008	692080	90.84%	10.791%
93	12.041	3325	3328	3331	rBV2	333	242	0.03%	0.004%
94	12.189	3362	3374	3392	rBV	380136	621895	81.63%	9.697%
95	12.555	3485	3488	3492	rBV2	189	176	0.02%	0.003%
96	12.735	3540	3544	3545	rBV	277	210	0.03%	0.003%
97	12.767	3551	3554	3556	rBV	266	161	0.02%	0.003%
98	13.851	3885	3891	3900	rVB4	1020	1385	0.18%	0.022%
99	14.452	4075	4078	4079	rBV	367	242	0.03%	0.004%
100	15.201	4307	4311	4319	rBV2	640	928	0.12%	0.014%




Sum of corrected areas: 6413293

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053670.D
Acq On : 12 Apr 2023 18:29
Operator : JC/MD
Sample : 02252-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

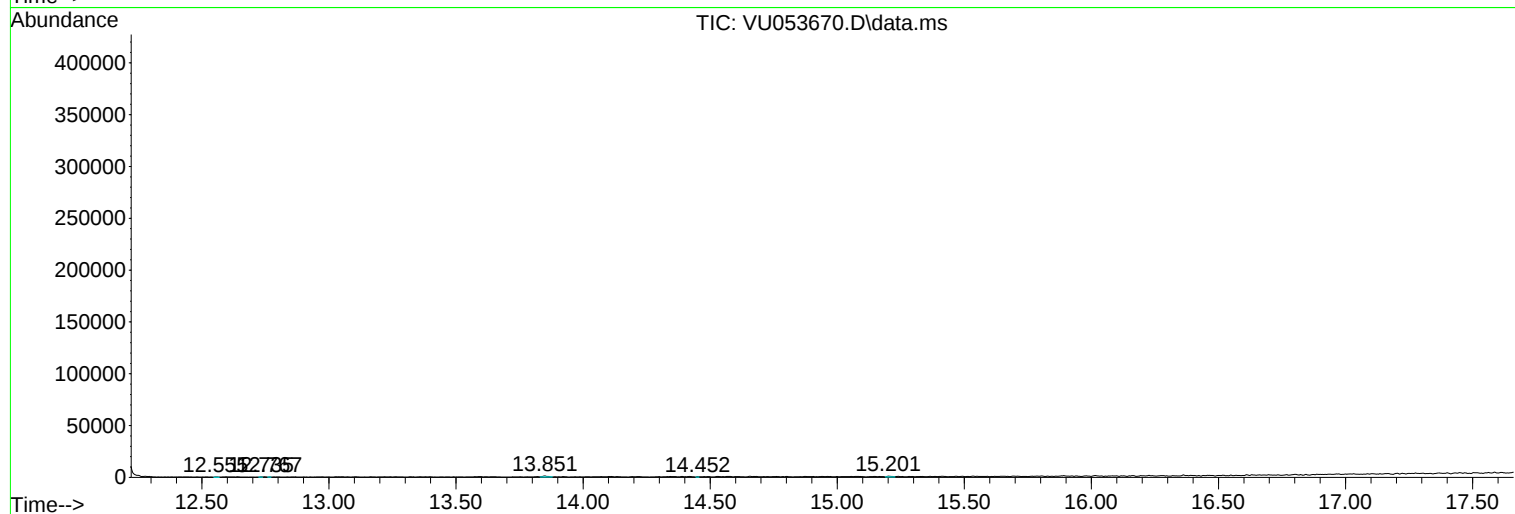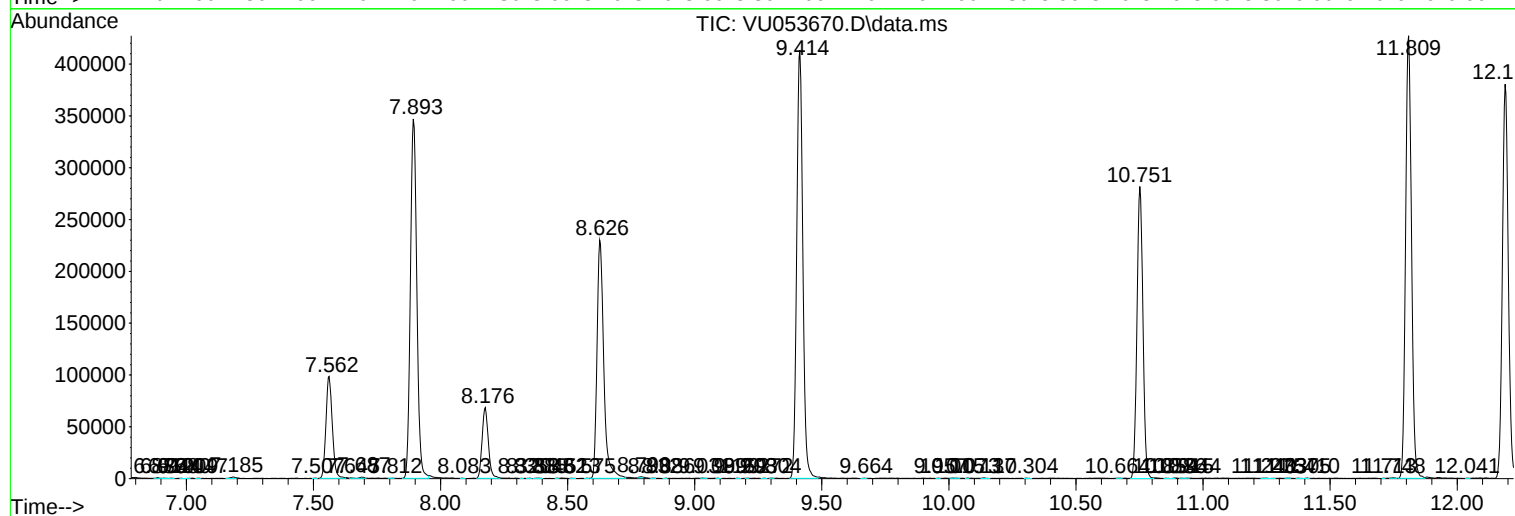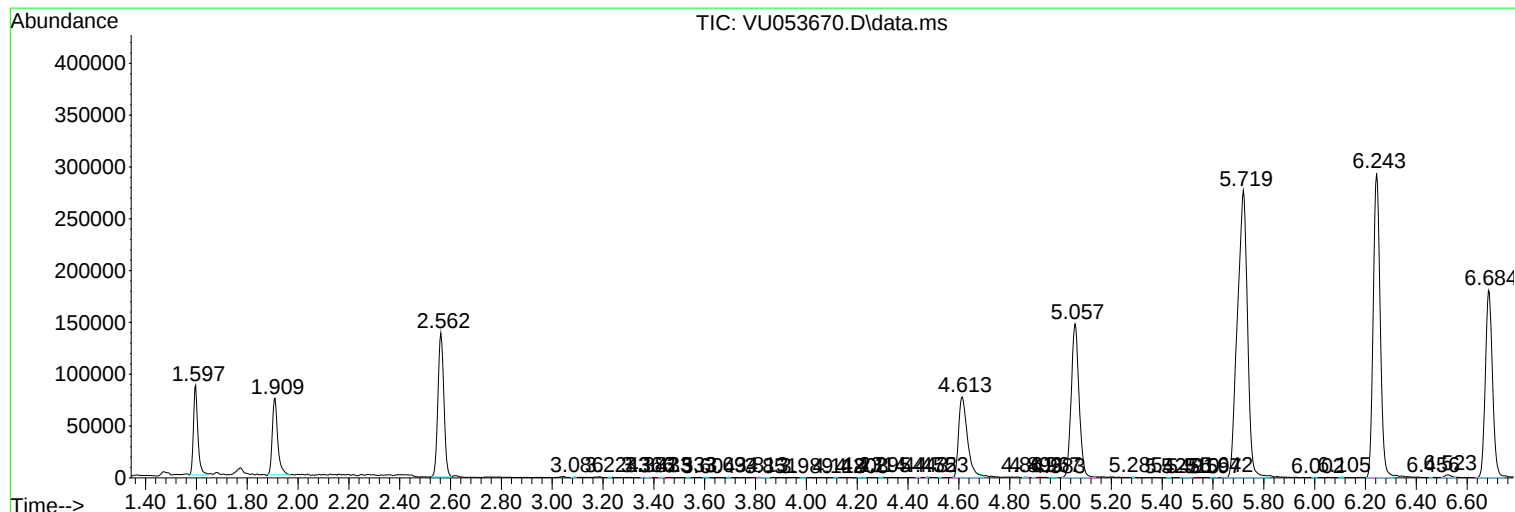

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053670.D
Acq On : 12 Apr 2023 18:29
Operator : JC/MD
Sample : 02252-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053670.D
Acq On : 12 Apr 2023 18:29
Operator : JC/MD
Sample : 02252-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------