

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053672.D
 Acq On : 12 Apr 2023 19:17
 Operator : JC/MD
 Sample : 02252-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	83890	97035	10.91%	1.491%
2	1.909	169	177	193	rBV	70850	101069	11.36%	1.553%
3	2.562	369	380	394	rBV	131685	212938	23.94%	3.271%
4	3.018	520	522	524	rBV2	235	106	0.01%	0.002%
5	3.044	524	530	540	rVB4	1176	1658	0.19%	0.025%
6	3.169	566	569	571	rBV	328	220	0.02%	0.003%
7	3.224	583	586	587	rBV2	205	119	0.01%	0.002%
8	3.266	595	599	601	rBV	255	216	0.02%	0.003%
9	3.353	618	626	636	rBV2	3753	7696	0.87%	0.118%
10	3.523	677	679	682	rBV	246	117	0.01%	0.002%
11	3.796	761	764	766	rBV2	247	179	0.02%	0.003%
12	3.899	794	796	801	rVB2	303	212	0.02%	0.003%
13	4.034	835	838	840	rBV	309	160	0.02%	0.002%
14	4.250	902	905	909	rVB2	265	190	0.02%	0.003%
15	4.301	919	921	923	rVB	201	84	0.01%	0.001%
16	4.359	937	939	945	rVB	299	175	0.02%	0.003%
17	4.613	1006	1018	1039	rBV	73156	172466	19.39%	2.649%
18	4.957	1122	1125	1126	rBV	289	166	0.02%	0.003%
19	4.996	1135	1137	1138	rBV	216	75	0.01%	0.001%
20	5.057	1141	1156	1177	rVV	141179	309092	34.75%	4.748%
21	5.288	1226	1228	1233	rVB2	281	125	0.01%	0.002%
22	5.494	1290	1292	1294	rBV	187	122	0.01%	0.002%
23	5.719	1341	1362	1370	rBV2	261040	722369	81.20%	11.096%
24	6.038	1459	1461	1463	rBV	209	103	0.01%	0.002%
25	6.092	1474	1478	1479	rBV	224	152	0.02%	0.002%
26	6.182	1504	1506	1509	rVB2	204	114	0.01%	0.002%
27	6.243	1509	1525	1542	rBV	295171	559963	62.95%	8.602%
28	6.491	1599	1602	1605	rBV	195	148	0.02%	0.002%
29	6.526	1605	1613	1628	rVB4	4136	7581	0.85%	0.116%
30	6.581	1628	1630	1632	rBV	182	77	0.01%	0.001%
31	6.639	1645	1648	1649	rBV	352	195	0.02%	0.003%
32	6.684	1649	1662	1681	rVV	173111	338152	38.01%	5.194%
33	6.851	1711	1714	1715	rBV	237	128	0.01%	0.002%
34	7.002	1759	1761	1763	rVB	245	101	0.01%	0.002%
35	7.134	1799	1802	1804	rBV	254	178	0.02%	0.003%
36	7.182	1810	1817	1825	rBV4	1250	2098	0.24%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053672.D
 Acq On : 12 Apr 2023 19:17
 Operator : JC/MD
 Sample : 02252-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.259	1838	1841	1843	rBV	184	87	0.01%	0.001%
38	7.292	1849	1851	1854	rBV2	205	119	0.01%	0.002%
39	7.391	1879	1882	1887	rVB	173	143	0.02%	0.002%
40	7.410	1887	1888	1889	rBV	204	47	0.01%	0.001%
41	7.484	1907	1911	1916	rBV2	492	588	0.07%	0.009%
42	7.562	1923	1935	1955	rBV	91887	160209	18.01%	2.461%
43	7.690	1968	1975	1986	rBV4	1038	1838	0.21%	0.028%
44	7.758	1994	1996	1999	rVB	275	121	0.01%	0.002%
45	7.819	2012	2015	2018	rBV2	237	170	0.02%	0.003%
46	7.893	2025	2038	2068	rBV	336598	584689	65.73%	8.981%
47	8.172	2115	2125	2144	rBV	65900	110648	12.44%	1.700%
48	8.336	2171	2176	2179	rVB	272	229	0.03%	0.004%
49	8.507	2226	2229	2233	rBV	293	219	0.02%	0.003%
50	8.542	2239	2240	2241	rBV	322	120	0.01%	0.002%
51	8.626	2255	2266	2294	rBV	214926	392419	44.11%	6.028%
52	8.899	2348	2351	2352	rBV	154	103	0.01%	0.002%
53	8.906	2352	2353	2358	rVB2	242	166	0.02%	0.003%
54	9.012	2383	2386	2387	rBV	154	62	0.01%	0.001%
55	9.021	2387	2389	2392	rVB	194	104	0.01%	0.002%
56	9.050	2395	2398	2402	rBV	297	206	0.02%	0.003%
57	9.414	2497	2511	2513	rBV	439017	573909	64.52%	8.816%
58	9.639	2579	2581	2583	rBV	141	87	0.01%	0.001%
59	9.664	2585	2589	2595	rVV4	445	490	0.06%	0.008%
60	9.713	2601	2604	2607	rBV2	290	205	0.02%	0.003%
61	9.867	2649	2652	2656	rBV	207	210	0.02%	0.003%
62	10.124	2726	2732	2734	rBV	506	377	0.04%	0.006%
63	10.217	2757	2761	2767	rVB2	369	370	0.04%	0.006%
64	10.259	2772	2774	2777	rBV	279	117	0.01%	0.002%
65	10.340	2797	2799	2803	rBV2	273	182	0.02%	0.003%
66	10.668	2899	2901	2905	rBV	233	138	0.02%	0.002%
67	10.751	2915	2927	2953	rBV	270867	437575	49.19%	6.722%
68	10.886	2966	2969	2971	rBV	538	343	0.04%	0.005%
69	10.947	2984	2988	2992	rVB2	277	249	0.03%	0.004%
70	11.037	3012	3016	3019	rBV	271	232	0.03%	0.004%
71	11.169	3052	3057	3060	rBV	443	461	0.05%	0.007%
72	11.459	3144	3147	3152	rBV2	257	268	0.03%	0.004%
73	11.523	3163	3167	3172	rBV2	258	215	0.02%	0.003%
74	11.568	3179	3181	3182	rBV2	242	114	0.01%	0.002%
75	11.651	3204	3207	3210	rBV	389	248	0.03%	0.004%
76	11.741	3227	3235	3244	rBV3	15554	23734	2.67%	0.365%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053672.D
 Acq On : 12 Apr 2023 19:17
 Operator : JC/MD
 Sample : 02252-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	11.809	3244	3256	3260	rBV	477512	783989	88.13%	12.043%
78	11.954	3299	3301	3303	rBV	428	180	0.02%	0.003%
79	12.192	3362	3375	3399	rBV3	411739	889571	100.00%	13.665%
80	12.992	3621	3624	3627	rVB2	504	333	0.04%	0.005%
81	13.330	3725	3729	3734	rBV3	383	353	0.04%	0.005%
82	13.555	3797	3799	3803	rBB	226	99	0.01%	0.002%
83	13.703	3842	3845	3849	rBV2	381	368	0.04%	0.006%
84	13.786	3869	3871	3874	rBV	331	203	0.02%	0.003%
85	13.844	3882	3889	3896	rBV4	5270	7471	0.84%	0.115%
86	14.262	4017	4019	4020	rBV	245	70	0.01%	0.001%




Sum of corrected areas: 6510027

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053672.D
Acq On : 12 Apr 2023 19:17
Operator : JC/MD
Sample : 02252-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

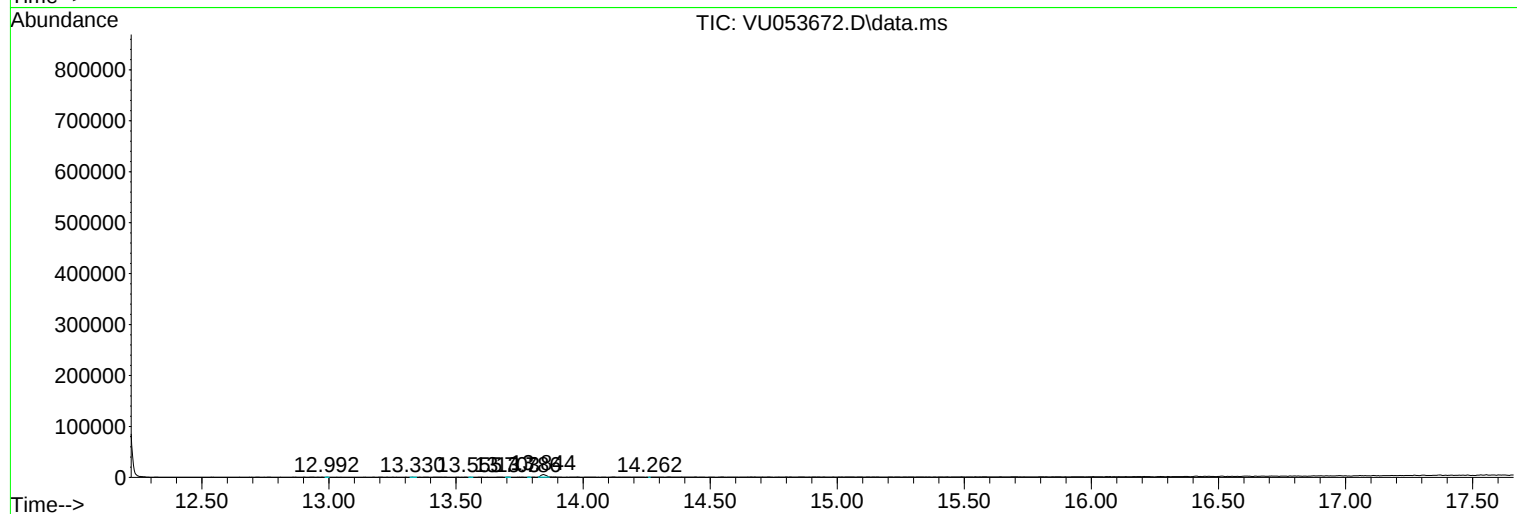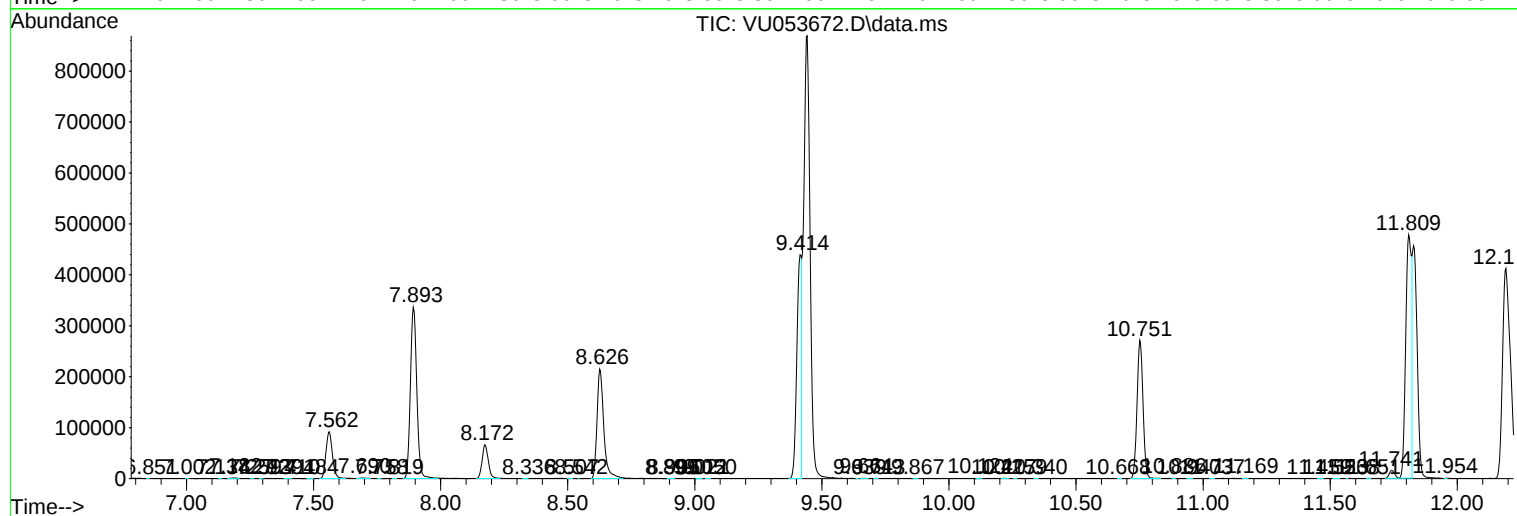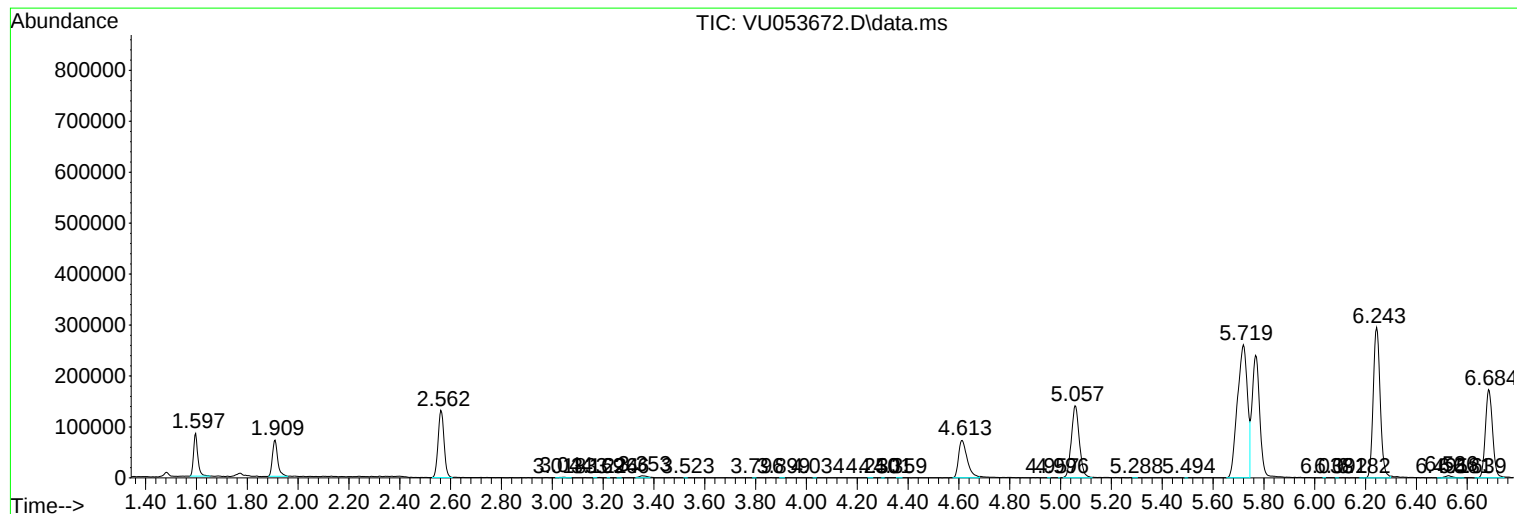

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053672.D
Acq On : 12 Apr 2023 19:17
Operator : JC/MD
Sample : 02252-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053672.D
Acq On : 12 Apr 2023 19:17
Operator : JC/MD
Sample : 02252-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------