

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053673.D
 Acq On : 12 Apr 2023 19:41
 Operator : JC/MD
 Sample : 02252-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	82572	110714	12.48%	1.673%
2	1.909	171	177	192	rVB	71589	100025	11.27%	1.512%
3	2.562	369	380	396	rVB	136531	221460	24.96%	3.347%
4	3.034	523	527	528	rBV2	779	512	0.06%	0.008%
5	3.169	565	569	574	rBV3	443	484	0.05%	0.007%
6	3.649	715	718	725	rBV	299	226	0.03%	0.003%
7	3.957	811	814	817	rVB	231	114	0.01%	0.002%
8	3.977	817	820	821	rBV	170	78	0.01%	0.001%
9	4.076	847	851	854	rBV	280	200	0.02%	0.003%
10	4.160	875	877	882	rVB	280	115	0.01%	0.002%
11	4.231	897	899	901	rBV	240	158	0.02%	0.002%
12	4.533	989	993	995	rBV2	361	328	0.04%	0.005%
13	4.613	1006	1018	1040	rBV	77235	184565	20.80%	2.789%
14	5.057	1140	1156	1177	rBV2	139232	312703	35.24%	4.726%
15	5.276	1222	1224	1229	rVB2	563	457	0.05%	0.007%
16	5.616	1327	1330	1332	rBV	359	298	0.03%	0.005%
17	5.719	1341	1362	1371	rBV3	274993	755450	85.13%	11.417%
18	5.980	1440	1443	1445	rBV2	132	95	0.01%	0.001%
19	6.086	1474	1476	1479	rBV	176	62	0.01%	0.001%
20	6.111	1479	1484	1486	rBV2	388	303	0.03%	0.005%
21	6.195	1509	1510	1511	rBV2	102	26	0.00%	0.000%
22	6.243	1511	1525	1543	rBV	292440	554363	62.47%	8.378%
23	6.529	1607	1614	1623	rVB3	1002	1649	0.19%	0.025%
24	6.687	1649	1663	1680	rBV	174123	346995	39.10%	5.244%
25	6.986	1754	1756	1757	rVB	258	76	0.01%	0.001%
26	7.063	1779	1780	1783	rBV	190	83	0.01%	0.001%
27	7.137	1800	1803	1808	rVB	302	204	0.02%	0.003%
28	7.185	1809	1818	1823	rBV3	1609	2273	0.26%	0.034%
29	7.391	1879	1882	1886	rBV	247	153	0.02%	0.002%
30	7.427	1891	1893	1898	rBV	160	64	0.01%	0.001%
31	7.562	1923	1935	1960	rBV	96354	167962	18.93%	2.538%
32	7.690	1969	1975	1979	rBV3	1030	1329	0.15%	0.020%
33	7.893	2025	2038	2062	rBV	348618	602491	67.89%	9.106%
34	8.079	2094	2096	2100	rBV3	403	283	0.03%	0.004%
35	8.131	2109	2112	2115	rBV	348	290	0.03%	0.004%
36	8.176	2115	2126	2145	rVV2	68754	114152	12.86%	1.725%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
 Data File : VU053673.D
 Acq On : 12 Apr 2023 19:41
 Operator : JC/MD
 Sample : 02252-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	8.308	2164	2167	2172	rVB2	274	274	0.03%	0.004%
38	8.343	2175	2178	2183	rVB2	216	201	0.02%	0.003%
39	8.369	2183	2186	2190	rBV2	296	195	0.02%	0.003%
40	8.529	2233	2236	2240	rBV2	314	324	0.04%	0.005%
41	8.626	2255	2266	2297	rBV	233809	421472	47.50%	6.370%
42	8.828	2327	2329	2330	rBV	254	65	0.01%	0.001%
43	8.841	2330	2333	2337	rVB2	262	158	0.02%	0.002%
44	8.989	2377	2379	2382	rVB	290	114	0.01%	0.002%
45	9.002	2382	2383	2386	rBV	120	49	0.01%	0.001%
46	9.066	2401	2403	2405	rBV	170	78	0.01%	0.001%
47	9.124	2420	2421	2422	rBB	65	31	0.00%	0.000%
48	9.217	2447	2450	2452	rBV	263	217	0.02%	0.003%
49	9.272	2465	2467	2468	rBV	168	53	0.01%	0.001%
50	9.414	2497	2511	2513	rBV	435611	568872	64.11%	8.598%
51	9.725	2607	2608	2609	rVB	175	34	0.00%	0.001%
52	9.838	2640	2643	2644	rBV	236	112	0.01%	0.002%
53	9.915	2664	2667	2669	rBV	241	132	0.01%	0.002%
54	10.018	2696	2699	2704	rBV2	235	233	0.03%	0.004%
55	10.102	2722	2725	2728	rVB	337	194	0.02%	0.003%
56	10.124	2730	2732	2733	rBV	222	68	0.01%	0.001%
57	10.590	2874	2877	2881	rVB	275	148	0.02%	0.002%
58	10.613	2882	2884	2887	rBV	193	103	0.01%	0.002%
59	10.751	2914	2927	2946	rBV	296109	462677	52.14%	6.993%
60	10.918	2977	2979	2981	rBV	175	86	0.01%	0.001%
61	11.021	3008	3011	3012	rBV	197	94	0.01%	0.001%
62	11.108	3035	3038	3044	rVB	352	231	0.03%	0.003%
63	11.314	3099	3102	3105	rBV	251	125	0.01%	0.002%
64	11.349	3110	3113	3116	rVB2	308	177	0.02%	0.003%
65	11.745	3227	3236	3244	rBV2	13804	19693	2.22%	0.298%
66	11.809	3244	3256	3260	rBV	478171	762339	85.91%	11.521%
67	12.192	3362	3375	3395	rBV4	429061	887401	100.00%	13.412%
68	12.397	3435	3439	3440	rBV	313	222	0.03%	0.003%
69	12.764	3551	3553	3556	rVB	386	134	0.02%	0.002%
70	12.851	3578	3580	3583	rBV2	283	126	0.01%	0.002%
71	12.970	3614	3617	3621	rVB	225	131	0.01%	0.002%
72	12.999	3621	3626	3627	rBV	301	297	0.03%	0.004%
73	13.127	3662	3666	3668	rBV	302	251	0.03%	0.004%
74	13.712	3844	3848	3851	rBV2	459	367	0.04%	0.006%
75	13.844	3882	3889	3899	rVB4	5368	7751	0.87%	0.117%
76	13.989	3933	3934	3936	rBV4	335	165	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053673.D
Acq On : 12 Apr 2023 19:41
Operator : JC/MD
Sample : 02252-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	14.616	4126	4129	4133	rBV2	583	552	0.06%	0.008%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 6616686

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053673.D
Acq On : 12 Apr 2023 19:41
Operator : JC/MD
Sample : 02252-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

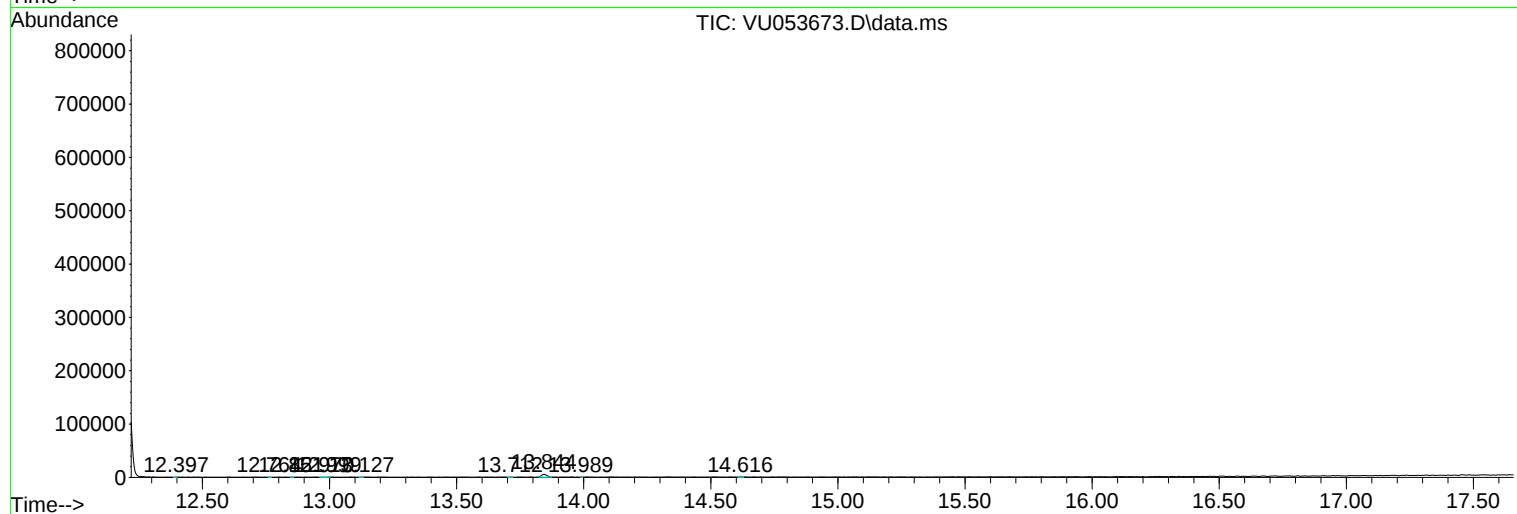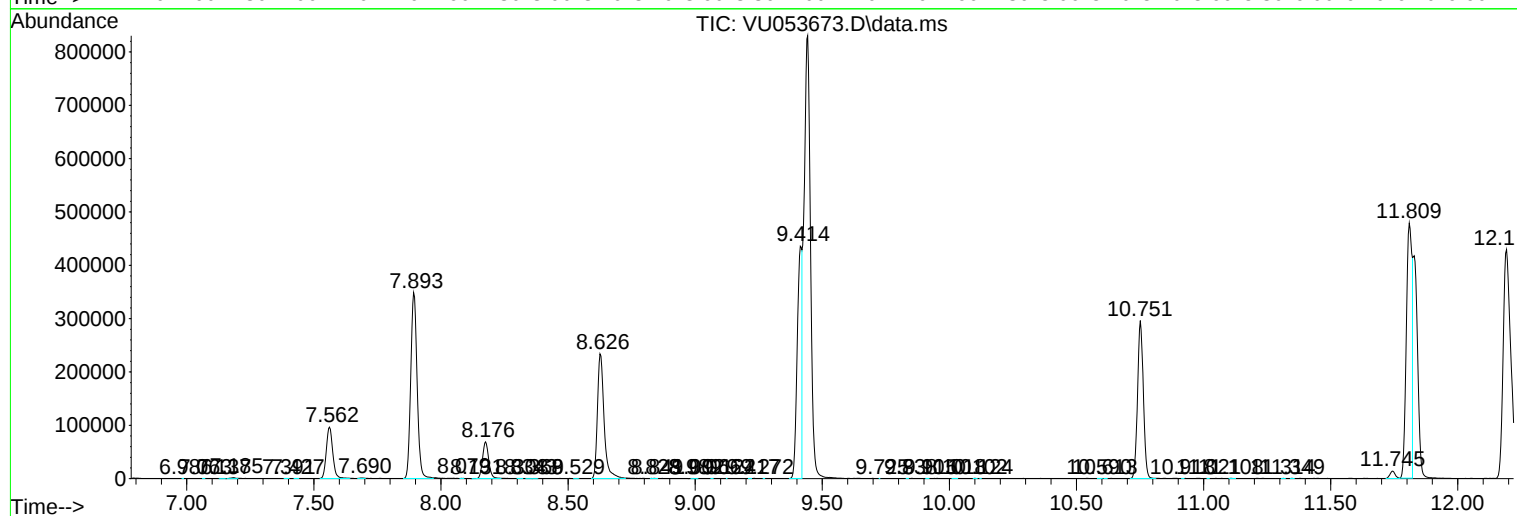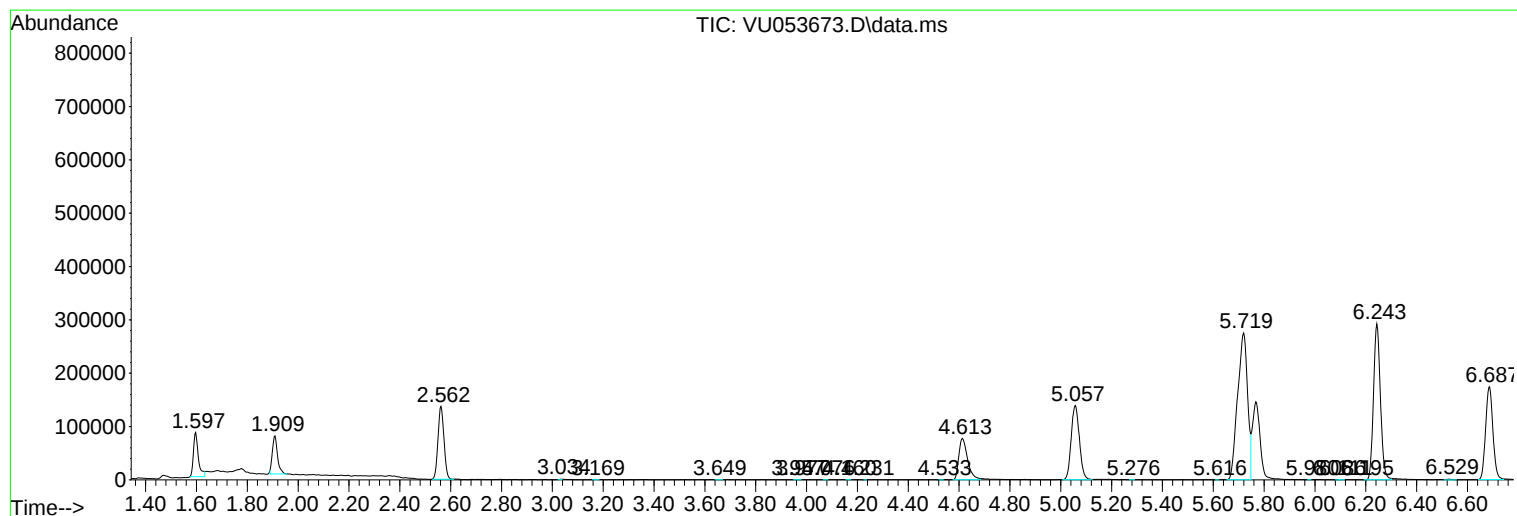

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053673.D
Acq On : 12 Apr 2023 19:41
Operator : JC/MD
Sample : 02252-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053673.D
Acq On : 12 Apr 2023 19:41
Operator : JC/MD
Sample : 02252-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------