
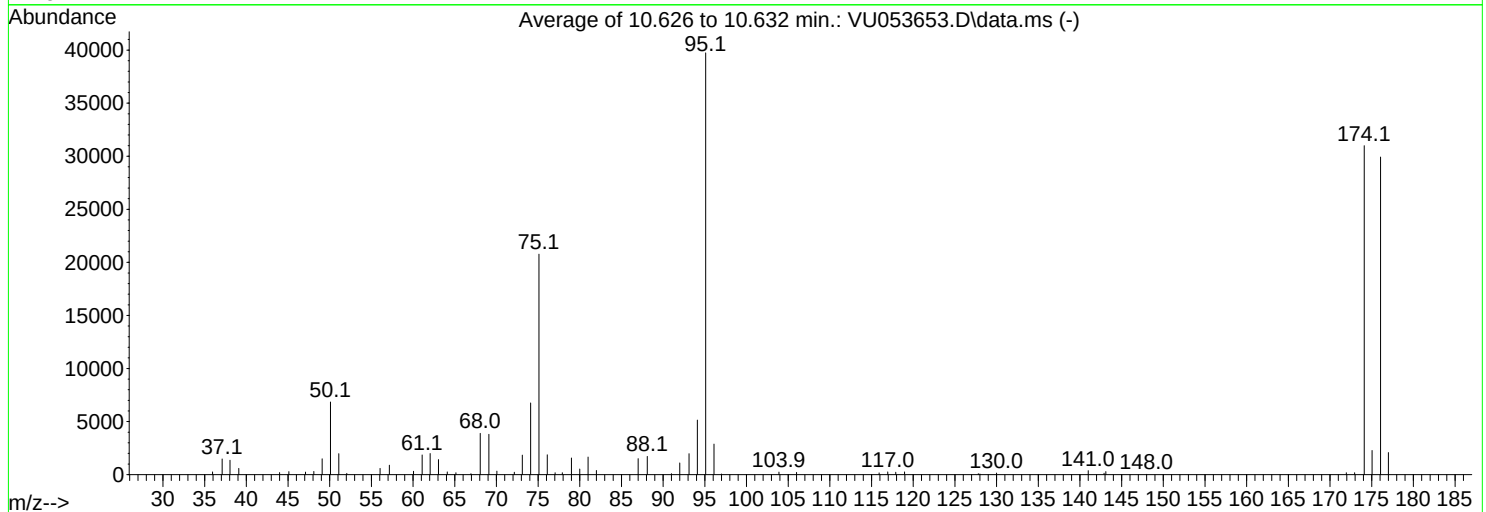


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041223\
Data File : VU053653.D
Acq On : 12 Apr 2023 09:00
Operator : JC/MD
Sample : BFB179
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB179

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis
Last Update : Thu Apr 13 01:39:36 2023

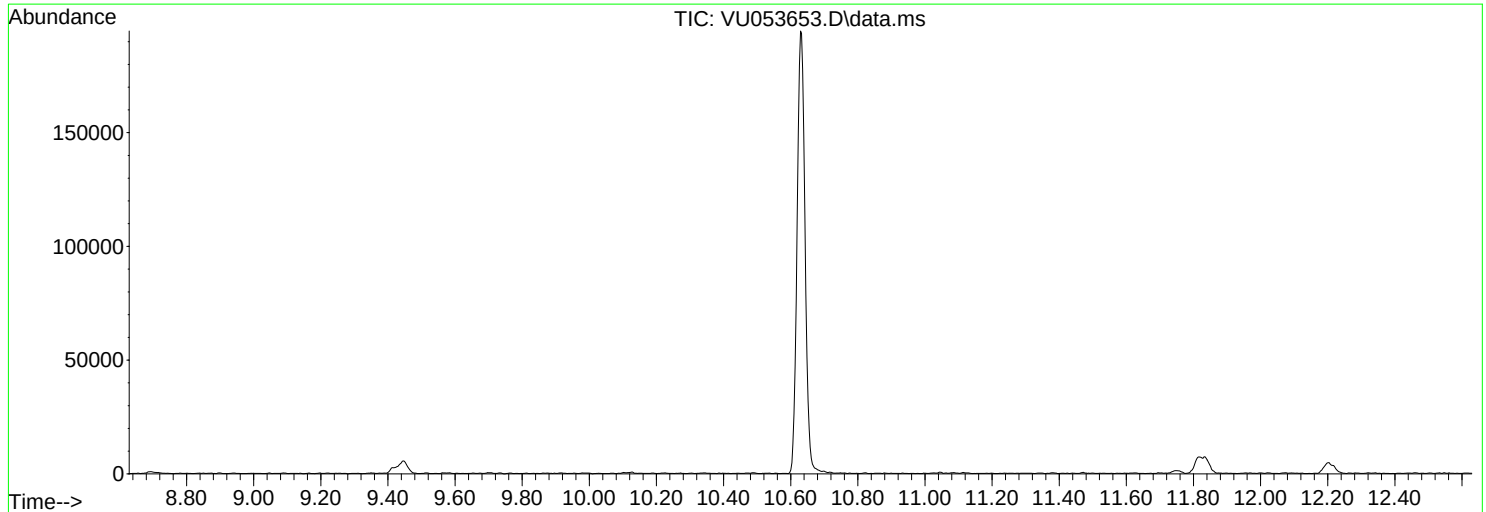

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	6845	PASS
75	95	30	80	52.3	20768	PASS
95	95	100	100	100.0	39741	PASS
96	95	5	9	7.3	2886	PASS
173	174	0.00	2	0.6	178	PASS
174	95	50	120	78.0	30989	PASS
175	174	5	9	7.3	2275	PASS
176	174	95	101	96.6	29920	PASS
177	176	5	9	6.9	2079	PASS

m/z	Abundance
43.90	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB179

m/z	Abundance
35.90	265.0
37.10	1389.0
38.10	1277.0
39.10	569.0
44.00	400.0
45.10	320.0
47.00	239.0
48.10	310.0
49.10	1492.0
50.10	6347.0
51.10	1987.0
52.00	116.0
56.10	575.0
57.20	814.0
60.10	344.0
61.10	1924.0
62.10	1906.0
63.10	1252.0
64.10	259.0
65.10	180.0
68.00	3802.0
69.10	3686.0
70.00	291.0
72.10	221.0
73.10	1798.0
74.10	6461.0
75.10	20032.0
76.10	1731.0
77.00	173.0
77.90	140.0
79.00	1398.0
80.00	496.0
81.00	1577.0
82.00	406.0
87.00	1352.0
88.10	1702.0
92.00	1088.0
93.10	1793.0
94.10	4882.0
95.10	37592.0
96.10	2761.0
103.90	238.0
106.00	196.0
115.90	177.0
116.90	197.0
117.90	311.0
119.00	235.0
127.80	139.0
130.00	105.0
141.00	333.0
142.90	402.0
172.00	160.0
172.90	143.0
174.10	29408.0
175.10	2064.0
176.10	28184.0
177.00	1943.0

Instrument :
MSVOA_U
ClientSampleId :
BFB179

m/z	Abundance
36.00	259.0
37.10	1527.0
38.00	1387.0
39.10	620.0
44.10	369.0
45.10	299.0
47.10	231.0
48.10	324.0
49.10	1542.0
50.10	7078.0
51.10	1965.0
52.10	138.0
56.10	621.0
57.10	910.0
60.10	309.0
61.10	1903.0
62.00	2066.0
63.00	1455.0
64.10	287.0
65.10	175.0
66.90	115.0
68.00	3985.0
69.10	3896.0
70.10	352.0
72.10	233.0
73.10	1924.0
74.10	6907.0
75.10	21440.0
76.10	1930.0
77.10	181.0
77.90	192.0
79.00	1601.0
80.00	535.0
81.00	1725.0
82.00	410.0
87.00	1529.0
88.10	1767.0
91.00	127.0
92.00	1160.0
93.10	2109.0
94.10	5321.0
95.10	40904.0
96.10	2989.0
97.00	102.0
103.90	251.0
106.00	209.0
115.90	165.0
117.00	262.0
117.90	236.0
119.00	265.0
127.80	151.0
130.00	152.0
141.00	384.0
143.10	404.0
148.00	102.0
172.00	185.0
173.00	177.0
174.10	31656.0
175.00	2357.0
176.10	30624.0
177.00	2162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB179

m/z	Abundance
36.00	264.0
37.10	1499.0
38.00	1409.0
39.10	566.0
44.10	356.0
45.10	266.0
47.20	251.0
48.10	294.0
49.10	1436.0
50.10	7111.0
51.10	1975.0
52.10	110.0
56.00	578.0
57.10	952.0
60.00	294.0
61.10	1741.0
62.00	2012.0
63.00	1559.0
64.10	248.0
65.20	213.0
67.00	166.0
68.10	3884.0
69.10	3808.0
70.10	342.0
72.20	212.0
73.10	1812.0
74.10	6913.0
75.10	20832.0
76.10	1940.0
77.10	194.0
77.90	217.0
79.00	1718.0
80.00	572.0
81.00	1664.0
82.00	370.0
87.00	1657.0
88.10	1701.0
91.00	163.0
92.00	1033.0
93.10	2024.0
94.10	5227.0
95.10	40728.0
96.10	2907.0
97.00	102.0
103.90	228.0
106.00	216.0
115.90	151.0
117.00	331.0
117.90	129.0
118.90	274.0
128.00	161.0
130.00	189.0
141.00	405.0
143.10	447.0
171.90	190.0
173.00	215.0
174.10	31904.0
175.00	2405.0
176.00	30952.0
177.00	2133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB179