

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041224\
 Data File : VU058669.D
 Acq On : 12 Apr 2024 21:43
 Operator : MD/SY
 Sample : VU0412WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Apr 13 01:05:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 23:43:07 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	70951	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	68545	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	28210	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	20069	4.272	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.400%
7) Chloroethane-d5	1.904	69	20002	4.900	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.000%
11) 1,1-Dichloroethene-d2	2.560	65	10104	4.752	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.000%
20) 2-Butanone-d5	4.621	46	51885	52.413	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.820%
24) Chloroform-d	5.052	84	48925	5.217	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.400%
26) 1,2-Dichloroethane-d4	5.695	65	24477	5.593	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.800%
32) Benzene-d6	5.721	84	91361	4.951	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
36) 1,2-Dichloropropane-d6	6.682	67	31481	5.440	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.800%
41) Toluene-d8	7.891	98	74546	4.555	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%
43) trans-1,3-Dichloroprop...	8.177	79	8729	4.859	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.200%
46) 2-Hexanone-d5	8.630	63	36180	48.829	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.660%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	19668	4.814	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	23858	5.021	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.400%
Target Compounds						
					Qvalue	
35) Methylcyclohexane	6.685	83	6326	0.670	ug/L #	16
37) 1,2-Dichloropropane	6.682	63	3388	0.518	ug/L #	90
61) 1,2,3-Trichloropropane	11.807	75	4290	1.490	ug/L #	70
71) Naphthalene	14.113	128	1301	0.166	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041224\
Data File : VU058669.D
Acq On : 12 Apr 2024 21:43
Operator : MD/SY
Sample : VU0412WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Apr 13 01:05:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 23:43:07 2024
Response via : Initial Calibration

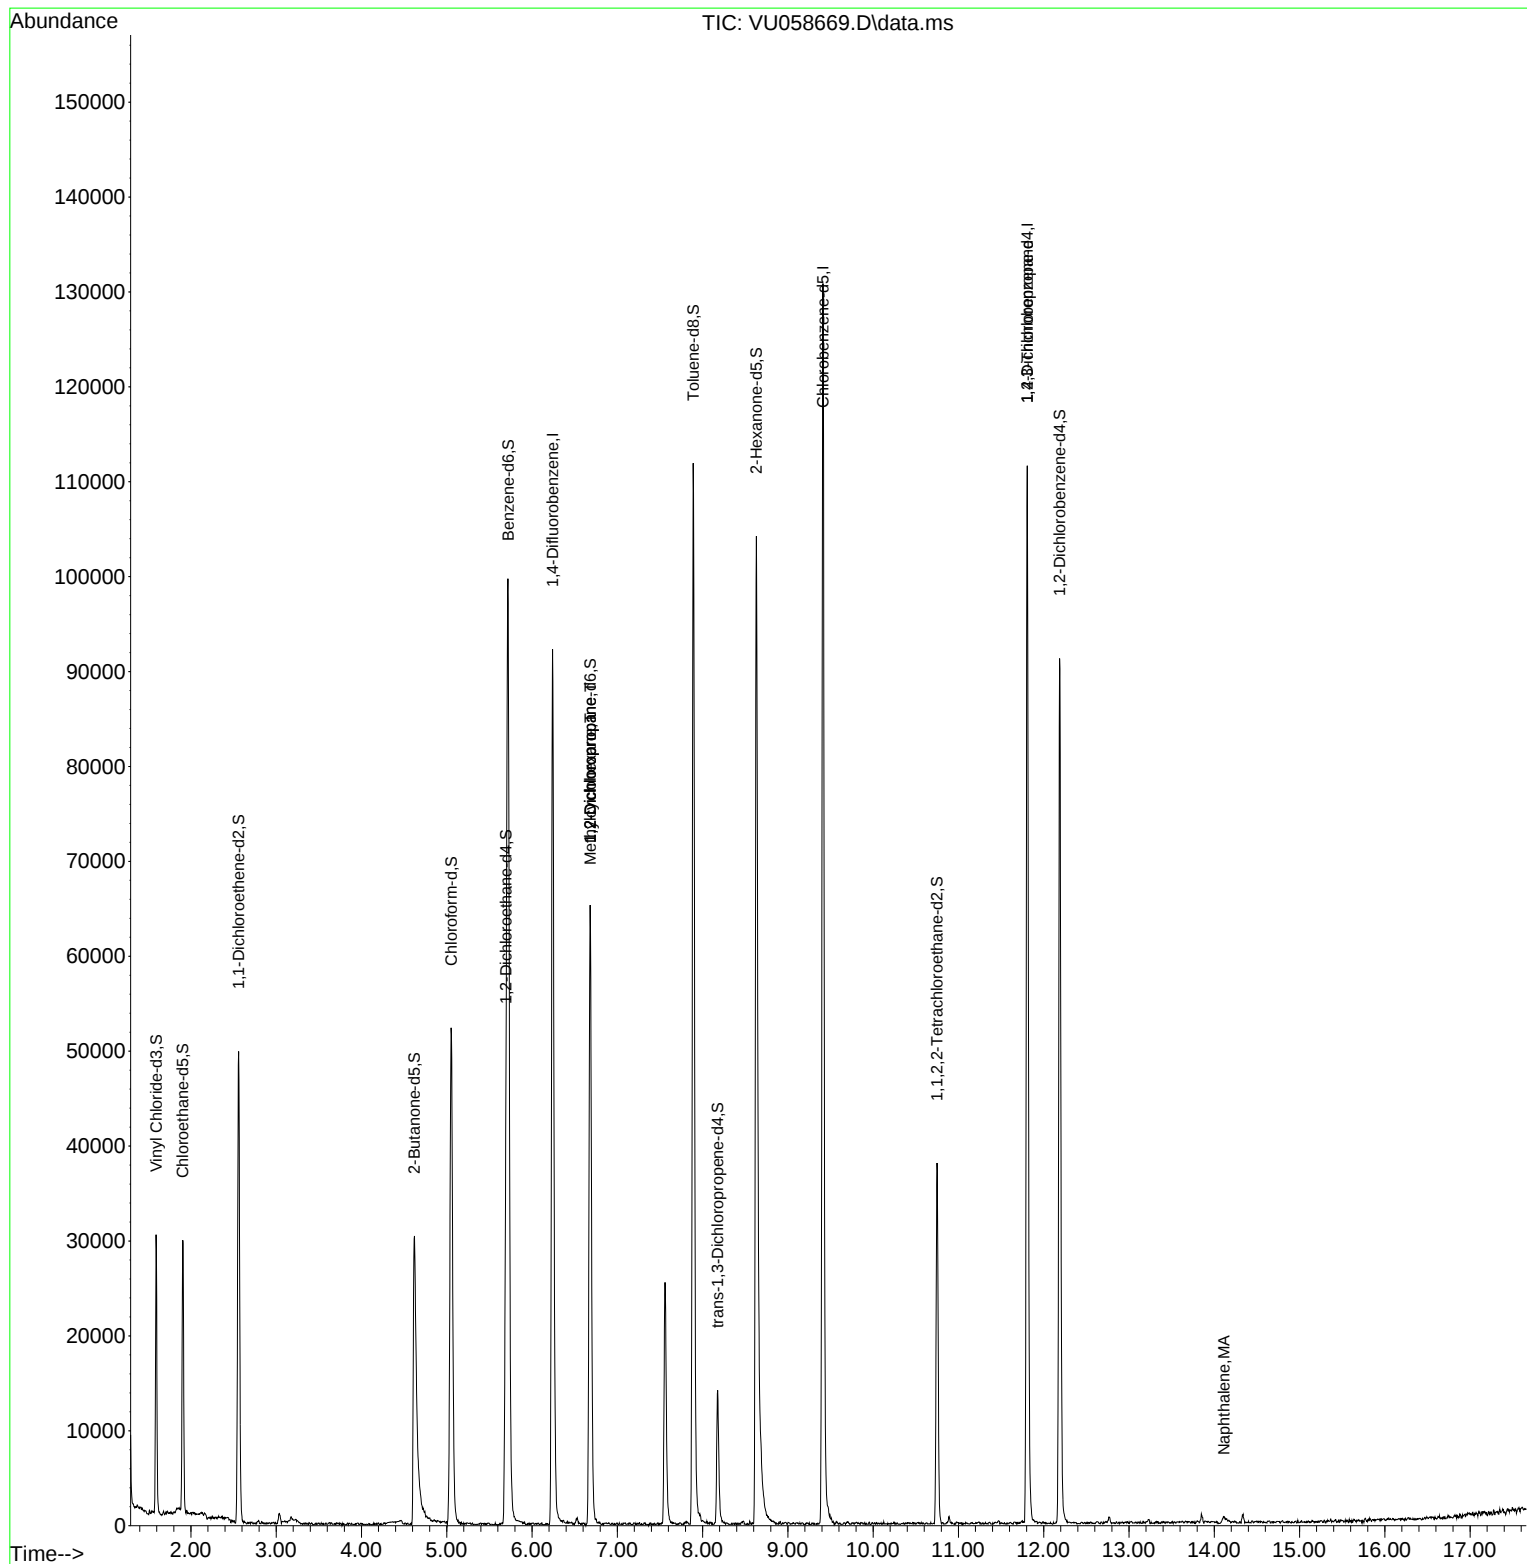

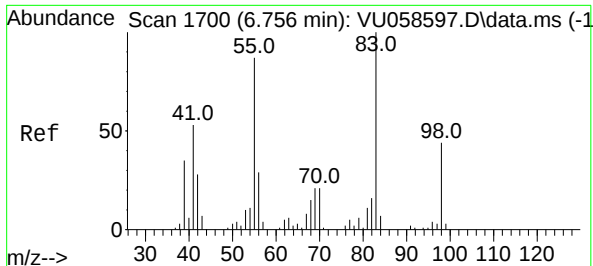

#35

Methylcyclohexane

Concen: 0.670 ug/L

RT: 6.685 min Scan# 1

Delta R.T. -0.071 min

Lab File: VU058669.D

Acq: 12 Apr 2024 21:43

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 83 Resp: 6326

Ion Ratio Lower Upper

83 100

55 0.0 66.2 99.4#

98 0.0 34.6 52.0#

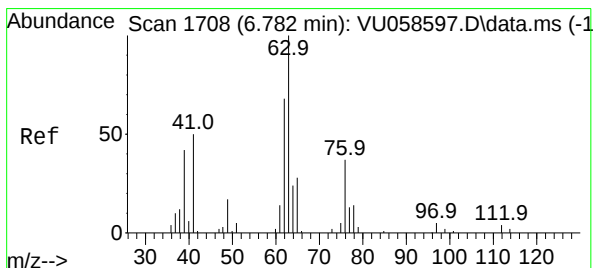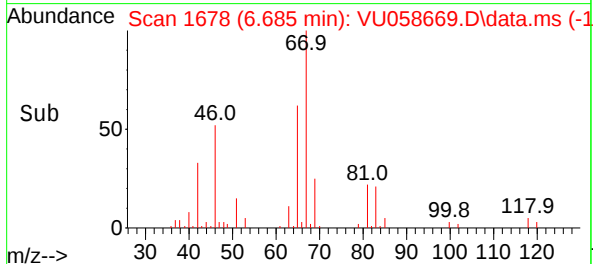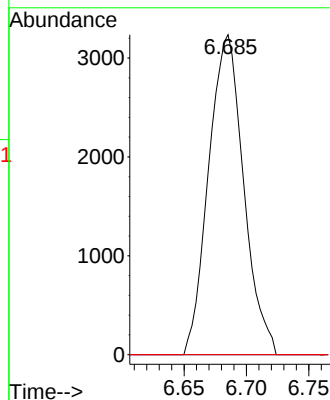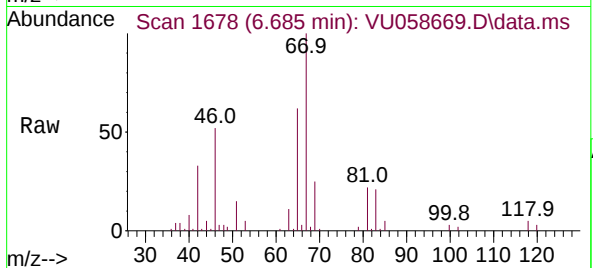

#37

1,2-Dichloropropane

Concen: 0.518 ug/L

RT: 6.682 min Scan# 1677

Delta R.T. -0.100 min

Lab File: VU058669.D




Acq: 12 Apr 2024 21:43


Tgt Ion: 63 Resp: 3388

Ion Ratio Lower Upper

63 100

112 0.0 2.6 4.0#

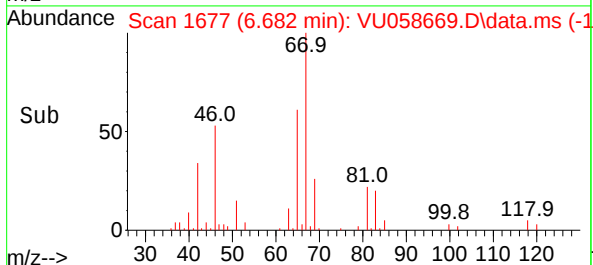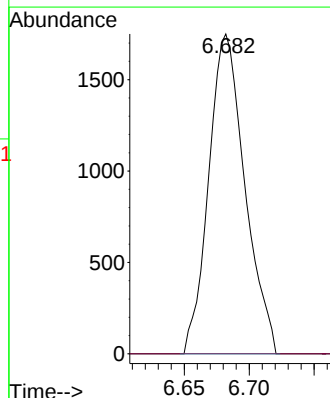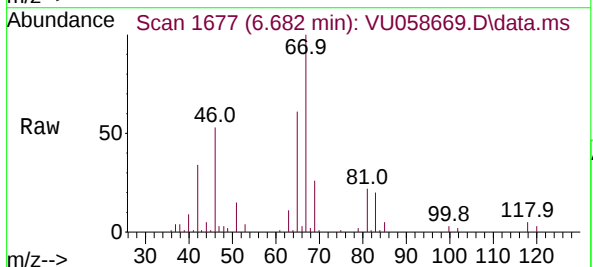

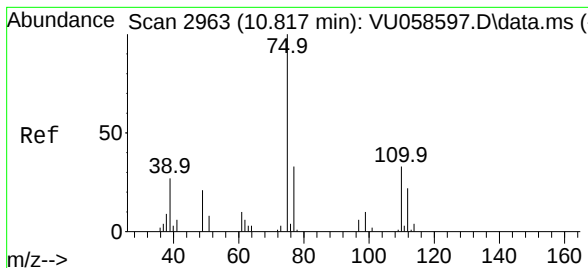

#61

1,2,3-Trichloropropane

Concen: 1.490 ug/L

RT: 11.807 min Scan# 31

Delta R.T. 0.990 min

Lab File: VU058669.D

Acq: 12 Apr 2024 21:43

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 75 Resp: 4290

Ion Ratio Lower Upper

75 100

110 0.0 25.8 38.6#

77 30.9 25.1 37.7

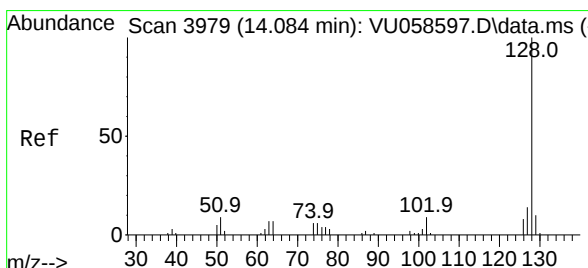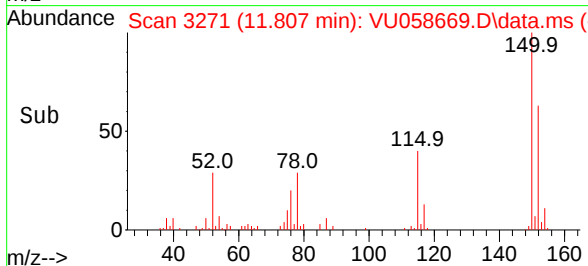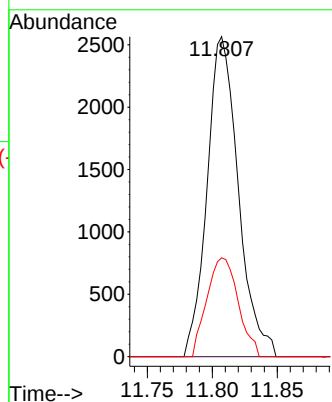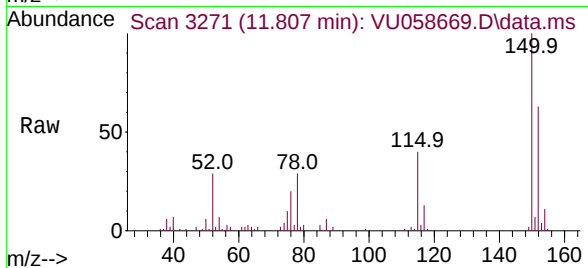

#71

Naphthalene

Concen: 0.166 ug/L

RT: 14.113 min Scan# 3988

Delta R.T. 0.029 min

Lab File: VU058669.D

Acq: 12 Apr 2024 21:43

Tgt Ion: 128 Resp: 1301

Ion Ratio Lower Upper

128 100

129 0.0 8.6 13.0#

127 0.0 11.0 16.6#

