


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041224\
Data File : VU058641.D
Acq On : 12 Apr 2024 09:17
Operator : MD/SY
Sample : BFB142
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB142

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Apr 12 23:43:07 2024

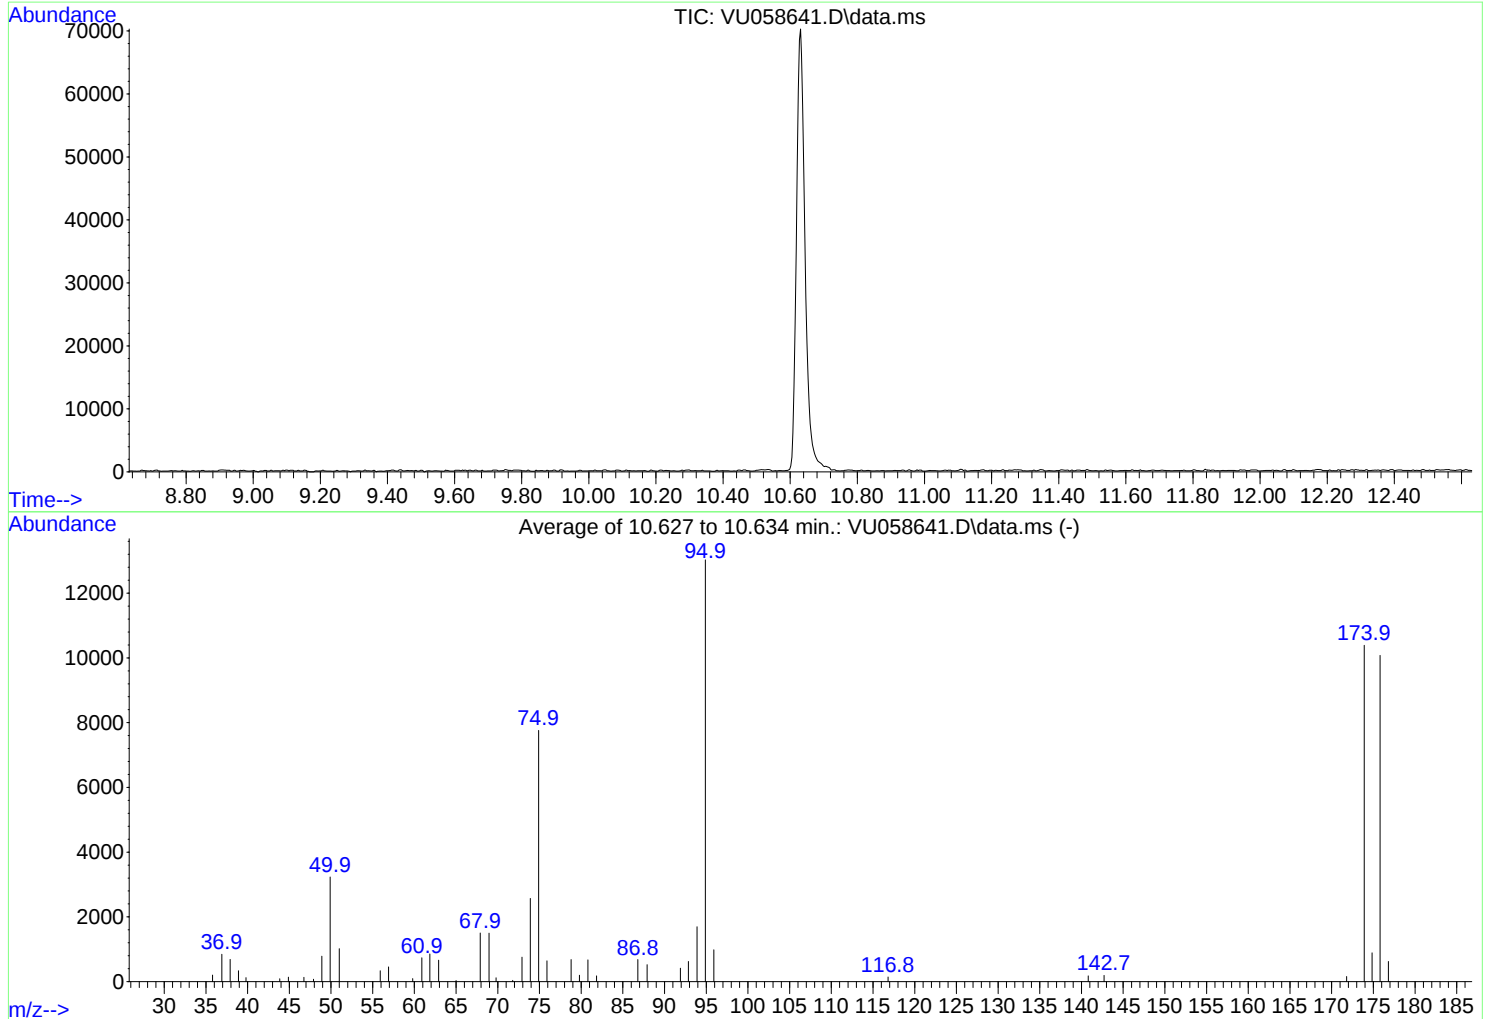

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.8	3234	PASS
75	95	30	80	59.6	7761	PASS
95	95	100	100	100.0	13029	PASS
96	95	5	9	7.5	983	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.8	10391	PASS
175	174	5	9	8.6	890	PASS
176	174	95	101	97.0	10079	PASS
177	176	5	9	6.2	623	PASS

m/z	Abundance
43.90	243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB142

m/z	Abundance
35.80	203.0
36.90	864.0
37.90	695.0
38.90	325.0
39.80	134.0
43.90	330.0
44.90	149.0
46.80	165.0
48.90	810.0
49.90	3287.0
51.00	1087.0
55.90	328.0
56.90	446.0
60.90	782.0
61.90	825.0
62.90	655.0
65.00	103.0
67.90	1599.0
68.90	1543.0
69.80	129.0
72.90	783.0
73.90	2539.0
74.90	7809.0
75.90	664.0
78.80	678.0
79.80	190.0
80.80	678.0
81.90	195.0
86.80	627.0
87.90	542.0
91.90	423.0
92.90	676.0
93.90	1663.0
94.90	13082.0
95.90	1022.0
116.80	145.0
140.80	181.0
142.70	176.0
171.80	140.0
173.90	10353.0
174.90	890.0
175.80	9997.0
176.80	630.0

Instrument :
MSVOA_U
ClientSampleId :
BFB142

m/z	Abundance
35.80	213.0
36.90	859.0
37.90	689.0
38.90	343.0
39.80	131.0
43.90	328.0
44.90	135.0
46.70	121.0
47.90	108.0
48.90	820.0
49.90	3362.0
51.00	1041.0
55.90	358.0
56.90	475.0
59.80	133.0
60.90	743.0
61.90	886.0
62.90	675.0
67.90	1560.0
68.90	1511.0
69.80	123.0
72.90	783.0
73.90	2637.0
74.90	8030.0
75.90	656.0
78.80	688.0
79.80	212.0
80.80	703.0
81.90	179.0
86.80	730.0
87.90	531.0
91.90	425.0
92.90	632.0
93.90	1743.0
94.90	13364.0
95.90	1015.0
116.80	152.0
140.80	185.0
142.70	209.0
171.80	160.0
173.90	10643.0
174.80	946.0
175.80	10402.0
176.80	652.0

Instrument :
MSVOA_U
ClientSampleId :
BFB142

m/z	Abundance
35.80	192.0
36.90	818.0
37.90	676.0
38.90	336.0
39.80	114.0
43.80	331.0
44.90	132.0
46.80	109.0
47.90	116.0
48.90	735.0
49.90	3054.0
51.00	924.0
55.90	321.0
56.90	446.0
59.80	152.0
60.90	693.0
61.80	847.0
62.90	654.0
67.90	1350.0
69.00	1445.0
69.80	101.0
71.80	113.0
72.90	704.0
73.90	2533.0
74.90	7445.0
75.90	615.0
78.80	675.0
79.80	198.0
80.80	635.0
81.80	163.0
86.80	683.0
87.90	498.0
91.90	395.0
92.80	565.0
93.90	1677.0
94.90	12641.0
95.90	913.0
116.80	138.0
140.80	165.0
142.70	201.0
171.80	172.0
173.90	10176.0
174.90	835.0
175.80	9839.0
176.80	587.0

Instrument :
MSVOA_U
ClientSampleId :
BFB142