
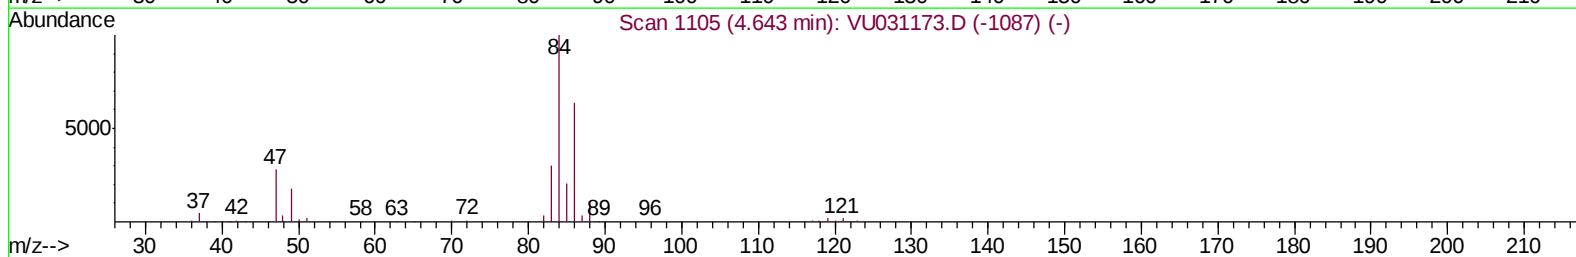
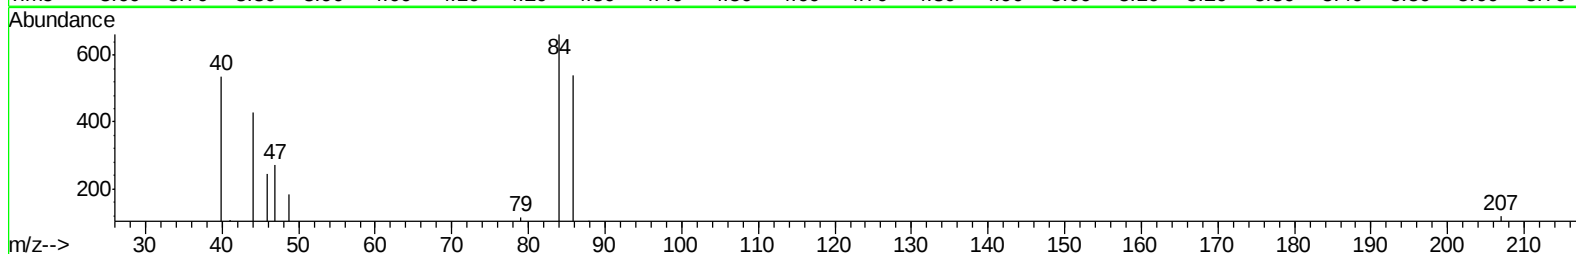


Data File : VU031191.D
Acq On : 14 Apr 2019 05:32
Operator : JC/SP
Sample : K2409-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Apr 15 01:43:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 15 01:39:53 2019
Response via : Initial Calibration

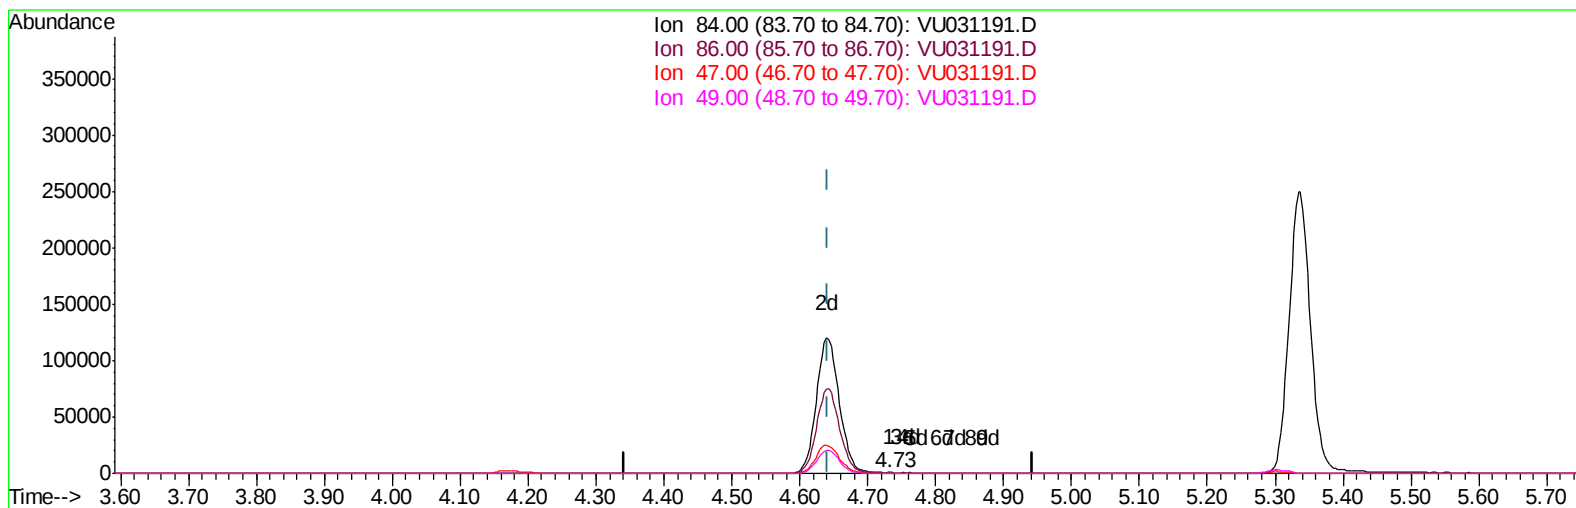

TIC: VU031191.D

(24) Chloroform-d (S)

4.733min (+0.090) 0.09ug/L

response 519

Ion	Exp%	Act%
84.00	100	100
86.00	62.90	57.23
47.00	47.00	46.63
49.00	26.80	20.04