
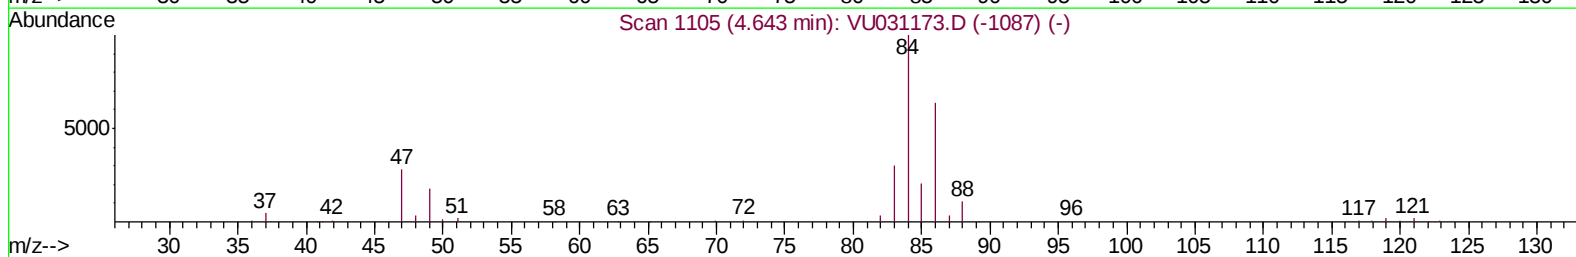
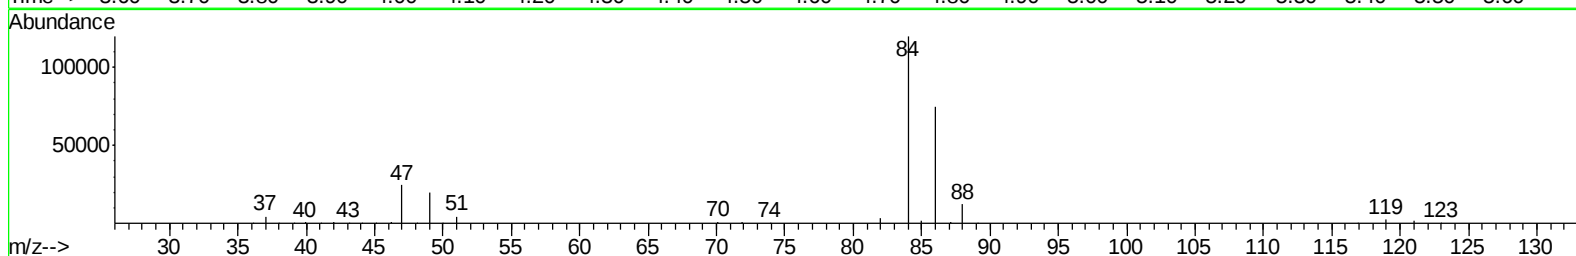


Data File : VU031191.D
Acq On : 14 Apr 2019 05:32
Operator : JC/SP
Sample : K2409-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Apr 15 03:55:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 15 01:39:53 2019
Response via : Initial Calibration

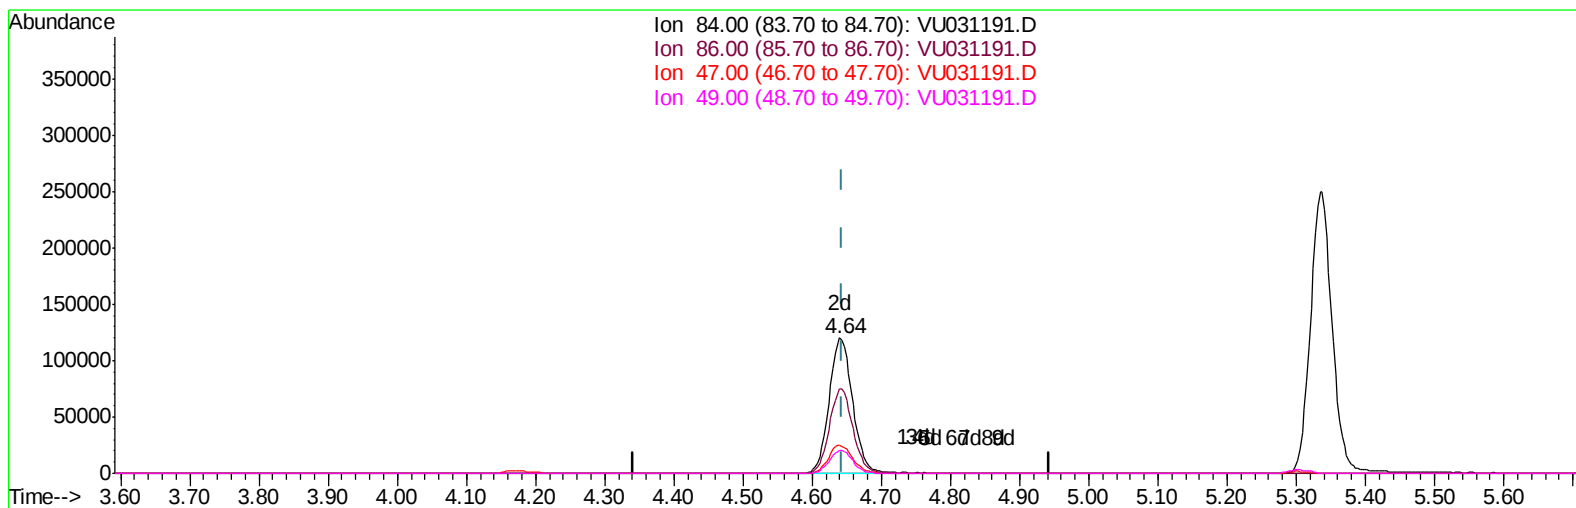

TIC: VU031191.D

(24) Chloroform-d (S)

4.640min (-0.003) 50.49ug/L m

response 281106

Ion	Exp%	Act%
84.00	100	100
86.00	62.90	0.11#
47.00	47.00	0.09#
49.00	26.80	0.04#