

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031171.D
 Acq On : 13 Apr 2019 20:54
 Operator : JC/SP
 Sample : K2353-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETJ63

Quant Time: Apr 15 11:55:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 22:25:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	481593	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	470595	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	185661	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	175212	40.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.52%
7) Chloroethane-d5	1.68	69	146535	44.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.82%
11) 1,1-Dichloroethene-d2	2.27	63	246921	31.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.52%
21) 2-Butanone-d5	4.17	46	332948	97.72	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.72%
24) Chloroform-d	4.64	84	314500	47.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.78%
26) 1,2-Dichloroethane-d4	5.31	65	215048	47.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.98%
32) Benzene-d6	5.33	84	640181	46.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.33	67	220109	46.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.50%
41) Toluene-d8	7.56	98	548058	45.01	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.02%
43) trans-1,3-Dichloropropene-	7.85	79	92345	43.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.02%
47) 2-Hexanone-d5	8.31	63	192098	89.27	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.27%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	308128	48.52	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.04%
64) 1,2-Dichlorobenzene-d4	11.86	152	193060	52.87	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.74%


Target Compounds					Ovalue
20) cis-1,2-Dichloroethene	4.22	96	535305	137.156 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031171.D
Acq On : 13 Apr 2019 20:54
Operator : JC/SP
Sample : K2353-07 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
ETJ63

Quant Time: Apr 15 11:55:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 22:25:59 2019
Response via : Initial Calibration

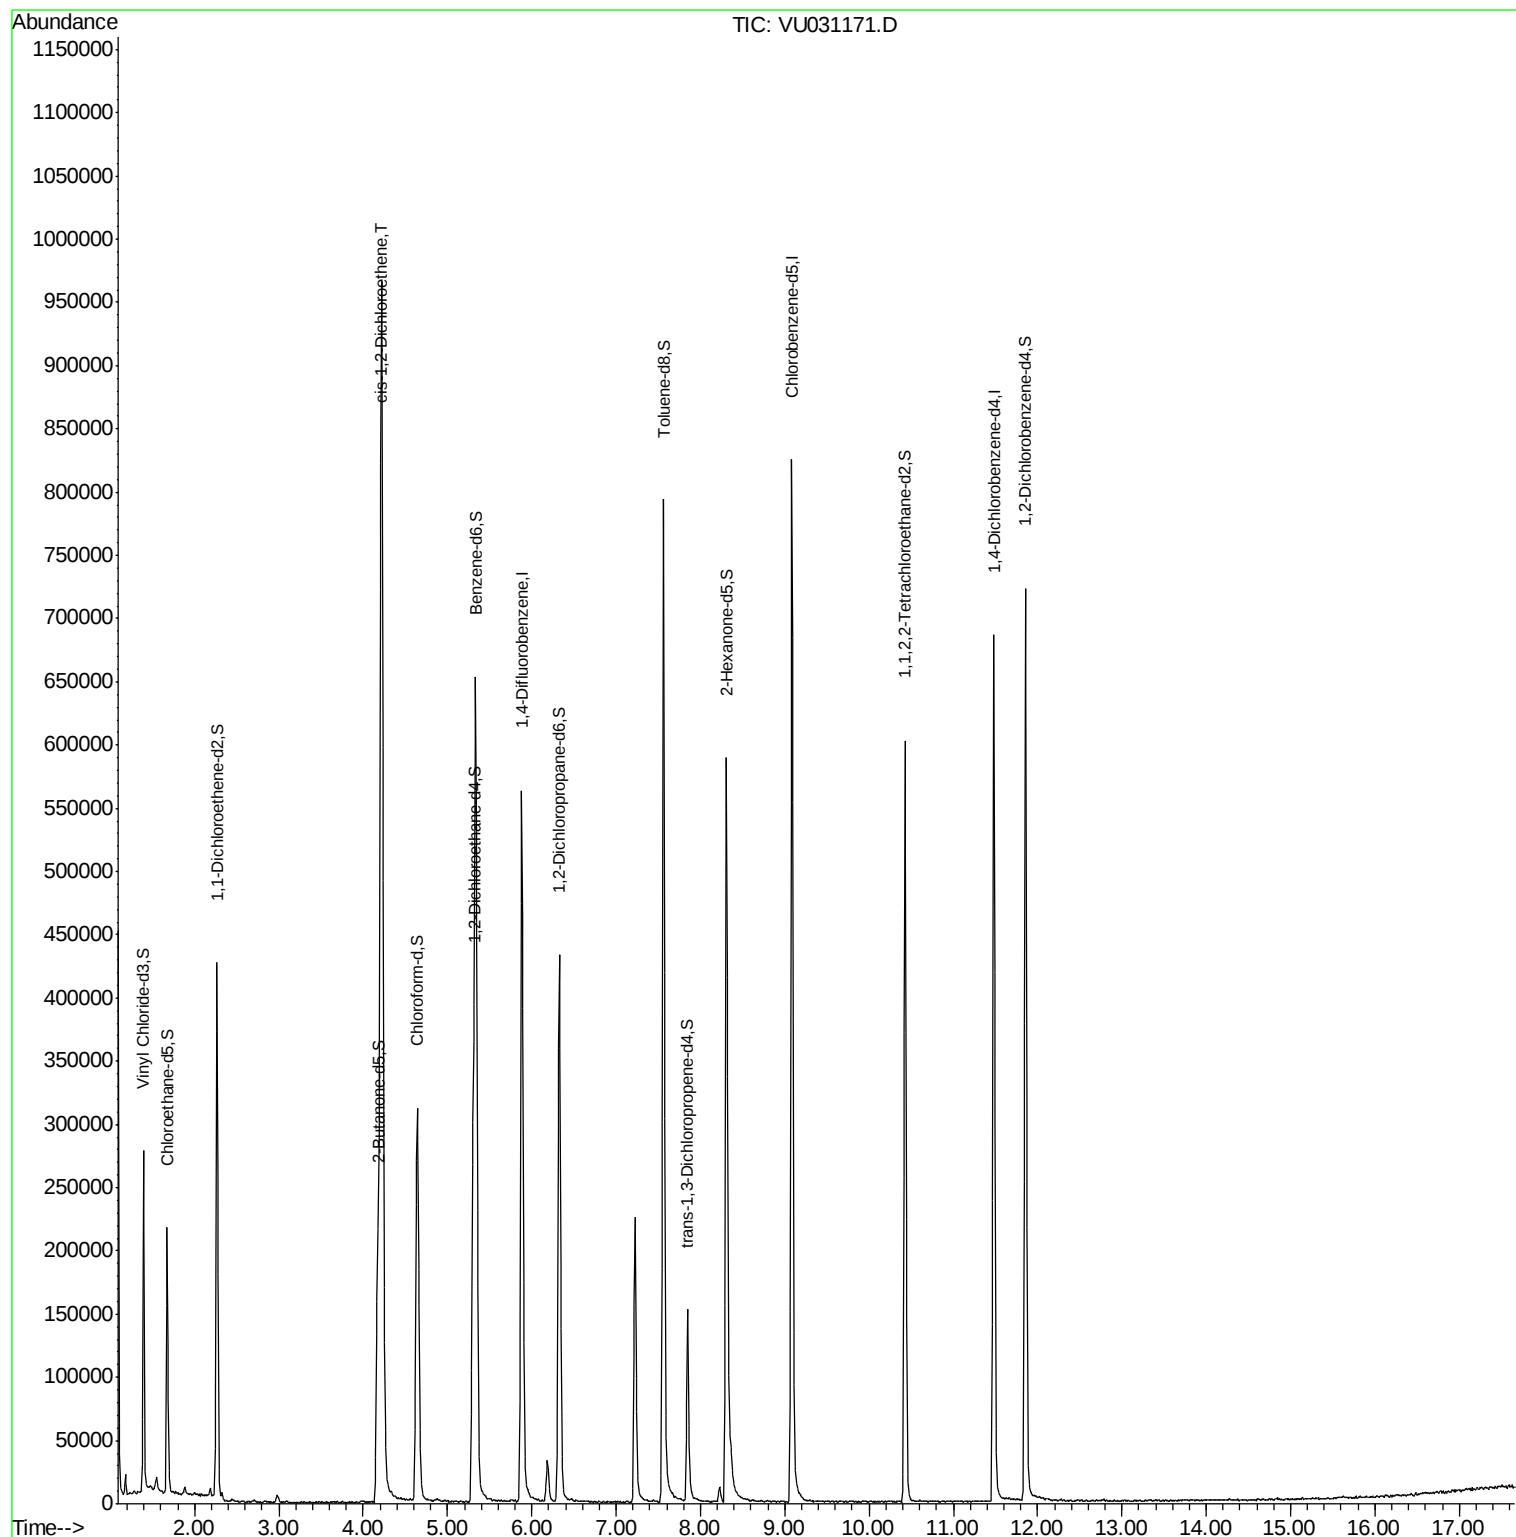

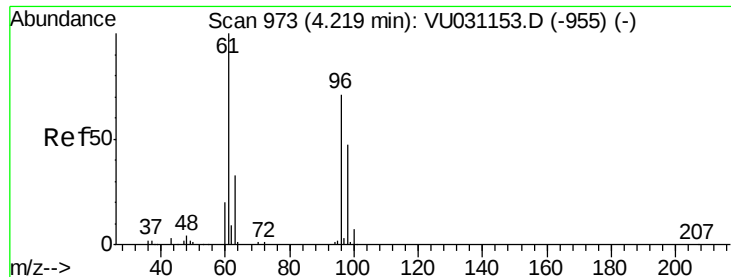

#20
 cis-1,2-Dichloroethene
 Concen: 137.156 ug/L
 RT: 4.22 min Scan# 973
 Delta R.T. -0.00 min
 Lab File: VU031171.D
 Acq: 13 Apr 2019 20:54

Instrument :
 MSVOA_U
 ClientSampleId :
 ETJ63

Tot Ion	Ion	Ratio	Lower	Upper
96	100			
61	134.5	102.9	191.1	
68	0.0	0.0	0.0	

