

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031176.D
 Acq On : 13 Apr 2019 23:14
 Operator : JC/SP
 Sample : K2403-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5129

Quant Time: Apr 15 12:14:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 23:49:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	483392	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	457605	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	179681	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	180097	41.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.48%
7) Chloroethane-d5	1.67	69	151875	46.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.74%
11) 1,1-Dichloroethene-d2	2.26	63	255052	32.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.36%
21) 2-Butanone-d5	4.17	46	322911	94.42	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.42%
24) Chloroform-d	4.64	84	329392	49.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.94%
26) 1,2-Dichloroethane-d4	5.30	65	219345	48.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.54%
32) Benzene-d6	5.33	84	669342	50.10	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	6.32	67	220988	48.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.54%
41) Toluene-d8	7.56	98	546993	46.20	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.85	79	91556	43.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.72%
47) 2-Hexanone-d5	8.31	63	190251	90.92	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.92%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	303129	49.09	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.18%
64) 1,2-Dichlorobenzene-d4	11.86	152	187110	52.95	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.90%


Target Compounds					Ovalue
13) Acetone	2.32	43	146772	41.940 ug/L	99
22) 2-Butanone	4.26	43	78224	19.064 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031176.D
Acq On : 13 Apr 2019 23:14
Operator : JC/SP
Sample : K2403-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5129

Quant Time: Apr 15 12:14:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 23:49:21 2019
Response via : Initial Calibration




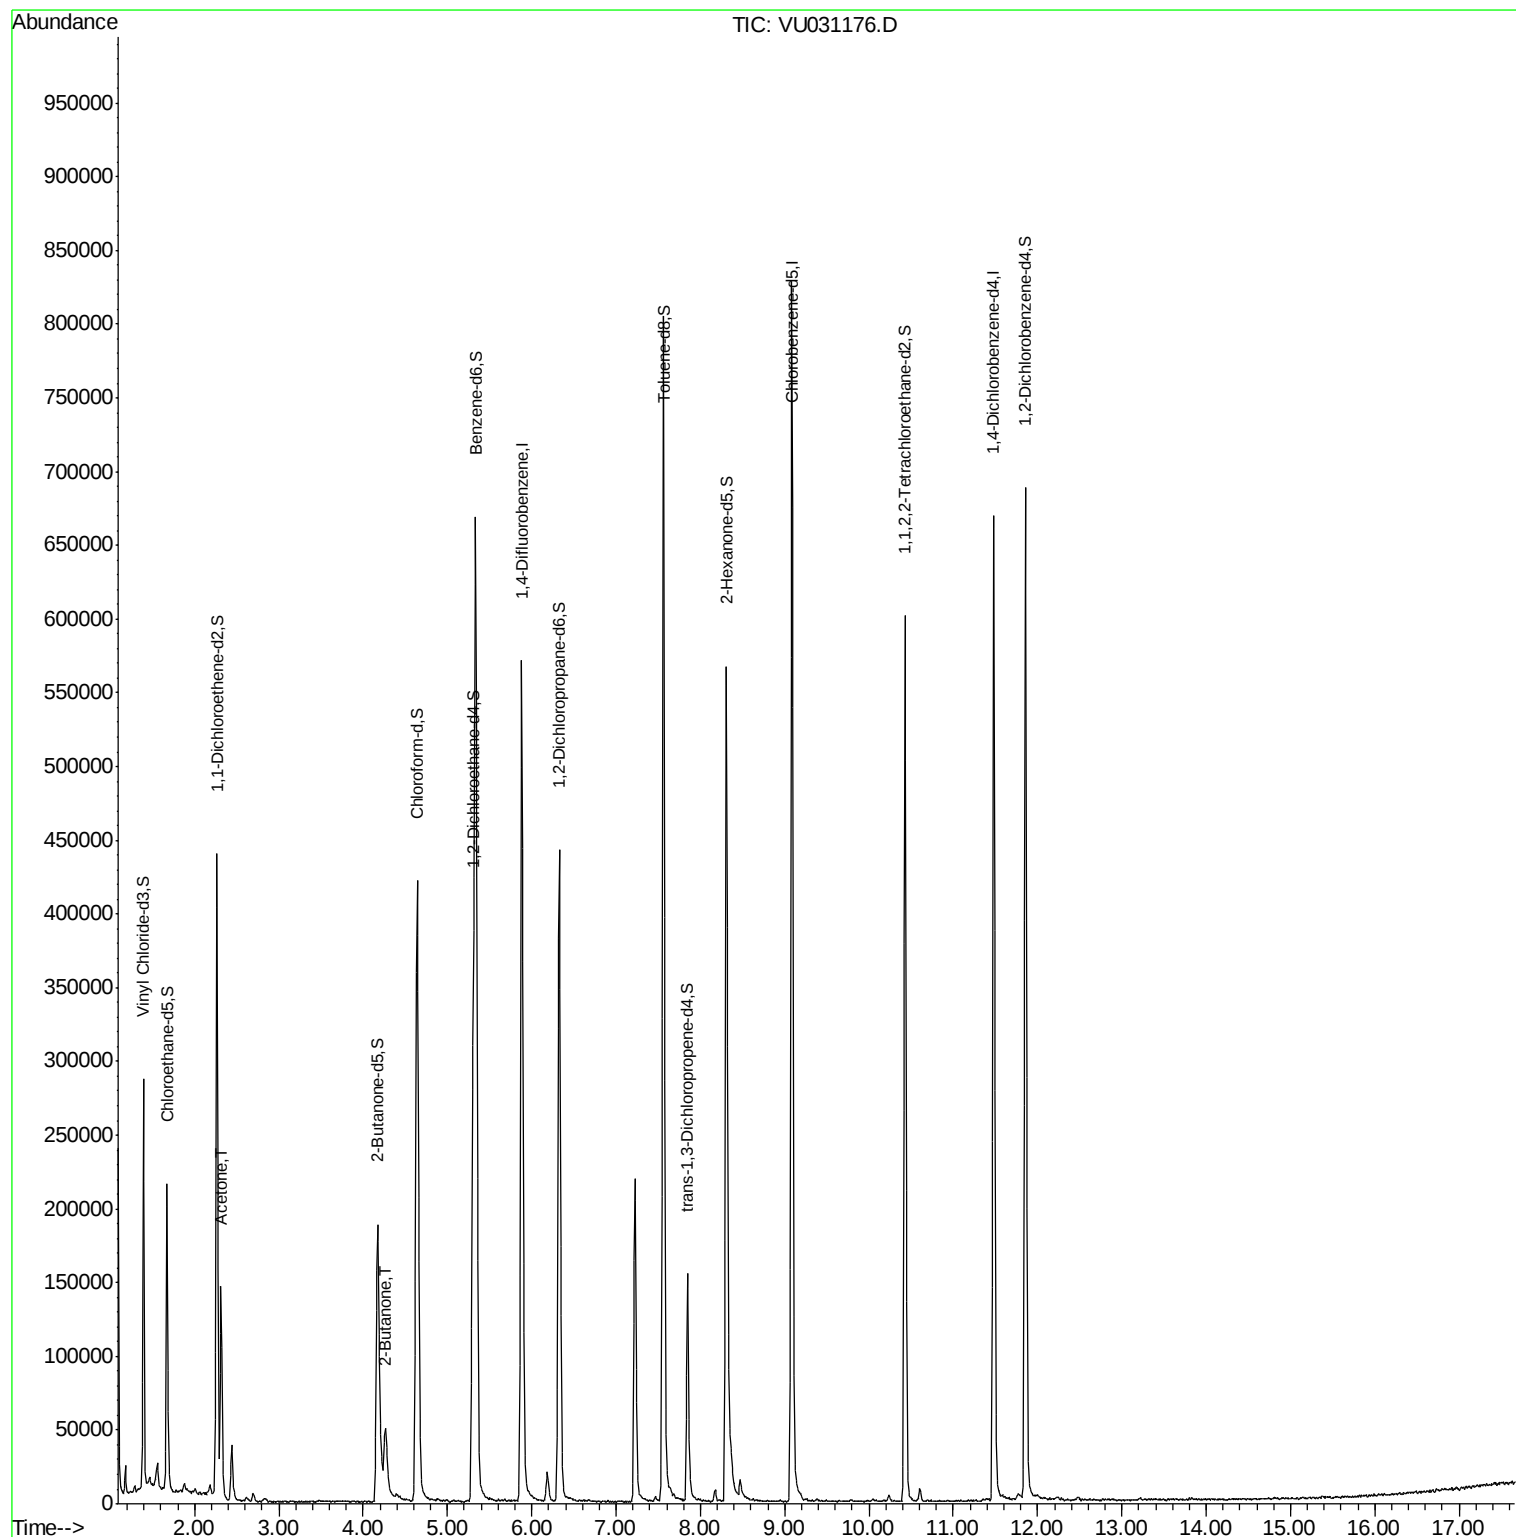


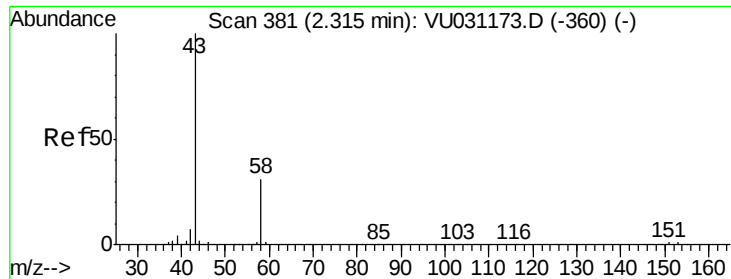

#13
Acetone
Concen: 41.940 ug/L
RT: 2.32 min Scan# 381
Delta R.T. 0.00 min
Lab File: VU031176.D
Acq: 13 Apr 2019 23:14

Instrument :
MSVOA_U
ClientSampleId :
A5129

Tot Ion: 43 Resp: 146772
Ion Ratio Lower Upper
43 100
58 31.4 0.0 64.0

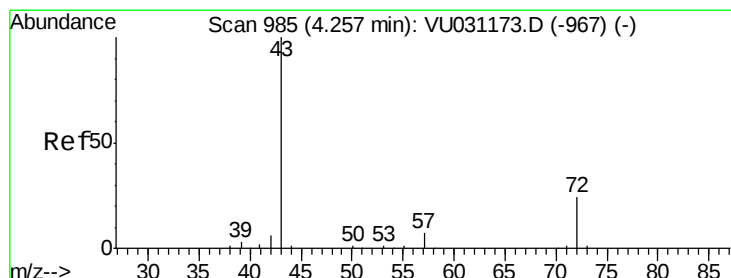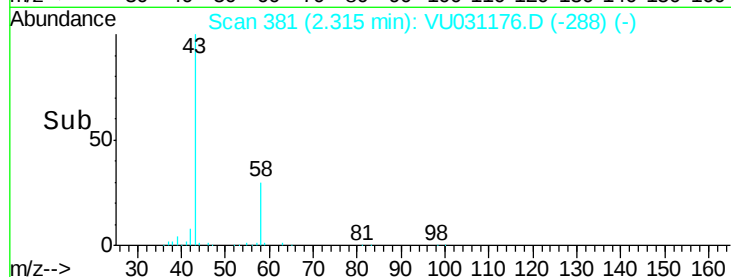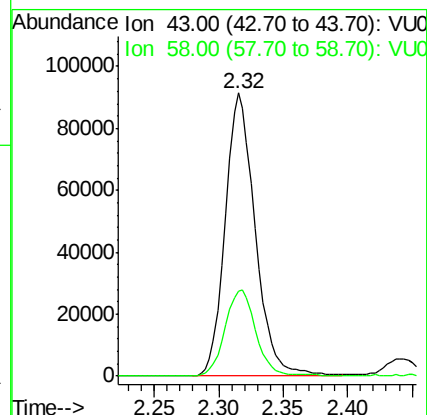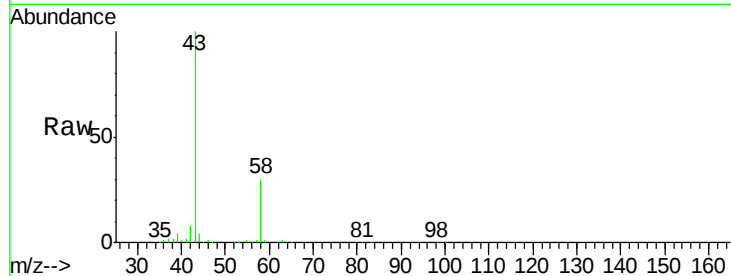

#22
2-Butanone
Concen: 19.064 ug/L
RT: 4.26 min Scan# 987
Delta R.T. 0.01 min
Lab File: VU031176.D
Acq: 13 Apr 2019 23:14

Tgt Ion: 43 Resp: 78224
Ion Ratio Lower Upper
43 100
72 24.3 10.8 32.4

