

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031169.D
 Acq On : 13 Apr 2019 20:08
 Operator : JC/SP
 Sample : K2341-14 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB736

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rVB2	15976	15129	0.52%	0.083%
2	1.392	87	94	105	rBV	280360	299664	10.27%	1.653%
3	1.675	174	182	198	rVB	198405	270994	9.29%	1.495%
4	1.875	241	244	254	rVB4	5675	7755	0.27%	0.043%
5	2.264	355	365	378	rVB	422434	644076	22.08%	3.552%
6	2.408	408	410	413	rVV2	826	573	0.02%	0.003%
7	2.444	413	421	436	rVB	6969	13245	0.45%	0.073%
8	2.566	456	459	462	rVV3	883	799	0.03%	0.004%
9	2.589	464	466	470	rVV3	1131	761	0.03%	0.004%
10	2.608	470	472	475	rVV3	672	447	0.02%	0.002%
11	2.653	482	486	489	rVB3	1276	858	0.03%	0.005%
12	2.675	489	493	494	rBV3	1173	663	0.02%	0.004%
13	2.698	495	500	511	rVB6	2815	4306	0.15%	0.024%
14	2.826	537	540	541	rBV3	872	457	0.02%	0.003%
15	2.978	577	587	600	rVV5	5494	10807	0.37%	0.060%
16	3.482	740	744	748	rBV3	676	676	0.02%	0.004%
17	3.894	866	872	874	rBV	934	908	0.03%	0.005%
18	4.170	945	958	964	rBV	189326	394165	13.51%	2.174%
19	4.412	1030	1033	1039	rBV6	1349	1064	0.04%	0.006%
20	4.511	1062	1064	1068	rVB2	973	725	0.02%	0.004%
21	4.534	1068	1071	1075	rBV5	714	465	0.02%	0.003%
22	4.640	1086	1104	1133	rBV2	303345	741374	25.42%	4.089%
23	4.781	1146	1148	1151	rVB3	895	502	0.02%	0.003%
24	4.801	1151	1154	1158	rBV4	776	553	0.02%	0.003%
25	4.830	1161	1163	1169	rVB5	1068	931	0.03%	0.005%
26	4.881	1174	1179	1181	rBV4	963	1030	0.04%	0.006%
27	5.100	1242	1247	1250	rBV4	879	866	0.03%	0.005%
28	5.135	1253	1258	1261	rBV3	578	580	0.02%	0.003%
29	5.209	1278	1281	1284	rVB3	845	518	0.02%	0.003%
30	5.228	1284	1287	1291	rBV2	943	1004	0.03%	0.006%
31	5.334	1297	1320	1351	rBV3	619251	1837852	63.01%	10.136%
32	5.727	1437	1442	1444	rBV2	1154	823	0.03%	0.005%
33	5.881	1477	1490	1516	rBV	549574	1120908	38.43%	6.182%
34	6.183	1569	1584	1612	rBV	448794	898087	30.79%	4.953%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031169.D
 Acq On : 13 Apr 2019 20:08
 Operator : JC/SP
 Sample : K2341-14 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB736

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.325	1615	1628	1653	rVV	425067	869767	29.82%	4.797%
36	6.659	1730	1732	1737	rVB4	1223	727	0.02%	0.004%
37	6.688	1737	1741	1743	rBV4	520	451	0.02%	0.002%
38	6.746	1755	1759	1762	rBV	1131	1006	0.03%	0.006%
39	6.810	1776	1779	1784	rBV3	668	630	0.02%	0.003%
40	6.865	1793	1796	1799	rBV4	747	606	0.02%	0.003%
41	6.958	1820	1825	1827	rBV2	1277	1011	0.03%	0.006%
42	7.116	1870	1874	1878	rVB3	591	586	0.02%	0.003%
43	7.167	1887	1890	1893	rBV2	602	447	0.02%	0.002%
44	7.225	1897	1908	1937	rBV	220243	414665	14.22%	2.287%
45	7.450	1972	1978	1981	rBV7	1299	1506	0.05%	0.008%
46	7.563	1999	2013	2030	rBV	796075	1426147	48.89%	7.865%
47	7.846	2091	2101	2122	rBV	153599	274241	9.40%	1.512%
48	7.993	2145	2147	2150	rVB4	1379	653	0.02%	0.004%
49	8.013	2151	2153	2157	rVB2	1171	711	0.02%	0.004%
50	8.119	2184	2186	2190	rVB4	901	465	0.02%	0.003%
51	8.164	2196	2200	2203	rBV3	1050	1002	0.03%	0.006%
52	8.222	2205	2218	2234	rBV	1709976	2916957	100.00%	16.088%
53	8.309	2236	2245	2280	rVB	573023	1162180	39.84%	6.410%
54	8.566	2322	2325	2327	rBV3	892	539	0.02%	0.003%
55	8.624	2336	2343	2348	rBV6	1332	1866	0.06%	0.010%
56	8.694	2362	2365	2368	rBV3	723	535	0.02%	0.003%
57	8.714	2368	2371	2376	rVB4	1237	1059	0.04%	0.006%
58	8.739	2376	2379	2381	rBV2	654	444	0.02%	0.002%
59	8.797	2394	2397	2403	rVB5	1230	1109	0.04%	0.006%
60	8.839	2406	2410	2412	rBV3	895	567	0.02%	0.003%
61	8.855	2413	2415	2418	rVB2	842	476	0.02%	0.003%
62	8.894	2422	2427	2428	rBV2	710	467	0.02%	0.003%
63	8.948	2442	2444	2453	rVB5	621	526	0.02%	0.003%
64	9.087	2474	2487	2512	rBV	837093	1434924	49.19%	7.914%
65	9.489	2609	2612	2613	rBV	831	469	0.02%	0.003%
66	9.617	2649	2652	2656	rBV	634	516	0.02%	0.003%
67	9.659	2661	2665	2669	rVB4	851	753	0.03%	0.004%
68	9.788	2699	2705	2707	rBV4	632	692	0.02%	0.004%
69	9.868	2726	2730	2733	rBV3	690	480	0.02%	0.003%
70	9.919	2744	2746	2752	rVB2	684	613	0.02%	0.003%
71	9.964	2752	2760	2762	rBV3	1046	1381	0.05%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031169.D
 Acq On : 13 Apr 2019 20:08
 Operator : JC/SP
 Sample : K2341-14 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB736

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.071	2790	2793	2796	rVB4	1063	779	0.03%	0.004%
73	10.093	2796	2800	2803	rBV2	1164	963	0.03%	0.005%
74	10.173	2822	2825	2828	rVB2	825	529	0.02%	0.003%
75	10.318	2867	2870	2874	rVB2	866	570	0.02%	0.003%
76	10.379	2884	2889	2890	rBV	684	564	0.02%	0.003%
77	10.427	2892	2904	2930	rVV	597119	967904	33.18%	5.338%
78	10.572	2946	2949	2951	rBV3	1084	670	0.02%	0.004%
79	10.601	2954	2958	2960	rVB3	1292	961	0.03%	0.005%
80	10.643	2969	2971	2976	rVB	729	454	0.02%	0.003%
81	10.842	3028	3033	3034	rBV2	856	641	0.02%	0.004%
82	10.968	3068	3072	3077	rBV3	619	506	0.02%	0.003%
83	11.398	3203	3206	3211	rBV2	644	441	0.02%	0.002%
84	11.421	3211	3213	3215	rBV	1206	581	0.02%	0.003%
85	11.482	3220	3232	3257	rBV	694848	1150205	39.43%	6.344%
86	11.858	3336	3349	3378	rBV	715431	1200204	41.15%	6.619%
87	12.260	3471	3474	3476	rBV2	873	512	0.02%	0.003%
88	12.408	3517	3520	3525	rVB5	847	631	0.02%	0.003%
89	12.533	3555	3559	3566	rVB5	1168	1499	0.05%	0.008%
90	12.572	3569	3571	3577	rVB3	640	515	0.02%	0.003%
91	12.627	3584	3588	3592	rBV3	1085	1069	0.04%	0.006%
92	12.781	3632	3636	3639	rBV3	648	654	0.02%	0.004%
93	12.810	3642	3645	3648	rBV3	889	653	0.02%	0.004%
94	13.074	3725	3727	3731	rVB3	1105	710	0.02%	0.004%
95	13.247	3779	3781	3784	rBV3	738	571	0.02%	0.003%
96	14.601	4199	4202	4206	rBV3	949	918	0.03%	0.005%
97	14.810	4265	4267	4270	rBV4	1102	751	0.03%	0.004%
98	15.131	4365	4367	4369	rBV3	950	473	0.02%	0.003%
99	15.250	4401	4404	4407	rVB	1382	776	0.03%	0.004%
100	15.701	4541	4544	4547	rBV4	1635	1290	0.04%	0.007%


Sum of corrected areas: 18131733

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031169.D
Acq On : 13 Apr 2019 20:08
Operator : JC/SP
Sample : K2341-14 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB736

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

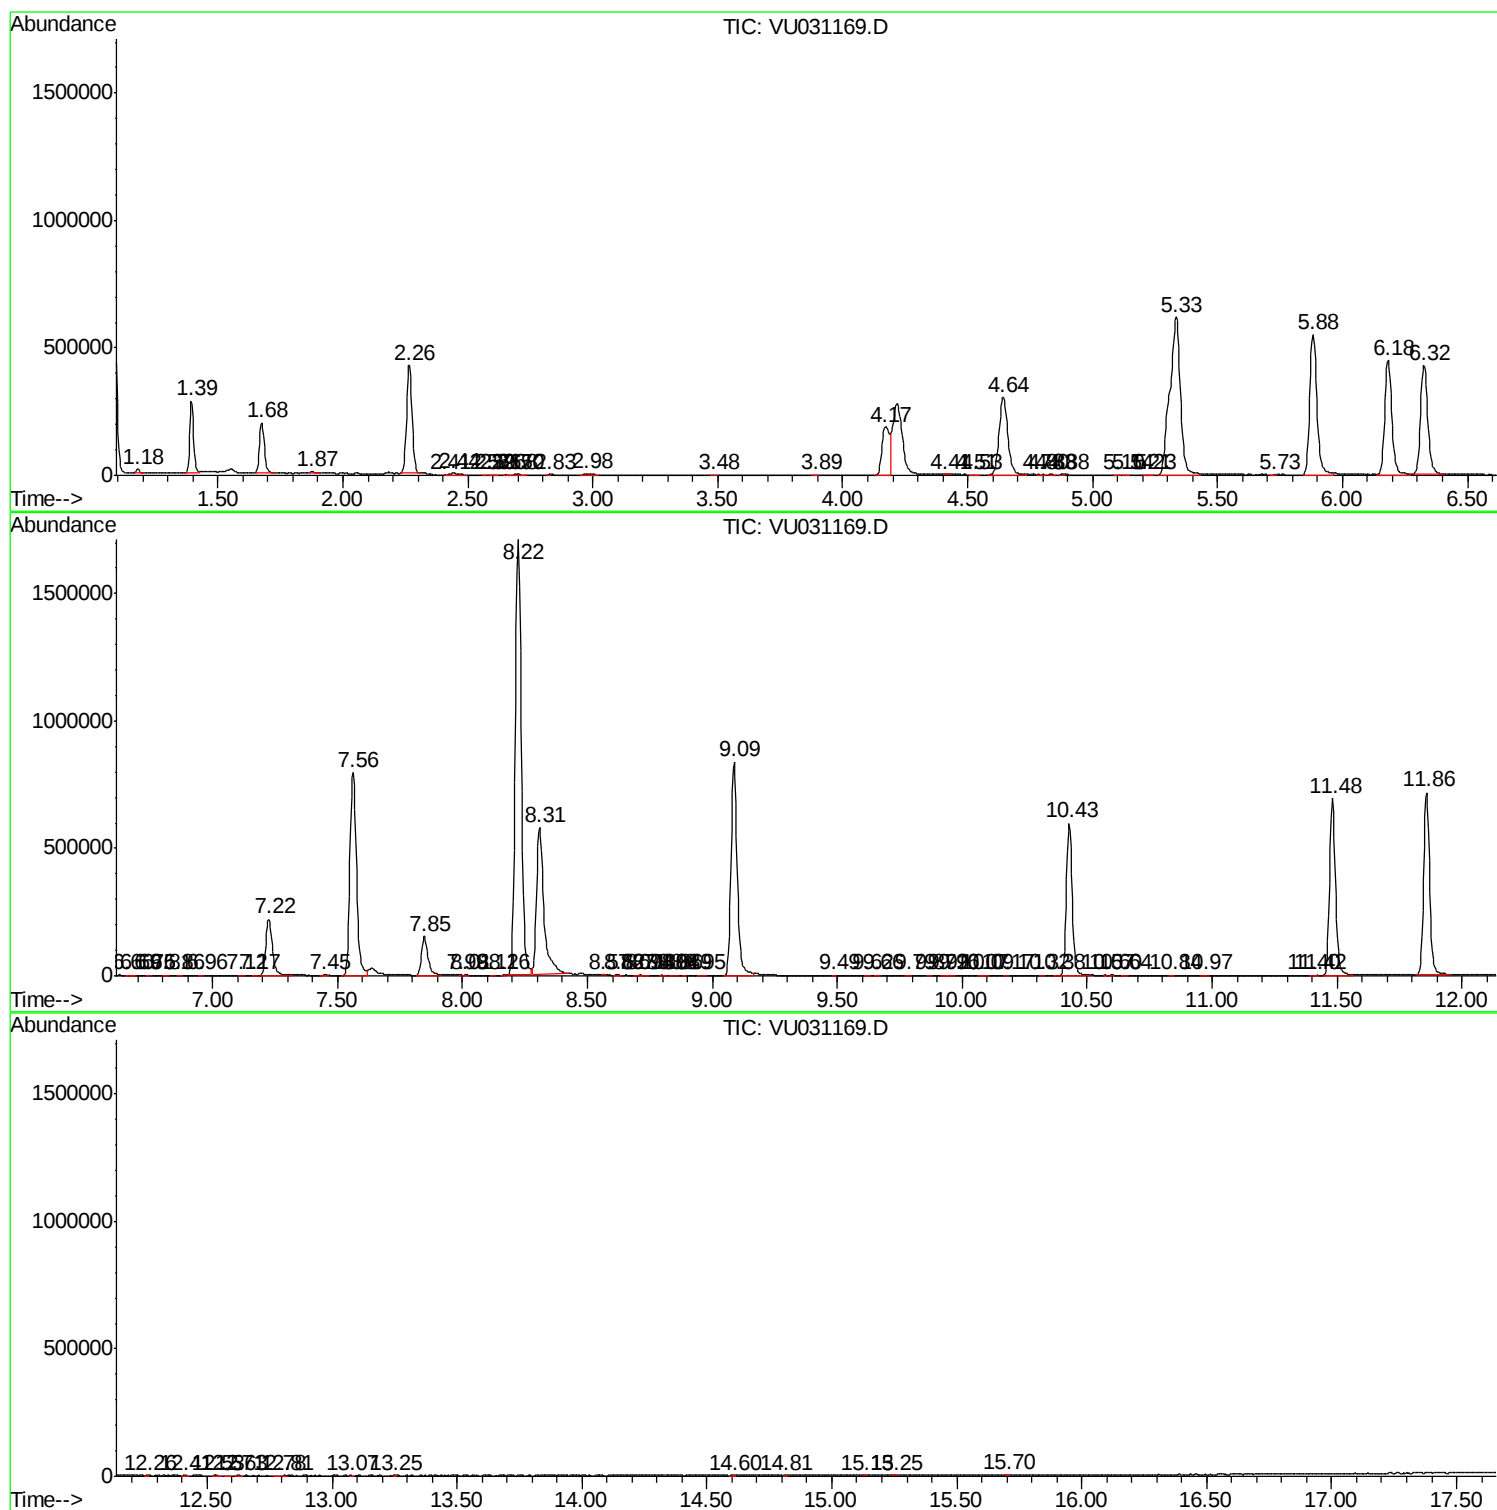

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031169.D
Acq On : 13 Apr 2019 20:08
Operator : JC/SP
Sample : K2341-14 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB736

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031169.D
Acq On : 13 Apr 2019 20:08
Operator : JC/SP
Sample : K2341-14 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB736

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc