

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031180.D
 Acq On : 14 Apr 2019 00:49
 Operator : JC/SP
 Sample : K2339-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	22	28	35	rBV3	19975	20769	1.04%	0.137%
2	1.254	47	51	57	rBV2	7776	8433	0.42%	0.055%
3	1.396	88	95	107	rVB	296128	307336	15.44%	2.021%
4	1.466	111	117	131	rVB	95707	104810	5.27%	0.689%
5	1.675	174	182	196	rVB	199933	271275	13.63%	1.784%
6	2.267	354	366	376	rBV	422951	659940	33.15%	4.339%
7	2.315	376	381	400	rVB2	44105	75494	3.79%	0.496%
8	2.441	411	420	440	rBV2	21407	41913	2.11%	0.276%
9	2.614	470	474	481	rBV4	1399	965	0.05%	0.006%
10	2.695	490	499	512	rVB2	15547	27374	1.38%	0.180%
11	2.781	522	526	529	rBV4	667	627	0.03%	0.004%
12	2.833	532	542	551	rBV5	3653	7457	0.37%	0.049%
13	2.994	580	592	606	rVB3	12150	26577	1.34%	0.175%
14	3.084	616	620	624	rBV3	859	757	0.04%	0.005%
15	3.177	642	649	651	rBV4	2852	3060	0.15%	0.020%
16	3.267	673	677	682	rVB4	607	538	0.03%	0.004%
17	3.376	707	711	714	rBV2	1021	871	0.04%	0.006%
18	3.431	722	728	734	rVB6	1107	1351	0.07%	0.009%
19	3.556	763	767	771	rBV2	624	558	0.03%	0.004%
20	3.711	811	815	819	rVB3	758	611	0.03%	0.004%
21	3.762	827	831	836	rVB2	708	556	0.03%	0.004%
22	3.936	881	885	888	rVB2	672	583	0.03%	0.004%
23	3.961	888	893	894	rBV2	1904	1350	0.07%	0.009%
24	3.994	895	903	910	rBV6	4264	7362	0.37%	0.048%
25	4.170	945	958	986	rBV	196382	528506	26.55%	3.475%
26	4.640	1087	1104	1129	rBV	329720	797009	40.04%	5.241%
27	4.871	1170	1176	1179	rBV3	1890	1938	0.10%	0.013%
28	4.923	1189	1192	1195	rBV3	826	548	0.03%	0.004%
29	5.026	1220	1224	1227	rBV4	670	663	0.03%	0.004%
30	5.125	1250	1255	1257	rBV2	771	649	0.03%	0.004%
31	5.154	1261	1264	1267	rBV3	900	626	0.03%	0.004%
32	5.215	1279	1283	1287	rVB3	732	683	0.03%	0.004%
33	5.334	1296	1320	1345	rBV2	671138	1990495	100.00%	13.089%
34	5.688	1428	1430	1434	rVB2	1170	858	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031180.D
 Acq On : 14 Apr 2019 00:49
 Operator : JC/SP
 Sample : K2339-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.817	1468	1470	1473	rVB3	1337	751	0.04%	0.005%
36	5.881	1473	1490	1513	rBV	577566	1151289	57.84%	7.570%
37	6.186	1573	1585	1597	rVV6	19661	41708	2.10%	0.274%
38	6.325	1613	1628	1652	rBV	450349	903648	45.40%	5.942%
39	6.659	1729	1732	1735	rBV4	975	777	0.04%	0.005%
40	6.730	1753	1754	1762	rVB3	1095	856	0.04%	0.006%
41	6.897	1804	1806	1811	rBV2	776	550	0.03%	0.004%
42	7.045	1850	1852	1857	rVB2	887	638	0.03%	0.004%
43	7.071	1857	1860	1865	rBV2	639	648	0.03%	0.004%
44	7.225	1896	1908	1929	rBV	217837	408540	20.52%	2.686%
45	7.405	1960	1964	1966	rBV4	1133	791	0.04%	0.005%
46	7.563	1999	2013	2031	rBV	826750	1462844	73.49%	9.619%
47	7.845	2091	2101	2126	rBV	155632	280954	14.11%	1.847%
48	8.058	2164	2167	2172	rVB4	864	665	0.03%	0.004%
49	8.170	2191	2202	2210	rBV7	8410	15726	0.79%	0.103%
50	8.202	2210	2212	2216	rVB2	1255	740	0.04%	0.005%
51	8.254	2223	2228	2232	rBV5	715	836	0.04%	0.005%
52	8.308	2234	2245	2282	rBV	586434	1151507	57.85%	7.572%
53	8.591	2329	2333	2337	rVB5	1075	1032	0.05%	0.007%
54	8.649	2349	2351	2358	rVB4	1005	756	0.04%	0.005%
55	8.765	2384	2387	2391	rBV2	562	616	0.03%	0.004%
56	8.781	2391	2392	2401	rVB2	1051	1006	0.05%	0.007%
57	8.849	2409	2413	2416	rBV2	1048	595	0.03%	0.004%
58	8.871	2417	2420	2427	rVB4	746	677	0.03%	0.004%
59	9.019	2462	2466	2473	rVB4	712	726	0.04%	0.005%
60	9.087	2473	2487	2509	rBV	818645	1419254	71.30%	9.332%
61	9.315	2556	2558	2567	rVB5	679	705	0.04%	0.005%
62	9.357	2567	2571	2572	rBV2	1061	807	0.04%	0.005%
63	9.386	2576	2580	2585	rVV5	1819	1780	0.09%	0.012%
64	9.553	2626	2632	2635	rBV4	1212	1000	0.05%	0.007%
65	9.652	2652	2663	2672	rBV3	19360	33071	1.66%	0.217%
66	9.710	2678	2681	2685	rBV5	791	649	0.03%	0.004%
67	9.730	2685	2687	2690	rBV3	1246	806	0.04%	0.005%
68	9.836	2715	2720	2721	rBV3	1336	1003	0.05%	0.007%
69	9.926	2739	2748	2766	rBV2	23649	46403	2.33%	0.305%
70	10.035	2773	2782	2804	rVB7	15590	33239	1.67%	0.219%
71	10.119	2805	2808	2813	rBV3	1178	1041	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031180.D
 Acq On : 14 Apr 2019 00:49
 Operator : JC/SP
 Sample : K2339-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.251	2845	2849	2855	rVB4	852	938	0.05%	0.006%
73	10.305	2863	2866	2870	rBV3	930	807	0.04%	0.005%
74	10.427	2892	2904	2924	rBV	607167	997651	50.12%	6.560%
75	10.578	2945	2951	2953	rBV5	1283	1365	0.07%	0.009%
76	10.607	2953	2960	2968	rVB4	4273	5629	0.28%	0.037%
77	10.878	3040	3044	3049	rVB3	856	740	0.04%	0.005%
78	11.324	3181	3183	3191	rVB3	1917	1593	0.08%	0.010%
79	11.376	3195	3199	3201	rBV3	2106	1713	0.09%	0.011%
80	11.479	3219	3231	3254	rBV	674752	1122550	56.40%	7.381%
81	11.739	3310	3312	3318	rBV4	1404	1144	0.06%	0.008%
82	11.855	3337	3348	3373	rBV	703840	1198383	60.21%	7.880%
83	12.279	3476	3480	3481	rBV3	1004	659	0.03%	0.004%
84	12.469	3536	3539	3542	rBV3	1127	801	0.04%	0.005%
85	12.530	3556	3558	3562	rBV	780	637	0.03%	0.004%
86	12.758	3625	3629	3631	rBV3	959	920	0.05%	0.006%
87	13.000	3701	3704	3706	rBV2	1199	760	0.04%	0.005%
88	13.122	3739	3742	3745	rVB2	1117	730	0.04%	0.005%
89	13.292	3792	3795	3797	rBV2	796	577	0.03%	0.004%
90	13.373	3818	3820	3826	rVB2	797	662	0.03%	0.004%
91	13.447	3840	3843	3844	rBV2	867	545	0.03%	0.004%
92	13.910	3985	3987	3995	rVB4	1093	967	0.05%	0.006%
93	13.990	4008	4012	4015	rBV4	1839	1265	0.06%	0.008%
94	14.057	4031	4033	4039	rVB4	1123	1004	0.05%	0.007%
95	14.090	4041	4043	4046	rBV2	981	547	0.03%	0.004%
96	14.401	4136	4140	4142	rBV	854	768	0.04%	0.005%
97	14.585	4194	4197	4199	rBV2	1251	821	0.04%	0.005%
98	14.784	4256	4259	4263	rBV2	1226	705	0.04%	0.005%
99	14.922	4300	4302	4307	rVB3	1111	790	0.04%	0.005%
100	15.784	4567	4570	4572	rBV2	1647	1071	0.05%	0.007%


Sum of corrected areas: 15207918

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031180.D
Acq On : 14 Apr 2019 00:49
Operator : JC/SP
Sample : K2339-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC51

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

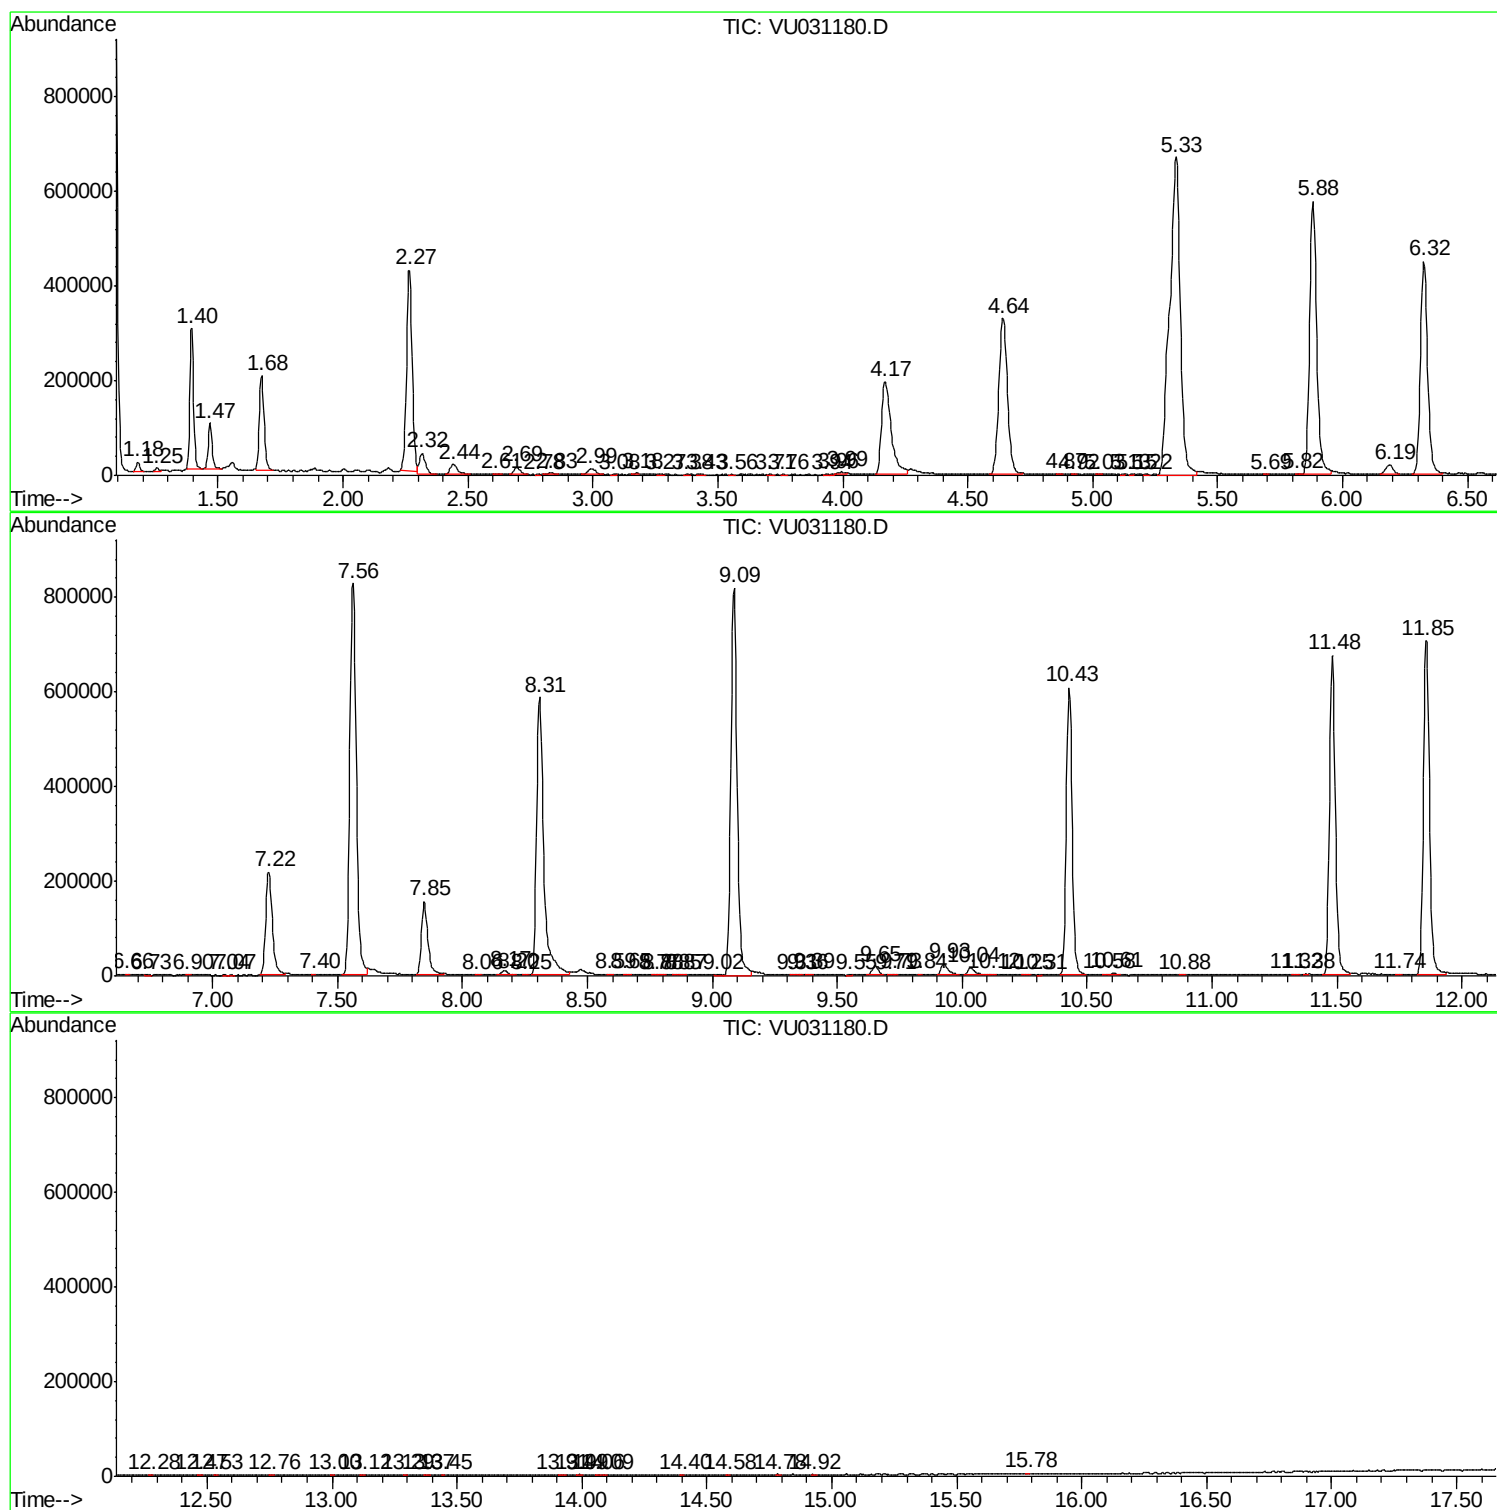

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031180.D
Acq On : 14 Apr 2019 00:49
Operator : JC/SP
Sample : K2339-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC51

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031180.D
Acq On : 14 Apr 2019 00:49
Operator : JC/SP
Sample : K2339-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC51

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc