

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031184.D
 Acq On : 14 Apr 2019 02:23
 Operator : JC/SP
 Sample : K2339-15DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	88	94	107	rBV	290720	310362	15.90%	1.953%
2	1.672	173	181	193	rVB	191106	259370	13.29%	1.632%
3	2.273	356	368	396	rVB4	855900	1581995	81.05%	9.954%
4	2.447	411	422	438	rVB2	7231	16802	0.86%	0.106%
5	2.505	438	440	445	rBV2	736	403	0.02%	0.003%
6	2.550	452	454	458	rVB3	901	503	0.03%	0.003%
7	2.662	486	489	491	rBV3	825	415	0.02%	0.003%
8	2.695	493	499	509	rVV5	4655	7081	0.36%	0.045%
9	2.743	512	514	516	rBV	567	345	0.02%	0.002%
10	2.817	533	537	539	rBV5	1235	1033	0.05%	0.006%
11	2.939	572	575	579	rBV2	349	332	0.02%	0.002%
12	3.039	604	606	609	rVV	436	247	0.01%	0.002%
13	3.122	630	632	635	rVB	477	229	0.01%	0.001%
14	3.135	635	636	639	rBB2	629	205	0.01%	0.001%
15	3.167	643	646	649	rBV2	268	170	0.01%	0.001%
16	3.193	652	654	657	rVB2	322	221	0.01%	0.001%
17	3.367	705	708	711	rVV3	619	466	0.02%	0.003%
18	3.383	711	713	716	rVB	732	389	0.02%	0.002%
19	3.441	716	731	757	rBV2	49727	114631	5.87%	0.721%
20	3.540	757	762	767	rVV2	884	1049	0.05%	0.007%
21	3.579	767	774	784	rVB2	983	1882	0.10%	0.012%
22	3.621	784	787	791	rBV2	532	458	0.02%	0.003%
23	3.640	791	793	797	rVB	386	241	0.01%	0.002%
24	3.724	815	819	822	rVB3	545	436	0.02%	0.003%
25	3.743	822	825	826	rBV2	402	239	0.01%	0.002%
26	3.775	831	835	837	rBV	363	281	0.01%	0.002%
27	3.807	843	845	849	rVB2	666	384	0.02%	0.002%
28	3.826	849	851	856	rBV	272	234	0.01%	0.001%
29	3.852	856	859	863	rBV3	537	411	0.02%	0.003%
30	3.907	873	876	879	rBV	304	214	0.01%	0.001%
31	4.006	904	907	912	rVB3	347	243	0.01%	0.002%
32	4.042	912	918	921	rBV3	473	427	0.02%	0.003%
33	4.122	939	943	946	rBV2	587	527	0.03%	0.003%
34	4.167	946	957	993	rBV	196613	609327	31.22%	3.834%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031184.D
 Acq On : 14 Apr 2019 02:23
 Operator : JC/SP
 Sample : K2339-15DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	4.640	1085	1104	1131	rBV2	322250	782378	40.08%	4.923%
36	4.826	1159	1162	1163	rBV2	813	395	0.02%	0.002%
37	5.039	1223	1228	1234	rVB3	846	850	0.04%	0.005%
38	5.068	1234	1237	1240	rBV	814	621	0.03%	0.004%
39	5.135	1254	1258	1261	rBV3	250	219	0.01%	0.001%
40	5.151	1261	1263	1265	rBV	375	170	0.01%	0.001%
41	5.164	1265	1267	1269	rBV2	465	223	0.01%	0.001%
42	5.206	1278	1280	1283	rBV	379	244	0.01%	0.002%
43	5.232	1286	1288	1292	rVB	818	447	0.02%	0.003%
44	5.334	1294	1320	1348	rBV2	654850	1951845	100.00%	12.282%
45	5.723	1437	1441	1442	rBV2	694	429	0.02%	0.003%
46	5.813	1466	1469	1473	rBV4	837	667	0.03%	0.004%
47	5.881	1474	1490	1514	rBV	565240	1129752	57.88%	7.109%
48	6.109	1558	1561	1565	rVB2	1179	866	0.04%	0.005%
49	6.183	1572	1584	1607	rBV6	43876	97700	5.01%	0.615%
50	6.325	1614	1628	1653	rBV	440205	894947	45.85%	5.631%
51	6.569	1700	1704	1706	rBV3	818	696	0.04%	0.004%
52	6.768	1764	1766	1768	rBV2	556	262	0.01%	0.002%
53	6.791	1771	1773	1776	rVV2	567	324	0.02%	0.002%
54	6.817	1779	1781	1787	rVB4	655	461	0.02%	0.003%
55	6.875	1797	1799	1800	rVB2	734	202	0.01%	0.001%
56	6.923	1812	1814	1817	rBV2	706	435	0.02%	0.003%
57	6.961	1824	1826	1828	rBV	437	187	0.01%	0.001%
58	6.981	1829	1832	1836	rVB3	730	491	0.03%	0.003%
59	7.019	1841	1844	1849	rVB2	529	523	0.03%	0.003%
60	7.045	1849	1852	1855	rBV2	687	547	0.03%	0.003%
61	7.080	1861	1863	1867	rVB3	642	478	0.02%	0.003%
62	7.103	1867	1870	1875	rBV3	531	514	0.03%	0.003%
63	7.125	1875	1877	1882	rVB2	454	304	0.02%	0.002%
64	7.151	1882	1885	1888	rVB3	484	279	0.01%	0.002%
65	7.225	1896	1908	1933	rBV	212602	401731	20.58%	2.528%
66	7.492	1989	1991	1993	rVB2	926	317	0.02%	0.002%
67	7.559	2000	2012	2031	rBV	776814	1386771	71.05%	8.726%
68	7.849	2091	2102	2119	rBV2	147012	264289	13.54%	1.663%
69	8.106	2180	2182	2185	rBV3	590	392	0.02%	0.002%
70	8.225	2206	2219	2234	rBV	268069	473987	24.28%	2.982%
71	8.309	2235	2245	2284	rVV	568975	1092370	55.97%	6.873%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031184.D
 Acq On : 14 Apr 2019 02:23
 Operator : JC/SP
 Sample : K2339-15DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	8.678	2358	2360	2361	rBV	448	187	0.01%	0.001%
73	8.894	2422	2427	2429	rBV2	725	639	0.03%	0.004%
74	8.929	2435	2438	2440	rBV	531	235	0.01%	0.001%
75	9.087	2473	2487	2518	rBV	790069	1348195	69.07%	8.483%
76	9.463	2601	2604	2607	rBV3	790	563	0.03%	0.004%
77	9.501	2614	2616	2620	rVB3	720	453	0.02%	0.003%
78	9.575	2633	2639	2643	rBV3	1041	1209	0.06%	0.008%
79	9.672	2664	2669	2673	rBV5	968	1127	0.06%	0.007%
80	9.772	2697	2700	2701	rBV	424	225	0.01%	0.001%
81	9.890	2735	2737	2739	rBV	450	183	0.01%	0.001%
82	10.067	2789	2792	2794	rBV2	632	422	0.02%	0.003%
83	10.247	2847	2848	2849	rBV	633	202	0.01%	0.001%
84	10.366	2881	2885	2888	rBV3	905	583	0.03%	0.004%
85	10.427	2892	2904	2926	rVV	615879	988641	50.65%	6.221%
86	10.579	2949	2951	2955	rBV2	515	391	0.02%	0.002%
87	10.604	2955	2959	2961	rBV	948	783	0.04%	0.005%
88	10.759	3005	3007	3010	rBV	763	481	0.02%	0.003%
89	10.784	3011	3015	3017	rVV	650	464	0.02%	0.003%
90	10.939	3060	3063	3065	rBV	856	613	0.03%	0.004%
91	10.987	3073	3078	3080	rBV2	657	675	0.03%	0.004%
92	11.035	3090	3093	3095	rBV	676	410	0.02%	0.003%
93	11.157	3128	3131	3138	rVB4	776	524	0.03%	0.003%
94	11.376	3196	3199	3203	rBV2	835	643	0.03%	0.004%
95	11.482	3220	3232	3256	rBV	618736	1023616	52.44%	6.441%
96	11.858	3337	3349	3374	rBV	662312	1118691	57.31%	7.039%
97	12.366	3504	3507	3510	rBV3	1096	695	0.04%	0.004%
98	12.771	3628	3633	3634	rBV2	941	809	0.04%	0.005%
99	12.990	3695	3701	3704	rBV3	1279	1357	0.07%	0.009%
100	14.549	4184	4186	4188	rBV2	1146	644	0.03%	0.004%


Sum of corrected areas: 15892525

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031184.D
Acq On : 14 Apr 2019 02:23
Operator : JC/SP
Sample : K2339-15DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC39DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

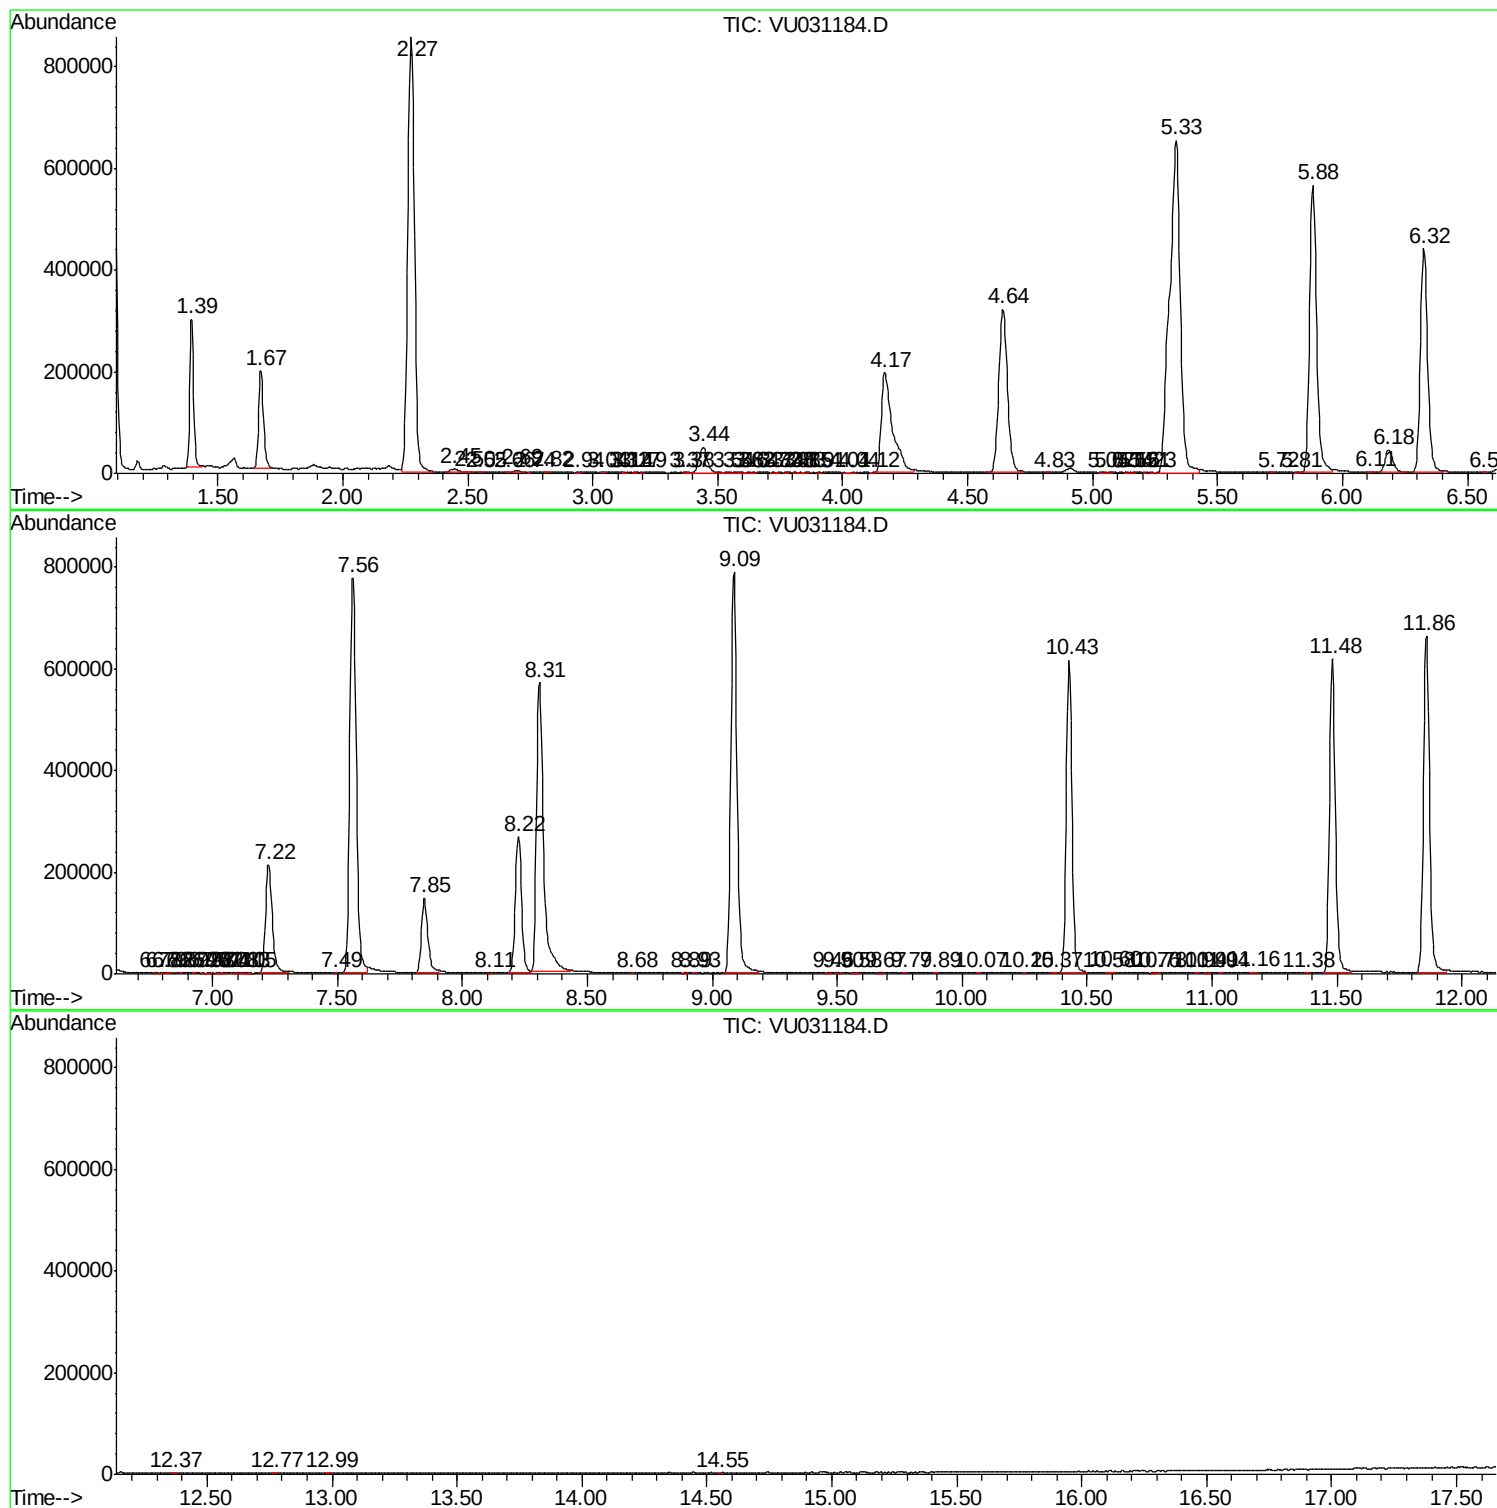

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031184.D
Acq On : 14 Apr 2019 02:23
Operator : JC/SP
Sample : K2339-15DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC39DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031184.D
Acq On : 14 Apr 2019 02:23
Operator : JC/SP
Sample : K2339-15DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC39DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc