

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031185.D
 Acq On : 14 Apr 2019 02:47
 Operator : JC/SP
 Sample : K2339-13DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC36DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	22	27	36	rBV2	16597	16811	0.87%	0.108%
2	1.392	88	94	105	rBV	271602	284473	14.79%	1.822%
3	1.669	173	180	195	rVB	200719	272960	14.19%	1.748%
4	2.267	354	366	379	rBV2	564596	949464	49.36%	6.081%
5	2.399	404	407	412	rBV3	1072	963	0.05%	0.006%
6	2.437	412	419	420	rBV4	3888	3551	0.18%	0.023%
7	2.511	440	442	449	rVB4	597	460	0.02%	0.003%
8	2.698	494	500	512	rVB9	2902	5088	0.26%	0.033%
9	2.791	524	529	533	rBV3	580	524	0.03%	0.003%
10	2.826	536	540	541	rBV2	1009	643	0.03%	0.004%
11	3.067	612	615	618	rVB	674	447	0.02%	0.003%
12	3.090	618	622	625	rBV2	643	464	0.02%	0.003%
13	3.177	645	649	651	rBV2	962	797	0.04%	0.005%
14	3.379	708	712	717	rVB4	1069	1011	0.05%	0.006%
15	3.444	717	732	750	rBV	23084	54417	2.83%	0.348%
16	3.778	834	836	839	rVB2	847	424	0.02%	0.003%
17	3.839	848	855	858	rBV2	739	832	0.04%	0.005%
18	3.984	896	900	902	rBV2	878	634	0.03%	0.004%
19	4.119	938	942	943	rBV	808	594	0.03%	0.004%
20	4.170	946	958	995	rBV2	188466	589230	30.63%	3.774%
21	4.563	1075	1080	1083	rBV2	906	904	0.05%	0.006%
22	4.643	1086	1105	1130	rBV	317915	759481	39.48%	4.864%
23	4.855	1167	1171	1172	rBV3	909	662	0.03%	0.004%
24	4.910	1176	1188	1201	rVB6	6971	17186	0.89%	0.110%
25	5.042	1223	1229	1231	rBV3	688	712	0.04%	0.005%
26	5.058	1231	1234	1238	rVB2	704	516	0.03%	0.003%
27	5.103	1246	1248	1254	rVB2	792	607	0.03%	0.004%
28	5.334	1297	1320	1344	rBV2	639394	1923702	100.00%	12.320%
29	5.669	1421	1424	1429	rBV4	614	627	0.03%	0.004%
30	5.688	1429	1430	1435	rVB3	782	476	0.02%	0.003%
31	5.736	1441	1445	1446	rBV	778	579	0.03%	0.004%
32	5.771	1453	1456	1457	rBV2	824	427	0.02%	0.003%
33	5.881	1475	1490	1518	rBV	552066	1119698	58.21%	7.171%
34	6.180	1569	1583	1608	rBV	606690	1204990	62.64%	7.717%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031185.D
 Acq On : 14 Apr 2019 02:47
 Operator : JC/SP
 Sample : K2339-13DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC36DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.325	1615	1628	1648	rBV	426718	857714	44.59%	5.493%
36	6.514	1684	1687	1693	rVB6	1155	1156	0.06%	0.007%
37	6.556	1698	1700	1703	rVB2	715	441	0.02%	0.003%
38	6.591	1709	1711	1714	rBV2	643	427	0.02%	0.003%
39	6.662	1731	1733	1740	rVB4	1107	1139	0.06%	0.007%
40	6.842	1784	1789	1793	rVB5	563	556	0.03%	0.004%
41	7.141	1878	1882	1886	rBV2	631	544	0.03%	0.003%
42	7.225	1896	1908	1927	rBV2	217330	392399	20.40%	2.513%
43	7.562	1994	2013	2042	rBV	743127	1340175	69.67%	8.583%
44	7.845	2090	2101	2124	rBV	142935	257276	13.37%	1.648%
45	8.064	2167	2169	2173	rBV3	686	467	0.02%	0.003%
46	8.160	2196	2199	2201	rBV3	1105	705	0.04%	0.005%
47	8.183	2204	2206	2210	rVB2	1553	848	0.04%	0.005%
48	8.228	2214	2220	2225	rBV6	2018	2513	0.13%	0.016%
49	8.308	2233	2245	2280	rBV	554587	1085851	56.45%	6.954%
50	8.550	2317	2320	2322	rBV3	784	491	0.03%	0.003%
51	8.768	2386	2388	2391	rBV4	888	493	0.03%	0.003%
52	8.820	2400	2404	2408	rBV3	546	613	0.03%	0.004%
53	9.086	2474	2487	2514	rBV	780374	1341946	69.76%	8.594%
54	9.276	2543	2546	2549	rBV3	1008	740	0.04%	0.005%
55	9.347	2563	2568	2574	rBV5	882	1183	0.06%	0.008%
56	9.640	2657	2659	2665	rVB2	934	682	0.04%	0.004%
57	9.672	2665	2669	2675	rBV2	757	988	0.05%	0.006%
58	9.730	2685	2687	2691	rVB	1131	677	0.04%	0.004%
59	9.775	2697	2701	2704	rVV2	774	596	0.03%	0.004%
60	9.810	2709	2712	2716	rVB2	764	494	0.03%	0.003%
61	9.871	2727	2731	2733	rBV2	692	432	0.02%	0.003%
62	9.916	2742	2745	2748	rBV2	858	562	0.03%	0.004%
63	9.939	2749	2752	2756	rBV3	711	645	0.03%	0.004%
64	9.980	2761	2765	2768	rBV2	514	543	0.03%	0.003%
65	10.067	2787	2792	2798	rBV4	948	914	0.05%	0.006%
66	10.202	2830	2834	2838	rBV2	797	785	0.04%	0.005%
67	10.337	2872	2876	2881	rVB3	992	1001	0.05%	0.006%
68	10.373	2883	2887	2890	rBV2	643	419	0.02%	0.003%
69	10.427	2890	2904	2926	rBV	591868	963900	50.11%	6.173%
70	10.598	2954	2957	2960	rBV4	993	732	0.04%	0.005%
71	10.742	3000	3002	3010	rVB3	743	623	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031185.D
 Acq On : 14 Apr 2019 02:47
 Operator : JC/SP
 Sample : K2339-13DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC36DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.845	3027	3034	3036	rVV3	549	566	0.03%	0.004%
73	11.003	3079	3083	3087	rBV4	589	688	0.04%	0.004%
74	11.479	3220	3231	3257	rBV	614025	1013102	52.66%	6.488%
75	11.858	3334	3349	3370	rBV	651611	1103420	57.36%	7.067%
76	12.141	3434	3437	3443	rBV5	977	823	0.04%	0.005%
77	12.266	3473	3476	3482	rBV4	830	616	0.03%	0.004%
78	12.360	3500	3505	3511	rBV3	877	1039	0.05%	0.007%
79	12.488	3543	3545	3550	rVB2	1121	782	0.04%	0.005%
80	12.620	3583	3586	3591	rVB2	672	611	0.03%	0.004%
81	12.929	3680	3682	3684	rBV2	801	462	0.02%	0.003%
82	13.009	3704	3707	3710	rBV2	732	438	0.02%	0.003%
83	13.041	3713	3717	3720	rBV3	672	608	0.03%	0.004%
84	13.202	3764	3767	3770	rBV2	809	623	0.03%	0.004%
85	13.266	3784	3787	3791	rBV2	1029	737	0.04%	0.005%
86	13.498	3856	3859	3866	rVB2	971	968	0.05%	0.006%
87	13.540	3870	3872	3879	rVV2	1128	892	0.05%	0.006%
88	13.581	3882	3885	3888	rVV3	886	512	0.03%	0.003%
89	13.906	3982	3986	3988	rBV2	1034	912	0.05%	0.006%
90	14.395	4134	4138	4141	rBV3	1151	953	0.05%	0.006%
91	14.517	4172	4176	4182	rBV5	1013	1437	0.07%	0.009%
92	14.591	4196	4199	4202	rBV3	979	747	0.04%	0.005%
93	14.733	4241	4243	4245	rBV3	842	427	0.02%	0.003%
94	14.761	4250	4252	4253	rBV	1055	489	0.03%	0.003%
95	14.877	4286	4288	4292	rVB2	1130	509	0.03%	0.003%
96	14.903	4293	4296	4301	rVV4	1424	1142	0.06%	0.007%
97	14.993	4320	4324	4326	rBV	1158	932	0.05%	0.006%
98	15.196	4384	4387	4393	rVB4	1703	1965	0.10%	0.013%
99	15.228	4394	4397	4401	rBV3	1358	1207	0.06%	0.008%
100	15.424	4455	4458	4462	rBV3	1480	1051	0.05%	0.007%


Sum of corrected areas: 15614682

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031185.D
Acq On : 14 Apr 2019 02:47
Operator : JC/SP
Sample : K2339-13DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC36DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

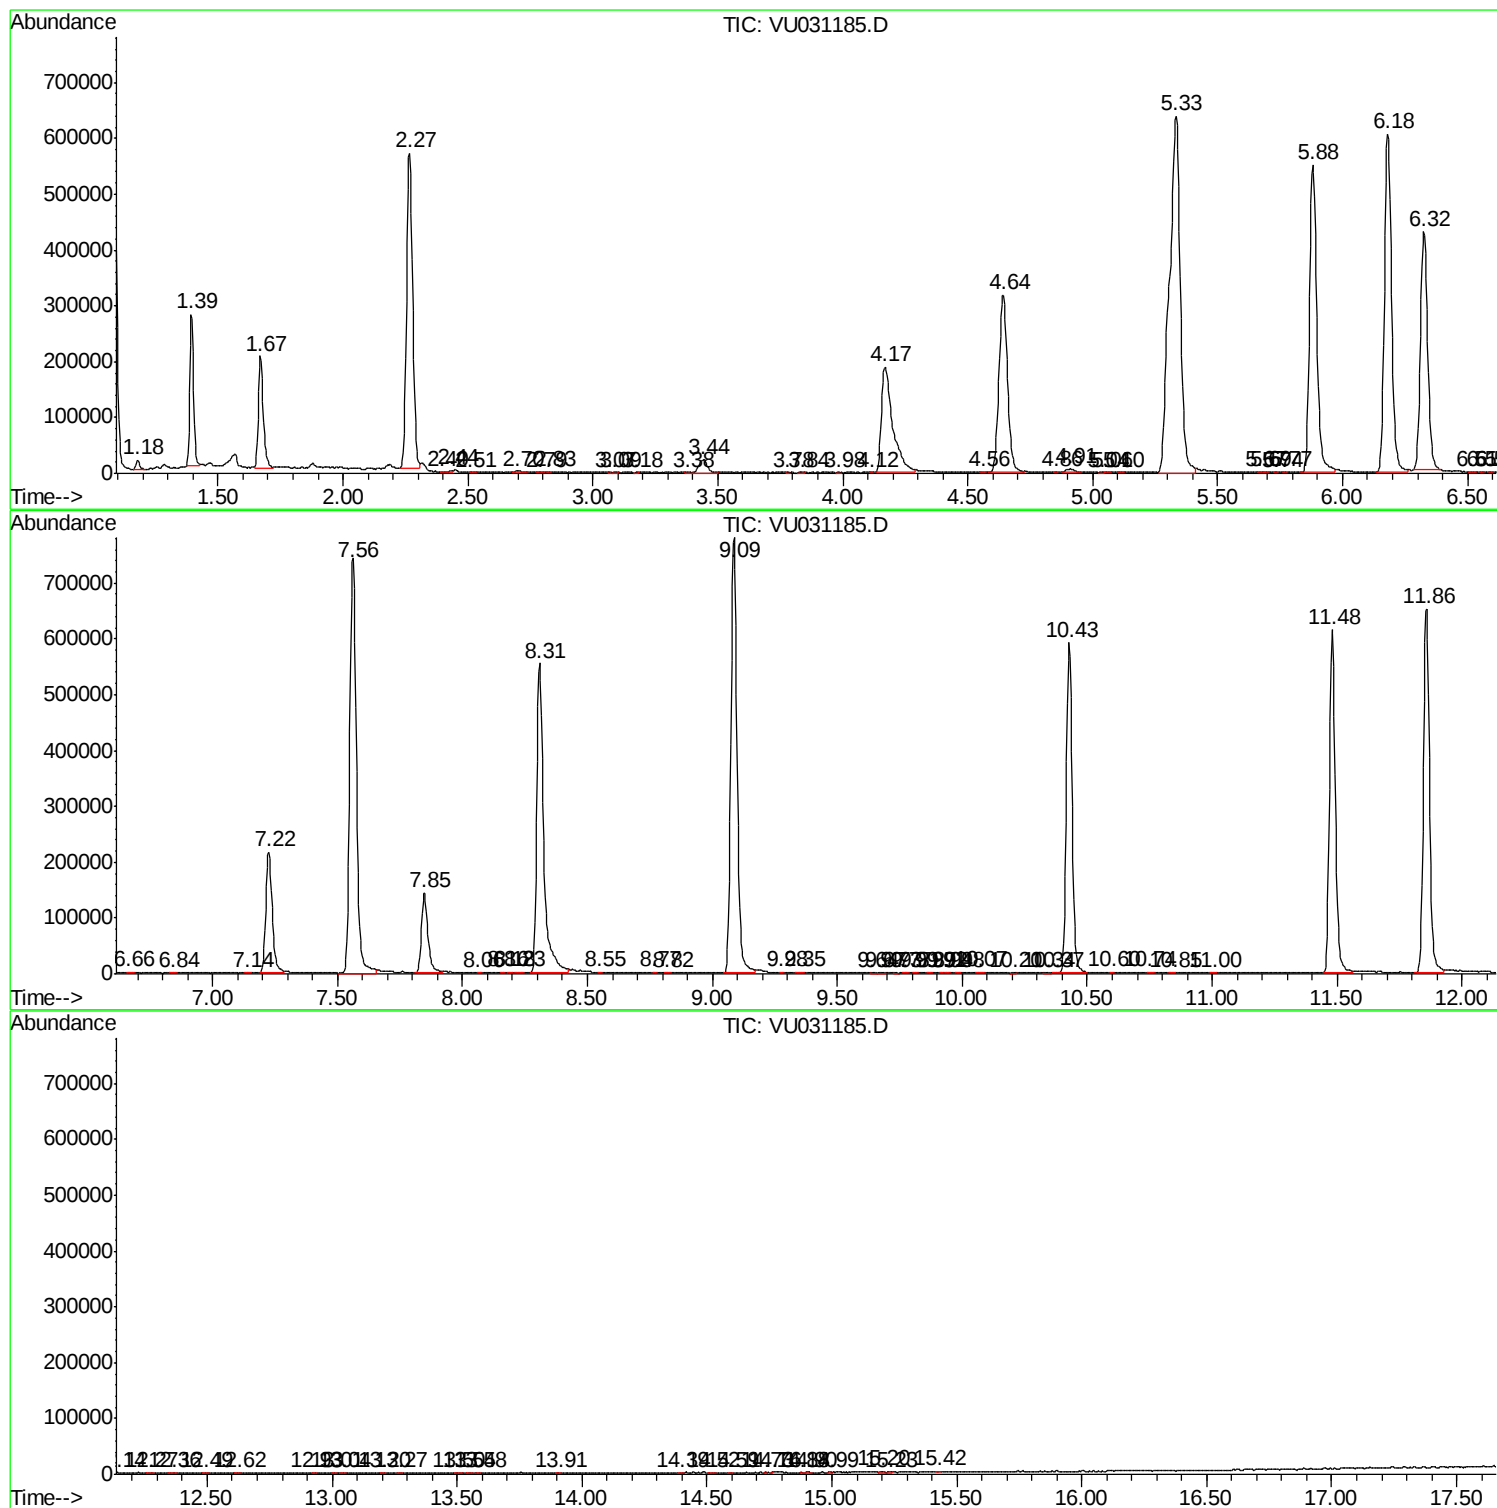

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031185.D
Acq On : 14 Apr 2019 02:47
Operator : JC/SP
Sample : K2339-13DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC36DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031185.D
Acq On : 14 Apr 2019 02:47
Operator : JC/SP
Sample : K2339-13DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC36DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc