

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031186.D
 Acq On : 14 Apr 2019 03:11
 Operator : JC/SP
 Sample : K2339-14DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC37DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	34	rVB2	14983	14259	0.73%	0.095%
2	1.392	87	94	111	rBV	279787	305577	15.66%	2.033%
3	1.672	173	181	198	rVB	204112	273302	14.00%	1.818%
4	2.264	355	365	380	rVB	520105	771363	39.52%	5.132%
5	2.389	400	404	406	rVB3	975	622	0.03%	0.004%
6	2.434	414	418	420	rBV3	2335	1991	0.10%	0.013%
7	2.543	448	452	459	rBV4	1050	1388	0.07%	0.009%
8	2.691	492	498	500	rBV3	1789	1666	0.09%	0.011%
9	2.826	535	540	541	rBV	1235	742	0.04%	0.005%
10	2.878	554	556	563	rVB2	1056	636	0.03%	0.004%
11	3.006	588	596	600	rBV3	623	1011	0.05%	0.007%
12	3.119	626	631	636	rBV3	645	801	0.04%	0.005%
13	3.180	647	650	653	rBV2	596	519	0.03%	0.003%
14	3.482	742	744	748	rVB2	786	444	0.02%	0.003%
15	3.511	748	753	756	rBV2	753	801	0.04%	0.005%
16	3.633	787	791	796	rVB3	514	498	0.03%	0.003%
17	3.698	806	811	813	rBV2	759	543	0.03%	0.004%
18	3.775	828	835	836	rBV	505	503	0.03%	0.003%
19	3.817	845	848	850	rBV	641	449	0.02%	0.003%
20	3.849	854	858	864	rVB3	815	975	0.05%	0.006%
21	3.878	864	867	872	rBV2	560	477	0.02%	0.003%
22	3.916	872	879	882	rBV3	638	727	0.04%	0.005%
23	4.064	921	925	929	rBV2	518	478	0.02%	0.003%
24	4.170	944	958	990	rBV	200406	553513	28.36%	3.683%
25	4.537	1070	1072	1074	rBV	820	521	0.03%	0.003%
26	4.640	1087	1104	1128	rBV	315619	774782	39.69%	5.155%
27	4.865	1172	1174	1177	rBV3	689	555	0.03%	0.004%
28	4.990	1208	1213	1216	rBV3	696	594	0.03%	0.004%
29	5.048	1227	1231	1234	rVB2	1158	718	0.04%	0.005%
30	5.157	1262	1265	1270	rVB5	629	607	0.03%	0.004%
31	5.186	1270	1274	1277	rBV2	652	443	0.02%	0.003%
32	5.334	1294	1320	1343	rBV2	656305	1951928	100.00%	12.988%
33	5.592	1397	1400	1402	rBV3	1150	819	0.04%	0.005%
34	5.646	1414	1417	1422	rBV4	793	772	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031186.D
 Acq On : 14 Apr 2019 03:11
 Operator : JC/SP
 Sample : K2339-14DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC37DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.733	1438	1444	1445	rBV3	690	606	0.03%	0.004%
36	5.881	1477	1490	1509	rBV	573224	1128593	57.82%	7.509%
37	6.122	1562	1565	1568	rBV3	655	593	0.03%	0.004%
38	6.183	1571	1584	1603	rBV	240892	476171	24.39%	3.168%
39	6.325	1614	1628	1654	rBV	433535	880466	45.11%	5.858%
40	6.743	1755	1758	1761	rBV3	789	712	0.04%	0.005%
41	6.810	1775	1779	1782	rVB3	631	459	0.02%	0.003%
42	6.855	1790	1793	1795	rBV2	708	569	0.03%	0.004%
43	6.891	1800	1804	1811	rBV2	1183	1212	0.06%	0.008%
44	6.952	1820	1823	1826	rBV	796	493	0.03%	0.003%
45	7.035	1844	1849	1853	rBV2	822	862	0.04%	0.006%
46	7.173	1885	1892	1894	rBV	761	713	0.04%	0.005%
47	7.225	1896	1908	1935	rBV	219174	407544	20.88%	2.712%
48	7.447	1974	1977	1979	rBV2	748	498	0.03%	0.003%
49	7.559	1999	2012	2032	rBV	797965	1433862	73.46%	9.541%
50	7.846	2089	2101	2122	rBV	147566	267555	13.71%	1.780%
51	7.984	2141	2144	2147	rBV3	938	631	0.03%	0.004%
52	8.019	2153	2155	2160	rVB4	977	775	0.04%	0.005%
53	8.228	2217	2220	2222	rBV3	1127	632	0.03%	0.004%
54	8.309	2231	2245	2281	rBV	581869	1140969	58.45%	7.592%
55	8.656	2351	2353	2355	rBV3	876	479	0.02%	0.003%
56	8.694	2362	2365	2369	rVB3	703	439	0.02%	0.003%
57	8.916	2431	2434	2435	rBV2	784	492	0.03%	0.003%
58	8.977	2449	2453	2455	rBV3	874	655	0.03%	0.004%
59	9.006	2457	2462	2463	rBV3	621	522	0.03%	0.003%
60	9.087	2474	2487	2508	rBV	824824	1400258	71.74%	9.317%
61	9.389	2578	2581	2587	rVB4	1186	899	0.05%	0.006%
62	9.431	2589	2594	2595	rBV2	946	806	0.04%	0.005%
63	9.505	2613	2617	2620	rBV3	578	483	0.02%	0.003%
64	9.601	2643	2647	2650	rBV2	713	657	0.03%	0.004%
65	9.672	2665	2669	2671	rBV3	609	455	0.02%	0.003%
66	9.836	2718	2720	2724	rVB3	707	473	0.02%	0.003%
67	9.907	2736	2742	2747	rBV4	1230	1205	0.06%	0.008%
68	9.952	2752	2756	2761	rBV2	789	942	0.05%	0.006%
69	9.980	2762	2765	2768	rVB	742	467	0.02%	0.003%
70	10.344	2874	2878	2879	rBV	776	454	0.02%	0.003%
71	10.427	2891	2904	2929	rBV	609948	983339	50.38%	6.543%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031186.D
 Acq On : 14 Apr 2019 03:11
 Operator : JC/SP
 Sample : K2339-14DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC37DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.524	2930	2934	2939	rVB3	839	965	0.05%	0.006%
73	10.566	2945	2947	2952	rVB2	1373	1163	0.06%	0.008%
74	10.601	2952	2958	2966	rBV5	1480	2656	0.14%	0.018%
75	10.749	3001	3004	3007	rVB2	860	552	0.03%	0.004%
76	10.794	3015	3018	3021	rBV3	908	587	0.03%	0.004%
77	10.826	3024	3028	3031	rBV3	507	455	0.02%	0.003%
78	10.887	3042	3047	3050	rBV3	953	626	0.03%	0.004%
79	10.913	3052	3055	3060	rVB3	605	506	0.03%	0.003%
80	10.939	3060	3063	3068	rBV4	810	667	0.03%	0.004%
81	11.138	3122	3125	3128	rVB3	824	577	0.03%	0.004%
82	11.177	3128	3137	3139	rBV2	821	1054	0.05%	0.007%
83	11.482	3220	3232	3250	rBV	646799	1053828	53.99%	7.012%
84	11.855	3336	3348	3373	rBV	665986	1148869	58.86%	7.644%
85	12.199	3452	3455	3458	rBV3	794	748	0.04%	0.005%
86	12.238	3464	3467	3472	rVB4	1115	1195	0.06%	0.008%
87	12.379	3508	3511	3516	rBV2	1668	1918	0.10%	0.013%
88	12.466	3535	3538	3541	rBV3	770	675	0.03%	0.004%
89	12.508	3548	3551	3557	rBV4	1024	1128	0.06%	0.008%
90	12.533	3557	3559	3562	rVB3	968	525	0.03%	0.003%
91	12.556	3562	3566	3570	rBV2	879	1046	0.05%	0.007%
92	13.151	3749	3751	3755	rVB2	764	444	0.02%	0.003%
93	13.334	3805	3808	3812	rBV3	1091	1194	0.06%	0.008%
94	13.366	3816	3818	3821	rBV2	811	573	0.03%	0.004%
95	13.543	3871	3873	3879	rVB2	855	578	0.03%	0.004%
96	13.797	3948	3952	3954	rBV3	1235	860	0.04%	0.006%
97	14.090	4040	4043	4046	rBV2	719	601	0.03%	0.004%
98	14.434	4146	4150	4152	rBV2	1550	1179	0.06%	0.008%
99	14.665	4219	4222	4225	rBV4	1149	971	0.05%	0.006%
100	15.180	4380	4382	4385	rBV	1190	896	0.05%	0.006%


Sum of corrected areas: 15029000

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031186.D
Acq On : 14 Apr 2019 03:11
Operator : JC/SP
Sample : K2339-14DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC37DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

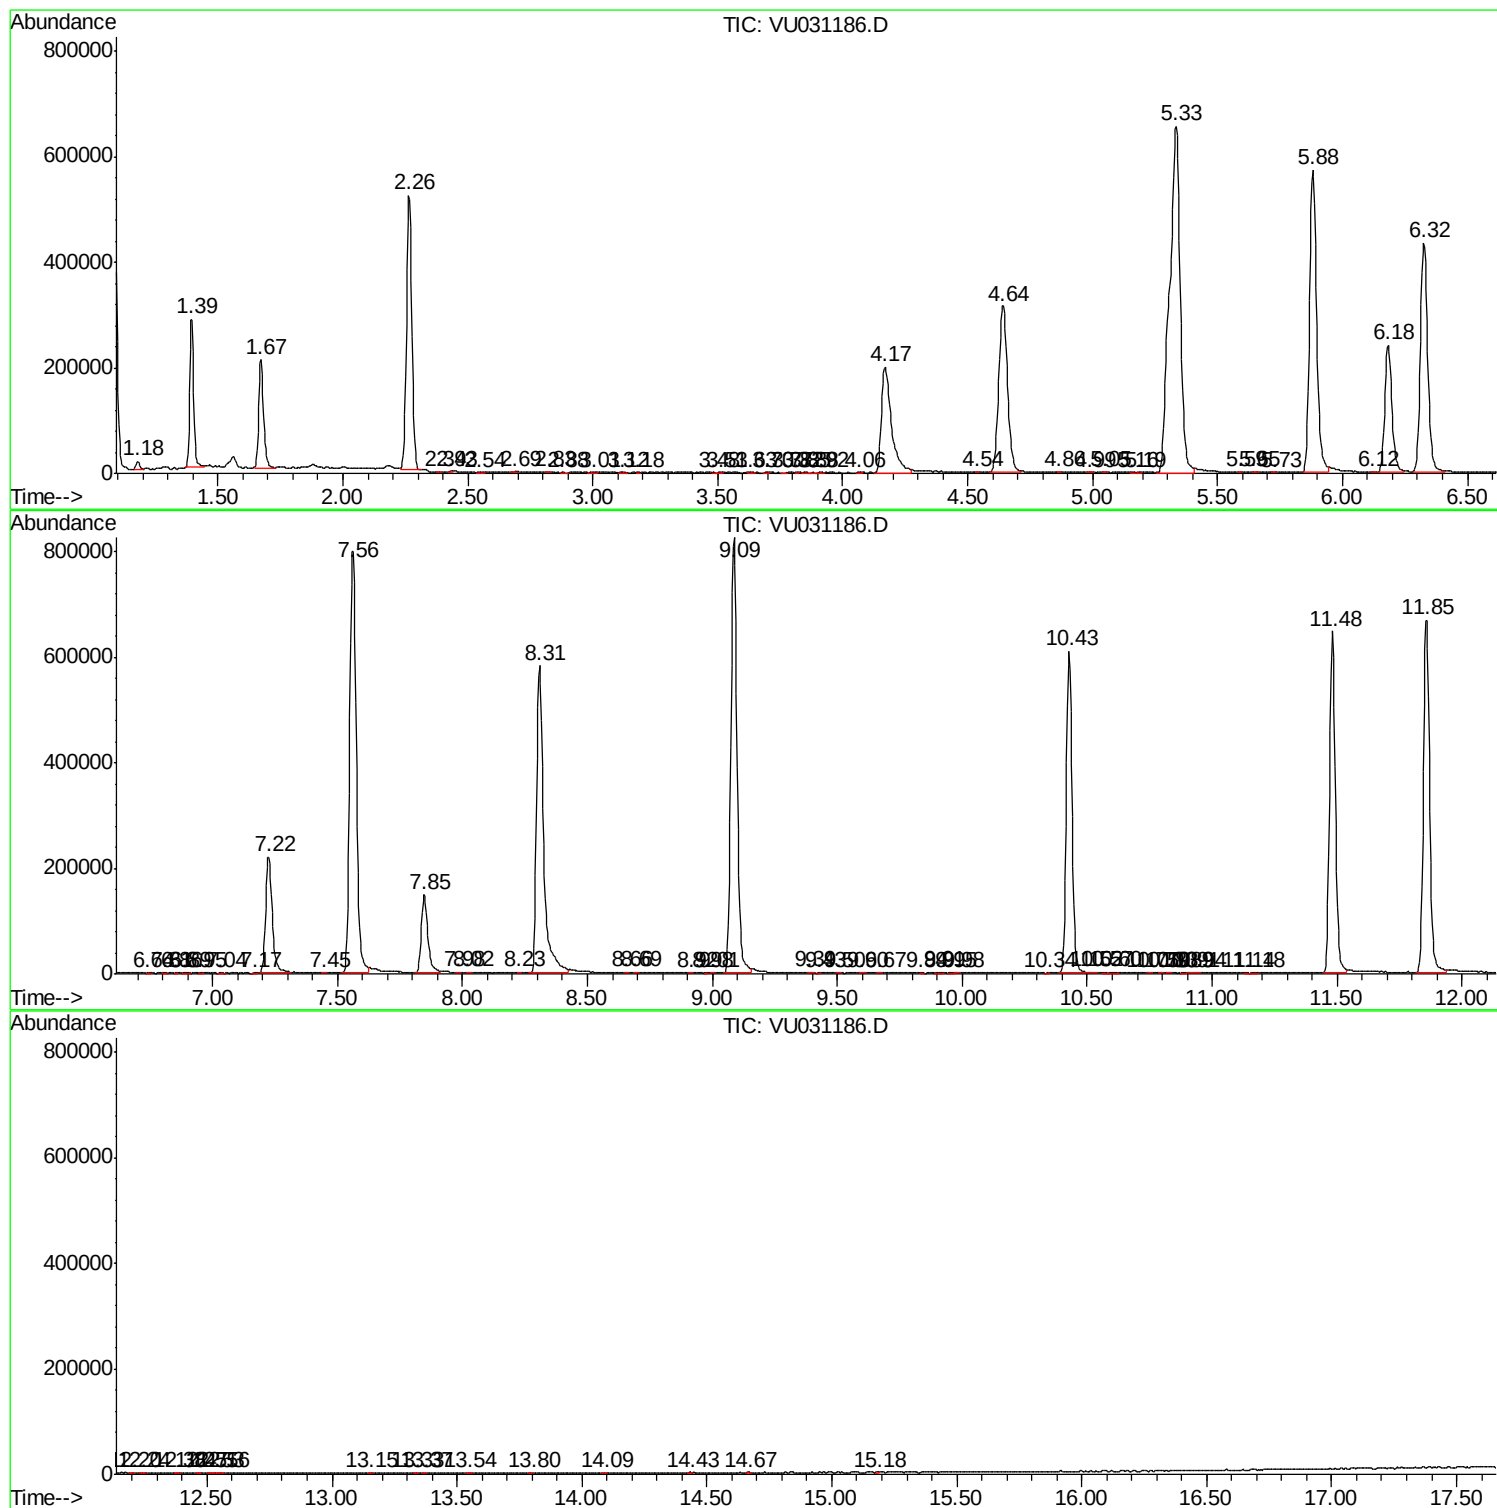

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031186.D
Acq On : 14 Apr 2019 03:11
Operator : JC/SP
Sample : K2339-14DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC37DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031186.D
Acq On : 14 Apr 2019 03:11
Operator : JC/SP
Sample : K2339-14DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC37DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc