

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031187.D
 Acq On : 14 Apr 2019 03:34
 Operator : JC/SP
 Sample : K2339-11DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC34DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	33	rBV2	12821	11736	0.18%	0.058%
2	1.395	88	95	106	rBV	290695	302163	4.64%	1.506%
3	1.672	173	181	195	rBV	216404	296092	4.55%	1.475%
4	2.267	355	366	379	rVB2	534657	845193	12.99%	4.212%
5	2.415	409	412	414	rBV2	1284	737	0.01%	0.004%
6	2.701	494	501	507	rVV9	2278	3737	0.06%	0.019%
7	2.733	509	511	515	rVB2	903	725	0.01%	0.004%
8	2.823	537	539	544	rVB4	654	520	0.01%	0.003%
9	3.109	622	628	630	rVB3	525	525	0.01%	0.003%
10	3.379	709	712	715	rBV2	1131	709	0.01%	0.004%
11	3.434	725	729	734	rBV4	1440	1467	0.02%	0.007%
12	3.527	753	758	762	rVV3	565	589	0.01%	0.003%
13	3.710	811	815	820	rVB2	585	531	0.01%	0.003%
14	3.791	835	840	845	rBV3	649	801	0.01%	0.004%
15	3.874	859	866	870	rBV2	712	723	0.01%	0.004%
16	4.083	928	931	934	rBV2	980	653	0.01%	0.003%
17	4.170	946	958	966	rBV2	179073	422579	6.50%	2.106%
18	4.640	1087	1104	1129	rBV	294213	714163	10.98%	3.559%
19	4.865	1170	1174	1175	rBV3	1230	867	0.01%	0.004%
20	4.910	1176	1188	1203	rVB4	10568	23850	0.37%	0.119%
21	4.990	1211	1213	1217	rVB4	1187	760	0.01%	0.004%
22	5.218	1279	1284	1289	rVB2	494	529	0.01%	0.003%
23	5.334	1296	1320	1354	rBV2	589613	1781534	27.38%	8.878%
24	5.636	1409	1414	1418	rBV4	1110	909	0.01%	0.005%
25	5.746	1444	1448	1450	rBV3	876	560	0.01%	0.003%
26	5.881	1477	1490	1514	rBV	525315	1061074	16.31%	5.288%
27	6.180	1568	1583	1615	rBV	3418281	6505904	100.00%	32.420%
28	6.324	1617	1628	1654	rVB	396229	816168	12.55%	4.067%
29	6.630	1719	1723	1725	rBV4	1460	1316	0.02%	0.007%
30	6.781	1767	1770	1775	rVV3	931	665	0.01%	0.003%
31	6.810	1775	1779	1783	rVB3	661	576	0.01%	0.003%
32	6.832	1783	1786	1789	rBV2	651	561	0.01%	0.003%
33	6.916	1807	1812	1813	rBV2	1077	646	0.01%	0.003%
34	7.013	1835	1842	1847	rBV4	801	1148	0.02%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031187.D
 Acq On : 14 Apr 2019 03:34
 Operator : JC/SP
 Sample : K2339-11DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC34DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	7.054	1852	1855	1859	rVB	824	561	0.01%	0.003%
36	7.225	1896	1908	1933	rBV2	204749	375996	5.78%	1.874%
37	7.562	1996	2013	2036	rBV	738643	1322011	20.32%	6.588%
38	7.845	2090	2101	2118	rBV2	133764	239078	3.67%	1.191%
39	8.093	2173	2178	2179	rBV2	1047	814	0.01%	0.004%
40	8.164	2194	2200	2201	rBV3	703	600	0.01%	0.003%
41	8.228	2211	2220	2228	rBV9	5256	10142	0.16%	0.051%
42	8.308	2234	2245	2284	rBV	532494	1042398	16.02%	5.194%
43	8.482	2296	2299	2303	rVB5	1838	1494	0.02%	0.007%
44	8.501	2303	2305	2308	rBV2	1429	759	0.01%	0.004%
45	8.533	2313	2315	2328	rVB8	2750	3863	0.06%	0.019%
46	8.620	2340	2342	2346	rVB3	1118	595	0.01%	0.003%
47	8.707	2365	2369	2374	rBV4	1304	1101	0.02%	0.005%
48	8.729	2374	2376	2379	rVB2	978	505	0.01%	0.003%
49	8.746	2379	2381	2387	rBV3	798	736	0.01%	0.004%
50	8.810	2398	2401	2405	rVB	1162	864	0.01%	0.004%
51	8.839	2405	2410	2412	rBV2	1229	765	0.01%	0.004%
52	8.987	2453	2456	2460	rBV3	1080	919	0.01%	0.005%
53	9.086	2473	2487	2511	rBV	761754	1293588	19.88%	6.446%
54	9.318	2555	2559	2560	rBV2	967	676	0.01%	0.003%
55	9.385	2576	2580	2582	rBV2	830	630	0.01%	0.003%
56	9.456	2600	2602	2606	rVB3	647	504	0.01%	0.003%
57	9.504	2614	2617	2623	rVB3	982	846	0.01%	0.004%
58	9.537	2623	2627	2630	rBV2	564	525	0.01%	0.003%
59	9.565	2630	2636	2639	rBV3	494	626	0.01%	0.003%
60	9.768	2695	2699	2704	rVV3	659	608	0.01%	0.003%
61	9.890	2733	2737	2741	rBV2	648	594	0.01%	0.003%
62	9.929	2747	2749	2752	rBV2	882	497	0.01%	0.002%
63	10.167	2821	2823	2829	rBV3	681	587	0.01%	0.003%
64	10.311	2863	2868	2874	rBV3	510	550	0.01%	0.003%
65	10.356	2878	2882	2887	rBV3	805	871	0.01%	0.004%
66	10.389	2887	2892	2893	rBV3	699	576	0.01%	0.003%
67	10.427	2893	2904	2928	rVV	543387	886822	13.63%	4.419%
68	10.604	2953	2959	2965	rVB5	1968	2462	0.04%	0.012%
69	10.636	2965	2969	2973	rBV2	687	663	0.01%	0.003%
70	10.668	2976	2979	2984	rBV4	910	842	0.01%	0.004%
71	10.720	2991	2995	2996	rBV	760	494	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031187.D
 Acq On : 14 Apr 2019 03:34
 Operator : JC/SP
 Sample : K2339-11DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC34DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.868	3037	3041	3047	rVB3	1013	1030	0.02%	0.005%
73	10.906	3047	3053	3057	rBV3	940	1048	0.02%	0.005%
74	10.935	3057	3062	3069	rBV2	837	1035	0.02%	0.005%
75	11.099	3110	3113	3118	rVB3	710	498	0.01%	0.002%
76	11.199	3138	3144	3146	rBV2	701	754	0.01%	0.004%
77	11.482	3219	3232	3255	rBV	611182	1010665	15.53%	5.036%
78	11.858	3336	3349	3370	rBV	622303	1036893	15.94%	5.167%
79	12.154	3436	3441	3443	rBV4	1036	992	0.02%	0.005%
80	12.257	3471	3473	3476	rBV3	841	644	0.01%	0.003%
81	12.318	3487	3492	3495	rBV3	1236	1137	0.02%	0.006%
82	12.372	3506	3509	3512	rBV3	621	547	0.01%	0.003%
83	12.495	3544	3547	3551	rVB4	1445	1083	0.02%	0.005%
84	12.588	3572	3576	3579	rVV	769	770	0.01%	0.004%
85	12.662	3596	3599	3606	rVB3	999	896	0.01%	0.004%
86	12.733	3614	3621	3624	rBV4	1649	2016	0.03%	0.010%
87	12.803	3638	3643	3646	rBV2	857	848	0.01%	0.004%
88	12.858	3656	3660	3662	rBV3	595	520	0.01%	0.003%
89	12.919	3673	3679	3681	rBV	605	712	0.01%	0.004%
90	12.970	3692	3695	3699	rBV2	1345	948	0.01%	0.005%
91	12.990	3699	3701	3706	rVB	822	651	0.01%	0.003%
92	13.392	3823	3826	3830	rVB2	1027	834	0.01%	0.004%
93	13.626	3896	3899	3904	rBV	763	577	0.01%	0.003%
94	13.890	3978	3981	3987	rVB	1586	1498	0.02%	0.007%
95	13.922	3987	3991	3993	rBV2	815	560	0.01%	0.003%
96	13.993	4011	4013	4016	rBV3	846	601	0.01%	0.003%
97	14.443	4150	4153	4156	rBV2	1037	778	0.01%	0.004%
98	15.038	4336	4338	4341	rBV	1059	646	0.01%	0.003%
99	15.237	4397	4400	4401	rBV2	1022	677	0.01%	0.003%
100	15.443	4461	4464	4465	rBV	1144	632	0.01%	0.003%


Sum of corrected areas: 20067362

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031187.D
Acq On : 14 Apr 2019 03:34
Operator : JC/SP
Sample : K2339-11DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

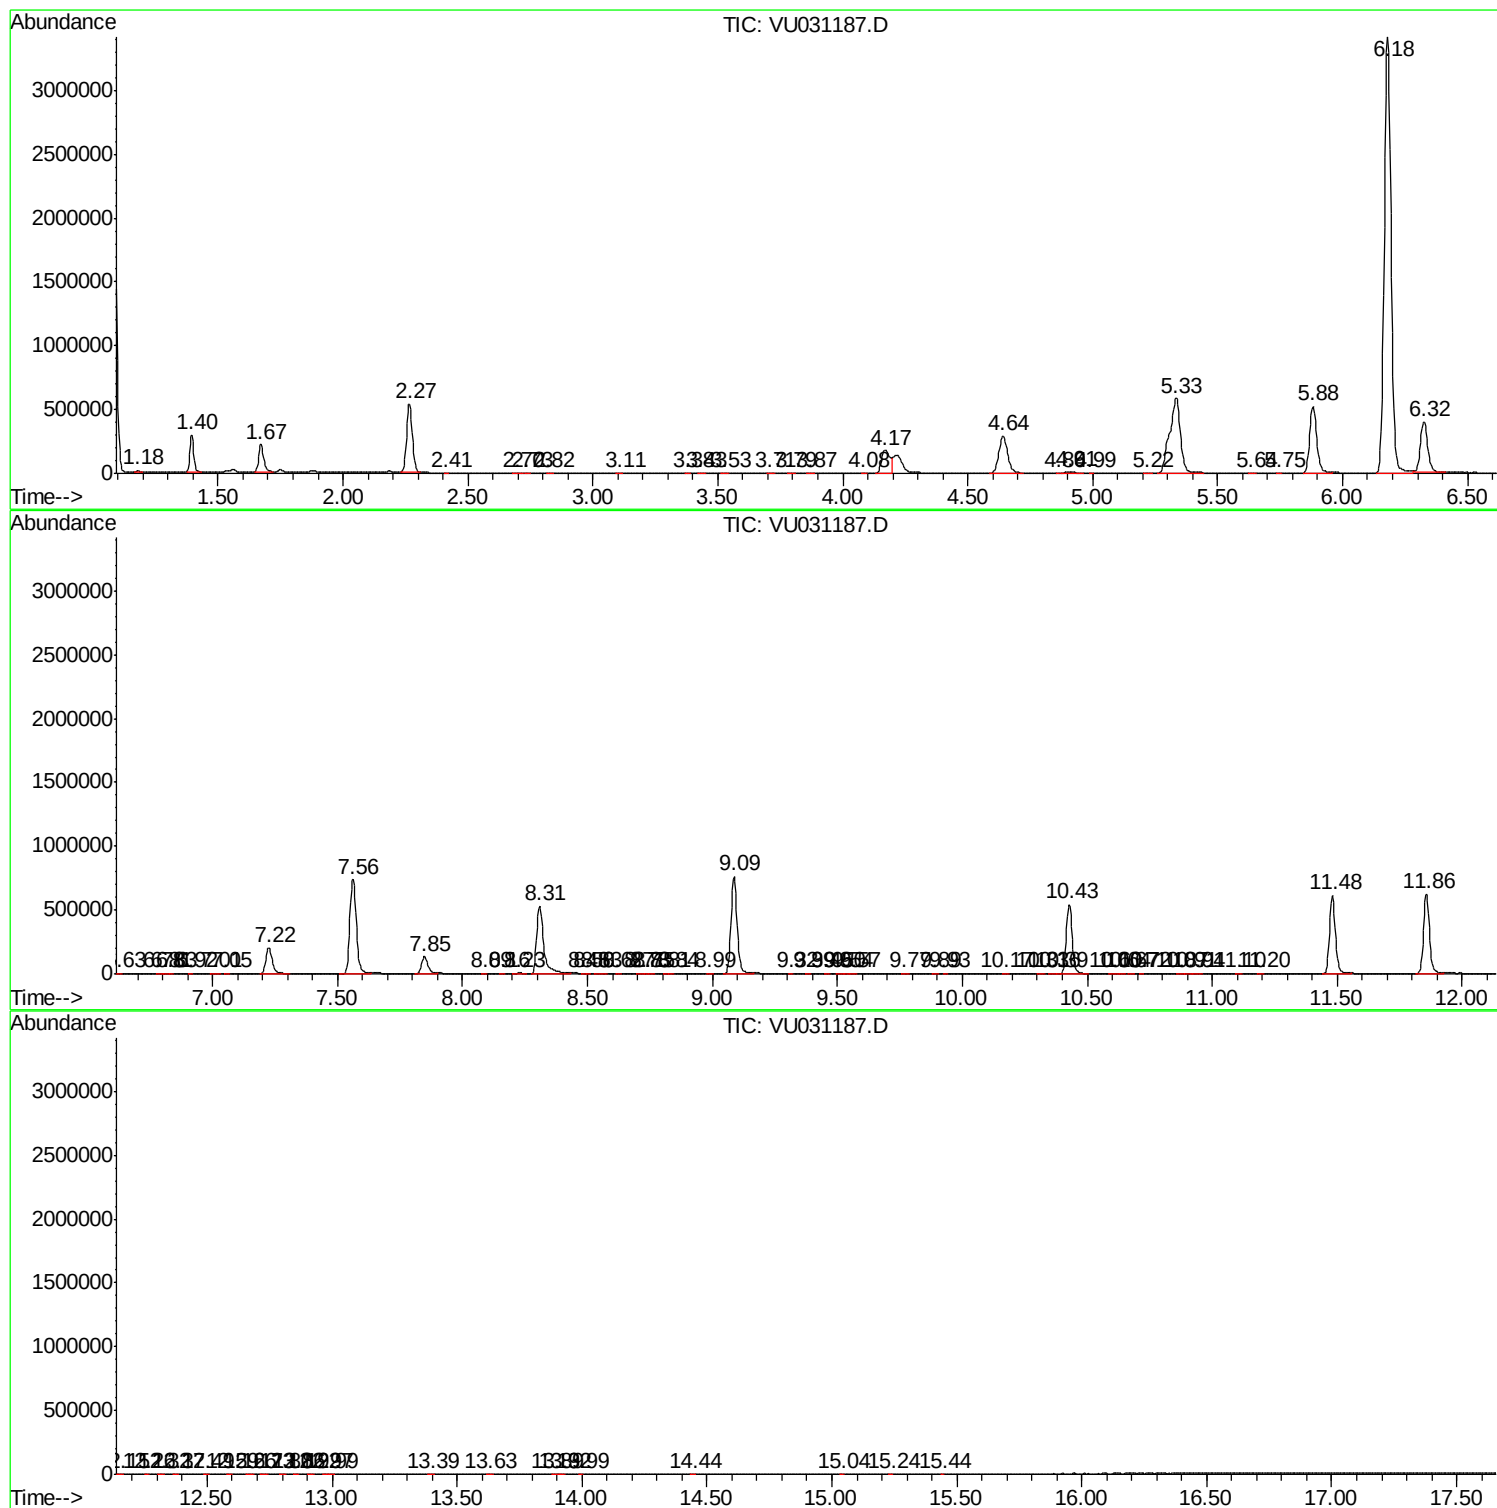

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031187.D
Acq On : 14 Apr 2019 03:34
Operator : JC/SP
Sample : K2339-11DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031187.D
Acq On : 14 Apr 2019 03:34
Operator : JC/SP
Sample : K2339-11DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc