

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031188.D
 Acq On : 14 Apr 2019 03:58
 Operator : JC/SP
 Sample : K2339-12DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rVB	12202	11977	0.09%	0.045%
2	1.395	87	95	107	rBV	253528	275300	2.08%	1.031%
3	1.672	173	181	198	rVB	253664	335783	2.53%	1.257%
4	2.267	355	366	381	rBV3	613337	1040926	7.86%	3.897%
5	2.694	494	499	507	rVB5	2491	3320	0.03%	0.012%
6	2.862	549	551	557	rVB3	1198	912	0.01%	0.003%
7	2.894	557	561	562	rBV	731	478	0.00%	0.002%
8	2.920	566	569	571	rBV2	924	602	0.00%	0.002%
9	2.977	584	587	590	rVB2	941	576	0.00%	0.002%
10	3.003	591	595	598	rVB5	856	611	0.00%	0.002%
11	3.026	599	602	605	rBV2	1039	593	0.00%	0.002%
12	3.444	724	732	740	rVB4	1327	2192	0.02%	0.008%
13	3.495	745	748	751	rBV2	671	507	0.00%	0.002%
14	4.170	944	958	986	rBV	181787	478875	3.61%	1.793%
15	4.473	1047	1052	1053	rBV2	629	520	0.00%	0.002%
16	4.640	1088	1104	1132	rVV	284929	695817	5.25%	2.605%
17	4.858	1169	1172	1175	rBV4	617	475	0.00%	0.002%
18	5.058	1231	1234	1236	rBV	731	508	0.00%	0.002%
19	5.334	1297	1320	1351	rBV2	572954	1735380	13.10%	6.497%
20	5.527	1378	1380	1384	rBV4	985	533	0.00%	0.002%
21	5.675	1423	1426	1430	rVB3	1202	785	0.01%	0.003%
22	5.765	1451	1454	1458	rVB2	903	624	0.00%	0.002%
23	5.881	1474	1490	1523	rBV	490912	1008058	7.61%	3.774%
24	6.180	1565	1583	1615	rBV	6976381	13248765	100.00%	49.601%
25	6.325	1617	1628	1655	rVB	405004	830442	6.27%	3.109%
26	6.620	1718	1720	1723	rBV3	790	523	0.00%	0.002%
27	6.800	1771	1776	1779	rBV3	825	712	0.01%	0.003%
28	6.842	1785	1789	1791	rBV2	642	558	0.00%	0.002%
29	6.900	1804	1807	1810	rBV2	716	548	0.00%	0.002%
30	7.029	1845	1847	1851	rVB	837	521	0.00%	0.002%
31	7.054	1851	1855	1860	rBV2	869	704	0.01%	0.003%
32	7.087	1861	1865	1868	rBV3	964	699	0.01%	0.003%
33	7.225	1895	1908	1928	rBV2	196681	366579	2.77%	1.372%
34	7.398	1959	1962	1967	rBV4	1181	1185	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031188.D
 Acq On : 14 Apr 2019 03:58
 Operator : JC/SP
 Sample : K2339-12DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	7.437	1970	1974	1979	rVB5	1587	1429	0.01%	0.005%
36	7.463	1979	1982	1984	rBV2	922	620	0.00%	0.002%
37	7.562	2000	2013	2034	rBV	715635	1278470	9.65%	4.786%
38	7.845	2090	2101	2122	rBV	132893	241197	1.82%	0.903%
39	8.003	2147	2150	2152	rBV3	731	494	0.00%	0.002%
40	8.054	2162	2166	2170	rBV6	774	691	0.01%	0.003%
41	8.234	2217	2222	2225	rBV5	1525	1351	0.01%	0.005%
42	8.308	2232	2245	2279	rBV	523118	1023499	7.73%	3.832%
43	8.627	2341	2344	2349	rVB3	1292	948	0.01%	0.004%
44	8.652	2349	2352	2356	rBV3	801	637	0.00%	0.002%
45	8.823	2401	2405	2408	rBV4	792	664	0.01%	0.002%
46	8.887	2421	2425	2428	rVV3	696	607	0.00%	0.002%
47	8.903	2428	2430	2433	rVV2	720	515	0.00%	0.002%
48	8.932	2437	2439	2443	rVV2	725	543	0.00%	0.002%
49	9.086	2472	2487	2511	rBV	715339	1225212	9.25%	4.587%
50	9.340	2562	2566	2569	rBV3	578	567	0.00%	0.002%
51	9.376	2569	2577	2580	rBV6	4789	5648	0.04%	0.021%
52	9.582	2636	2641	2645	rBV3	873	823	0.01%	0.003%
53	9.775	2695	2701	2702	rBV3	1832	1321	0.01%	0.005%
54	9.787	2702	2705	2709	rVB4	1791	1280	0.01%	0.005%
55	9.897	2736	2739	2746	rBV3	1205	1457	0.01%	0.005%
56	10.048	2783	2786	2791	rVB2	634	633	0.00%	0.002%
57	10.115	2804	2807	2810	rVB2	948	596	0.00%	0.002%
58	10.144	2810	2816	2820	rBV3	921	1069	0.01%	0.004%
59	10.373	2883	2887	2891	rVB2	1094	982	0.01%	0.004%
60	10.427	2891	2904	2927	rBV	543000	884677	6.68%	3.312%
61	10.604	2954	2959	2961	rBV5	1255	1272	0.01%	0.005%
62	10.652	2968	2974	2978	rBV3	793	786	0.01%	0.003%
63	10.762	3005	3008	3013	rVB	1037	661	0.00%	0.002%
64	10.820	3022	3026	3030	rBV4	635	549	0.00%	0.002%
65	10.858	3033	3038	3042	rVB2	856	744	0.01%	0.003%
66	10.996	3078	3081	3086	rVB2	894	699	0.01%	0.003%
67	11.029	3086	3091	3096	rVB3	794	989	0.01%	0.004%
68	11.067	3098	3103	3105	rBV3	872	667	0.01%	0.002%
69	11.196	3141	3143	3149	rVB2	760	723	0.01%	0.003%
70	11.231	3149	3154	3162	rBV5	1014	1281	0.01%	0.005%
71	11.311	3175	3179	3181	rBV	608	494	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031188.D
 Acq On : 14 Apr 2019 03:58
 Operator : JC/SP
 Sample : K2339-12DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	11.366	3193	3196	3203	rVV3	962	1159	0.01%	0.004%
73	11.401	3203	3207	3213	rVV3	543	577	0.00%	0.002%
74	11.482	3219	3232	3255	rBV	564002	936566	7.07%	3.506%
75	11.762	3315	3319	3321	rBV2	960	719	0.01%	0.003%
76	11.778	3321	3324	3331	rVV5	1062	1309	0.01%	0.005%
77	11.858	3336	3349	3364	rBV	600521	1019724	7.70%	3.818%
78	12.392	3513	3515	3522	rVV4	1253	1397	0.01%	0.005%
79	12.430	3523	3527	3530	rVB4	820	753	0.01%	0.003%
80	12.527	3553	3557	3561	rBV3	720	714	0.01%	0.003%
81	12.553	3562	3565	3569	rVV3	813	682	0.01%	0.003%
82	12.575	3570	3572	3577	rVB3	792	553	0.00%	0.002%
83	12.684	3603	3606	3609	rBV2	839	591	0.00%	0.002%
84	12.717	3612	3616	3619	rBV3	839	839	0.01%	0.003%
85	12.967	3691	3694	3700	rVB4	752	759	0.01%	0.003%
86	12.999	3700	3704	3707	rBV3	1093	817	0.01%	0.003%
87	13.051	3717	3720	3724	rVB	888	632	0.00%	0.002%
88	13.147	3747	3750	3752	rBV3	1024	612	0.00%	0.002%
89	13.170	3753	3757	3759	rBV3	1152	980	0.01%	0.004%
90	13.321	3802	3804	3807	rBV	978	647	0.00%	0.002%
91	13.424	3833	3836	3840	rBV3	805	792	0.01%	0.003%
92	13.646	3902	3905	3908	rBV3	770	540	0.00%	0.002%
93	13.726	3928	3930	3936	rBV3	913	723	0.01%	0.003%
94	14.244	4088	4091	4093	rBV	834	577	0.00%	0.002%
95	14.260	4093	4096	4099	rVV2	852	751	0.01%	0.003%
96	14.453	4154	4156	4161	rBV3	1085	1032	0.01%	0.004%
97	14.562	4187	4190	4194	rBV2	1111	957	0.01%	0.004%
98	15.273	4409	4411	4415	rBV2	907	737	0.01%	0.003%
99	15.694	4539	4542	4547	rBV4	1548	1294	0.01%	0.005%
100	16.568	4811	4814	4817	rBV5	2494	2066	0.02%	0.008%


Sum of corrected areas: 26710882

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031188.D
Acq On : 14 Apr 2019 03:58
Operator : JC/SP
Sample : K2339-12DL 400X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BFC35DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

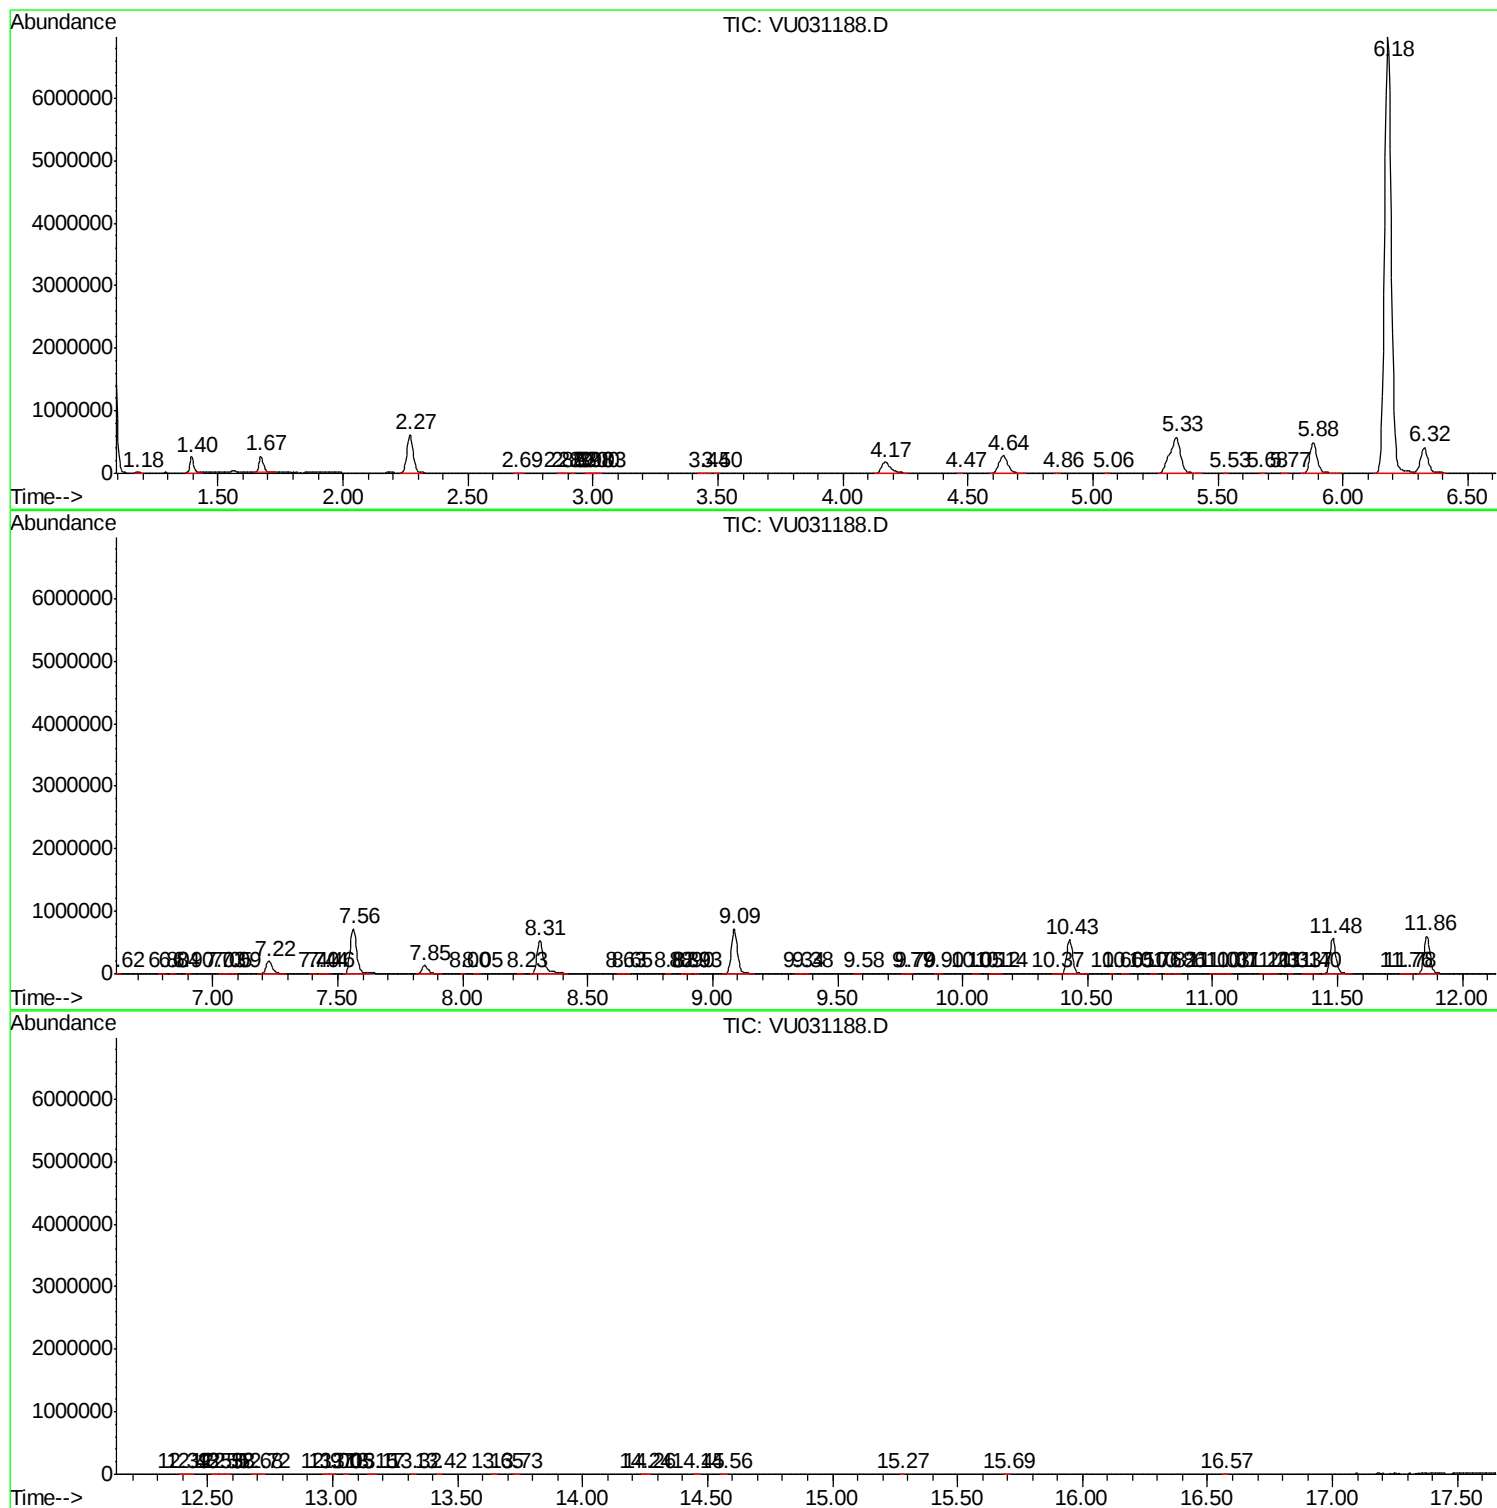

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031188.D
Acq On : 14 Apr 2019 03:58
Operator : JC/SP
Sample : K2339-12DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC35DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031188.D
Acq On : 14 Apr 2019 03:58
Operator : JC/SP
Sample : K2339-12DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC35DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc