

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031193.D
 Acq On : 14 Apr 2019 06:19
 Operator : JC/SP
 Sample : K2409-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	22	28	39	rVB	31728	31881	1.81%	0.235%
2	1.396	87	95	109	rBV	358056	392698	22.28%	2.892%
3	1.672	173	181	199	rVB	256393	352197	19.99%	2.594%
4	2.267	355	366	376	rBV	527297	813075	46.14%	5.987%
5	2.440	410	420	438	rBV	18458	35487	2.01%	0.261%
6	2.682	488	495	496	rBV3	1590	1239	0.07%	0.009%
7	2.833	530	542	549	rBV8	2023	4131	0.23%	0.030%
8	2.907	562	565	567	rBV2	776	428	0.02%	0.003%
9	2.968	579	584	586	rBV2	624	558	0.03%	0.004%
10	3.186	649	652	659	rBV4	550	528	0.03%	0.004%
11	3.296	683	686	689	rVV2	576	434	0.02%	0.003%
12	3.444	726	732	740	rVB6	1235	2049	0.12%	0.015%
13	3.556	760	767	770	rBV4	812	856	0.05%	0.006%
14	3.575	771	773	777	rVB	672	440	0.02%	0.003%
15	3.598	777	780	783	rBV	683	439	0.02%	0.003%
16	3.916	874	879	882	rBV4	520	433	0.02%	0.003%
17	3.939	882	886	890	rVB2	990	718	0.04%	0.005%
18	4.167	945	957	986	rBV	165956	459997	26.10%	3.387%
19	4.437	1039	1041	1045	rVB2	945	565	0.03%	0.004%
20	4.489	1053	1057	1059	rBV3	733	653	0.04%	0.005%
21	4.640	1087	1104	1126	rBV	295422	699311	39.68%	5.150%
22	4.768	1142	1144	1148	rVB4	891	541	0.03%	0.004%
23	4.810	1154	1157	1161	rVB3	725	535	0.03%	0.004%
24	4.839	1163	1166	1170	rVB2	795	574	0.03%	0.004%
25	4.945	1197	1199	1203	rVB3	908	538	0.03%	0.004%
26	5.055	1227	1233	1241	rVB4	817	1042	0.06%	0.008%
27	5.132	1255	1257	1262	rBV2	923	709	0.04%	0.005%
28	5.334	1296	1320	1353	rBV2	586652	1762201	100.00%	12.976%
29	5.591	1397	1400	1405	rVB4	1126	817	0.05%	0.006%
30	5.630	1409	1412	1416	rVB4	1225	960	0.05%	0.007%
31	5.672	1421	1425	1430	rBV4	941	955	0.05%	0.007%
32	5.800	1462	1465	1474	rVB3	1168	1503	0.09%	0.011%
33	5.881	1474	1490	1519	rBV	523332	1053229	59.77%	7.756%
34	6.186	1573	1585	1598	rBV5	21695	43580	2.47%	0.321%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031193.D
 Acq On : 14 Apr 2019 06:19
 Operator : JC/SP
 Sample : K2409-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.325	1613	1628	1652	rBV	391160	798683	45.32%	5.881%
36	6.620	1715	1720	1722	rBV2	653	501	0.03%	0.004%
37	6.646	1724	1728	1729	rBV	801	482	0.03%	0.004%
38	6.839	1785	1788	1792	rVB2	758	497	0.03%	0.004%
39	6.868	1792	1797	1799	rBV2	497	474	0.03%	0.003%
40	6.929	1814	1816	1823	rBV3	664	669	0.04%	0.005%
41	6.984	1829	1833	1837	rBV2	770	644	0.04%	0.005%
42	7.225	1896	1908	1932	rBV	191679	356869	20.25%	2.628%
43	7.482	1985	1988	1993	rVB4	1057	745	0.04%	0.005%
44	7.559	1997	2012	2031	rBV	721937	1290763	73.25%	9.505%
45	7.845	2091	2101	2120	rBV	135105	244586	13.88%	1.801%
46	8.119	2182	2186	2189	rVB2	759	556	0.03%	0.004%
47	8.308	2232	2245	2277	rBV2	497545	999459	56.72%	7.360%
48	8.701	2364	2367	2369	rVV2	915	426	0.02%	0.003%
49	8.714	2369	2371	2375	rVB3	810	440	0.02%	0.003%
50	8.742	2378	2380	2384	rVB2	907	504	0.03%	0.004%
51	8.852	2411	2414	2419	rVB2	918	602	0.03%	0.004%
52	8.881	2419	2423	2429	rBV3	938	1208	0.07%	0.009%
53	9.087	2471	2487	2509	rBV	752435	1277800	72.51%	9.409%
54	9.344	2564	2567	2570	rBV4	647	456	0.03%	0.003%
55	9.379	2576	2578	2582	rBV3	855	596	0.03%	0.004%
56	9.511	2615	2619	2623	rVB4	1085	849	0.05%	0.006%
57	9.627	2649	2655	2658	rBV3	884	885	0.05%	0.007%
58	9.704	2676	2679	2683	rBV2	780	587	0.03%	0.004%
59	9.762	2694	2697	2699	rBV2	1011	621	0.04%	0.005%
60	9.961	2754	2759	2762	rVV5	938	879	0.05%	0.006%
61	10.009	2766	2774	2781	rBV8	2221	3193	0.18%	0.024%
62	10.080	2793	2796	2798	rBV2	999	695	0.04%	0.005%
63	10.212	2834	2837	2840	rBV3	866	510	0.03%	0.004%
64	10.427	2891	2904	2923	rBV	535026	874995	49.65%	6.443%
65	10.598	2953	2957	2964	rVV5	1519	2120	0.12%	0.016%
66	10.742	2999	3002	3007	rVB2	1128	1013	0.06%	0.007%
67	10.922	3053	3058	3060	rBV2	561	561	0.03%	0.004%
68	10.961	3067	3070	3073	rBV2	695	467	0.03%	0.003%
69	11.054	3095	3099	3106	rVB3	710	597	0.03%	0.004%
70	11.083	3106	3108	3111	rBV2	637	455	0.03%	0.003%
71	11.257	3159	3162	3166	rBV2	527	487	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041319\
 Data File : VU031193.D
 Acq On : 14 Apr 2019 06:19
 Operator : JC/SP
 Sample : K2409-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	11.389	3199	3203	3204	rBV2	626	427	0.02%	0.003%
73	11.479	3220	3231	3253	rBV	591600	978546	55.53%	7.206%
74	11.855	3336	3348	3372	rBV	616786	1050703	59.62%	7.737%
75	12.032	3401	3403	3407	rVB4	1119	508	0.03%	0.004%
76	12.189	3450	3452	3457	rBV5	717	545	0.03%	0.004%
77	12.479	3539	3542	3548	rVB4	1242	1052	0.06%	0.008%
78	12.710	3610	3614	3617	rBV3	770	648	0.04%	0.005%
79	12.794	3637	3640	3646	rVB4	1180	1070	0.06%	0.008%
80	12.868	3660	3663	3666	rBV3	813	491	0.03%	0.004%
81	12.900	3671	3673	3681	rVB3	914	642	0.04%	0.005%
82	12.938	3681	3685	3689	rBV3	625	620	0.04%	0.005%
83	12.961	3690	3692	3696	rVB2	698	428	0.02%	0.003%
84	13.003	3702	3705	3710	rBV2	694	622	0.04%	0.005%
85	13.035	3713	3715	3720	rBV2	705	635	0.04%	0.005%
86	13.099	3732	3735	3738	rVB3	1143	747	0.04%	0.006%
87	13.498	3856	3859	3863	rBV2	1372	1337	0.08%	0.010%
88	13.672	3911	3913	3917	rVB3	984	541	0.03%	0.004%
89	13.733	3930	3932	3935	rBV2	684	453	0.03%	0.003%
90	13.768	3941	3943	3949	rBV3	657	663	0.04%	0.005%
91	13.813	3954	3957	3962	rBV	826	726	0.04%	0.005%
92	13.861	3970	3972	3977	rBV3	803	478	0.03%	0.004%
93	14.070	4034	4037	4040	rBV3	1176	596	0.03%	0.004%
94	14.286	4101	4104	4106	rBV3	676	498	0.03%	0.004%
95	14.517	4172	4176	4179	rBV3	1146	982	0.06%	0.007%
96	14.572	4191	4193	4197	rVB2	1115	716	0.04%	0.005%
97	14.594	4197	4200	4205	rBV3	1481	1218	0.07%	0.009%
98	14.643	4212	4215	4217	rBV	886	670	0.04%	0.005%
99	14.697	4230	4232	4240	rVB4	972	1063	0.06%	0.008%
100	14.823	4268	4271	4275	rBV3	1280	1150	0.07%	0.008%


Sum of corrected areas: 13579950

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041319\
Data File : VU031193.D
Acq On : 14 Apr 2019 06:19
Operator : JC/SP
Sample : K2409-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC32

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

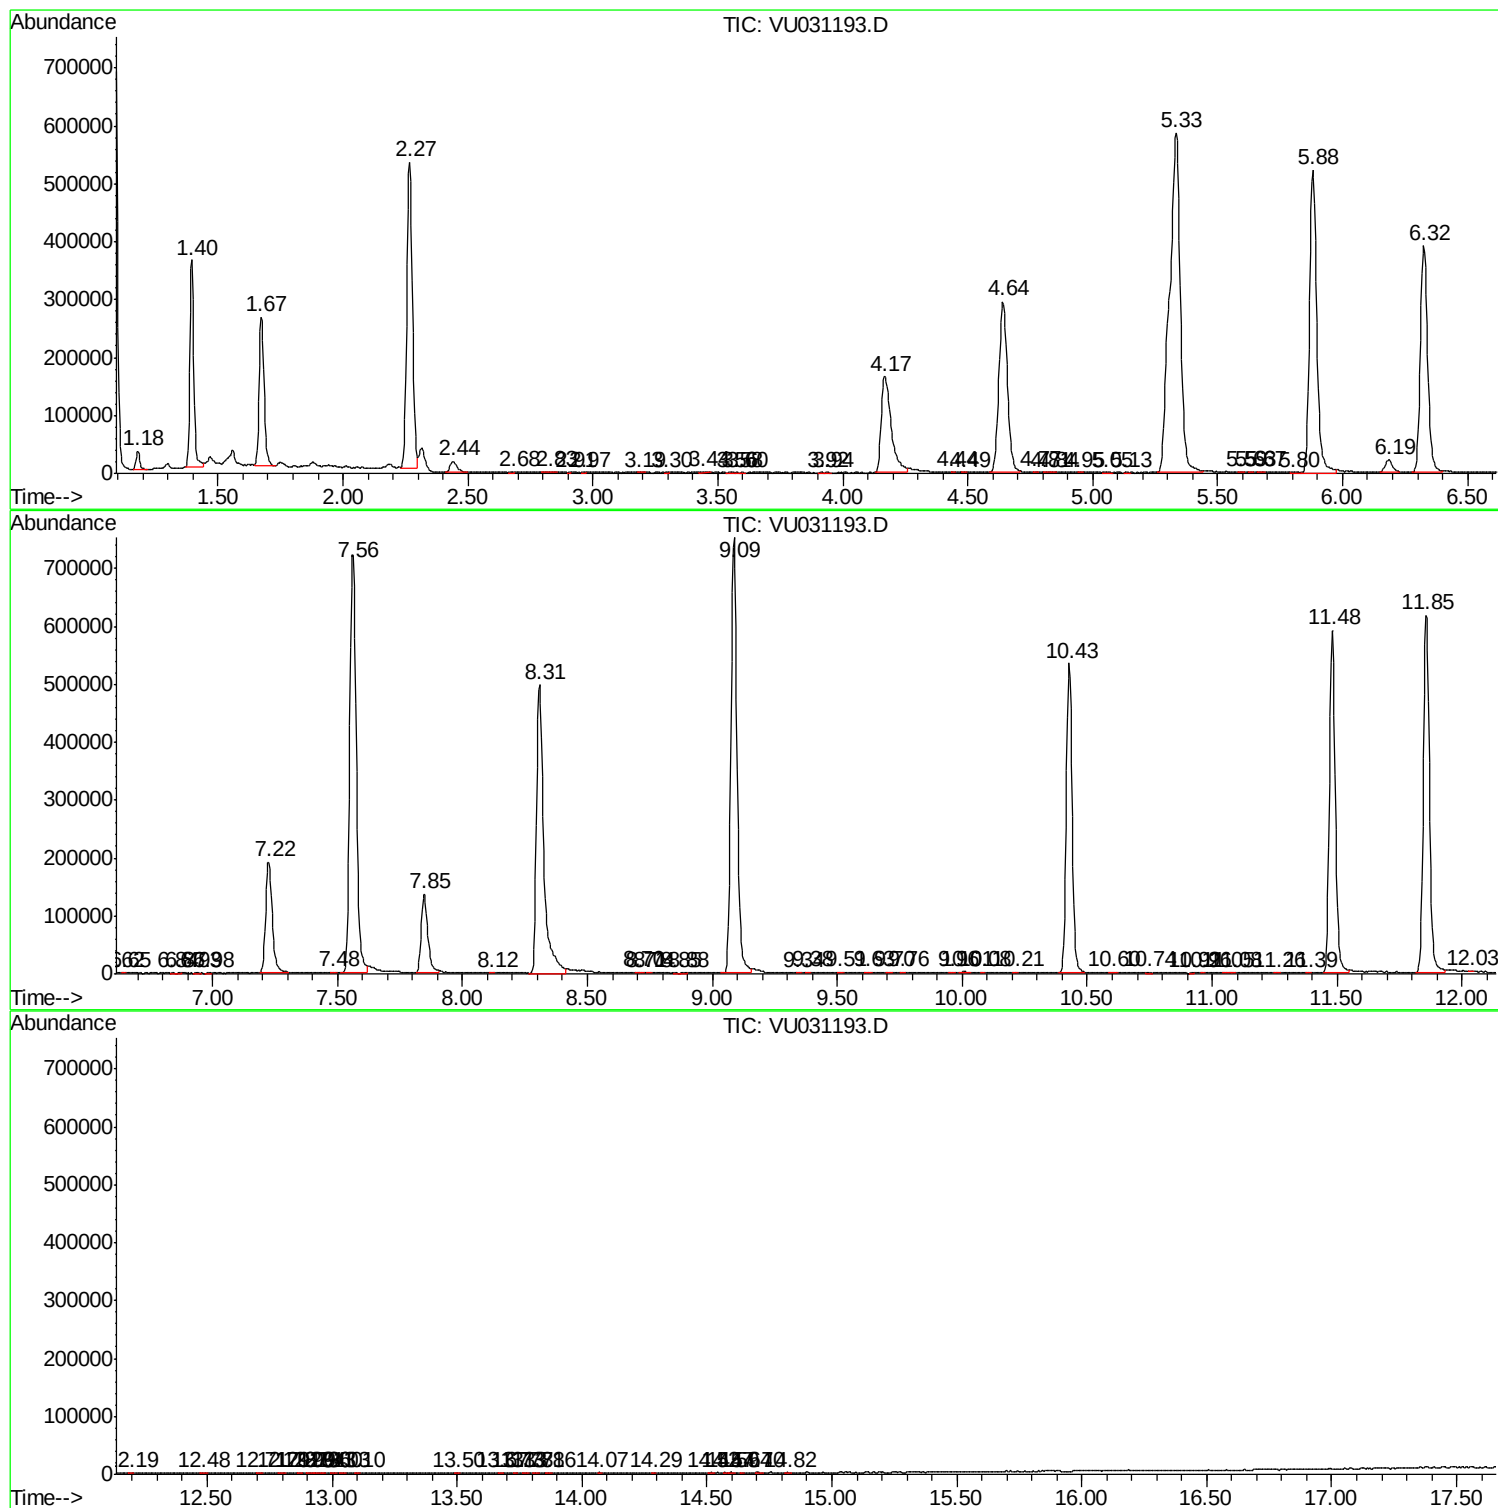

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031193.D
Acq On : 14 Apr 2019 06:19
Operator : JC/SP
Sample : K2409-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC32

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041319\
Data File : VU031193.D
Acq On : 14 Apr 2019 06:19
Operator : JC/SP
Sample : K2409-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC32

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc