


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041319\
 Data File : VU031152.D
 Acq On : 13 Apr 2019 10:49
 Operator : JC/SP
 Sample : BFB56
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB56

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 15 01:39:53 2019

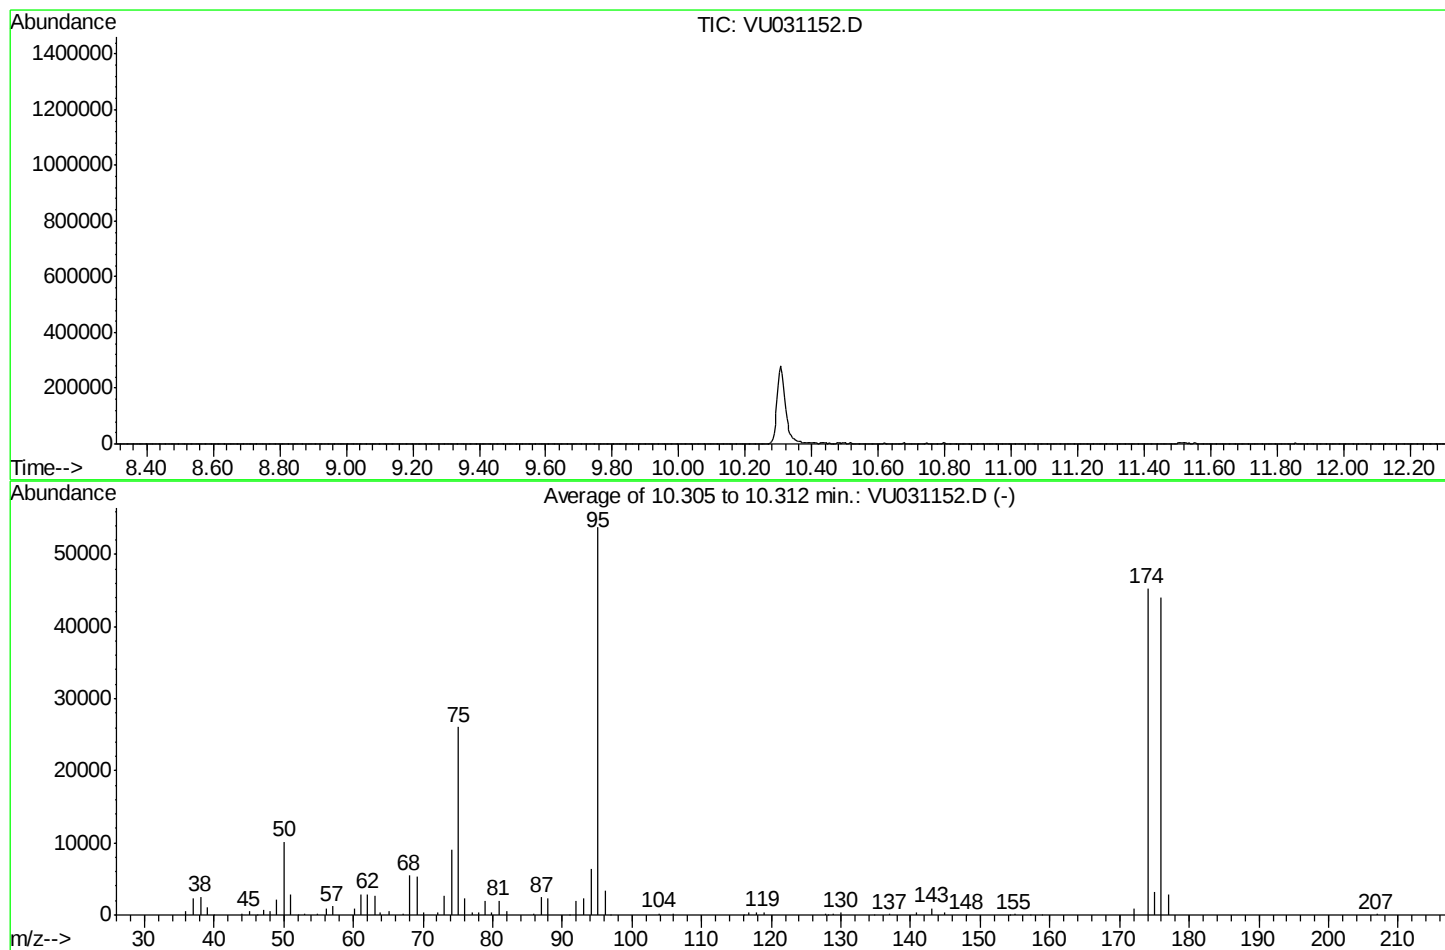

AutoFind: Scans 2866, 2867, 2868; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	10177	PASS
75	95	30	80	48.4	26034	PASS
95	95	100	100	100.0	53757	PASS
96	95	5	9	6.4	3414	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.1	45184	PASS
175	174	5	9	7.3	3282	PASS
176	174	95	101	97.6	44096	PASS
177	176	5	9	6.5	2873	PASS

m/z	Abundance
36.00	528.0
37.00	2234.0
38.00	2471.0
39.00	879.0
40.00	1019.0
44.00	895.0
45.10	394.0
46.20	114.0
47.10	779.0
48.00	389.0
49.10	1963.0
50.10	9537.0
51.00	2775.0
53.00	200.0
54.90	175.0
56.10	820.0
57.00	1273.0
60.10	607.0
61.00	2817.0
62.10	2652.0
63.10	2582.0
63.90	419.0
65.20	432.0
67.10	136.0
68.00	4763.0
69.10	5097.0
70.00	292.0
72.10	260.0
73.10	2498.0
74.10	8495.0
75.10	24392.0
76.00	2256.0
77.20	360.0
78.00	182.0
78.90	1811.0
79.90	477.0
80.90	2008.0
82.00	500.0
85.80	233.0
87.00	2283.0
88.00	2157.0
91.00	130.0
92.00	1783.0
93.00	2223.0
94.10	5819.0
95.10	50592.0
96.10	2877.0
104.00	211.0
106.00	130.0
116.90	370.0
118.00	222.0
118.90	381.0
128.10	143.0
128.90	160.0
130.10	282.0
141.00	460.0
143.00	910.0
145.00	368.0
155.00	113.0
172.10	886.0
174.00	41984.0
175.00	3115.0
176.00	41008.0
177.10	2720.0
206.80	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

Scan 2854 (10.267 min): VU031152.D
BFB56

m/z	Abundance
39.90	826.0
44.00	823.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.00	517.0
37.10	2336.0
38.10	2552.0
39.00	1236.0
40.00	783.0
43.90	1029.0
45.10	524.0
47.10	702.0
48.00	570.0
49.00	2305.0
50.10	10510.0
51.10	3108.0
52.10	142.0
53.00	292.0
54.90	197.0
56.10	852.0
57.00	1196.0
60.10	1035.0
61.10	2766.0
62.00	2910.0
63.00	2570.0
63.90	448.0
65.10	690.0
67.10	210.0
68.00	5890.0
69.10	5515.0
70.00	373.0
72.10	356.0
73.10	2599.0
74.10	9436.0
75.10	27072.0
76.00	2429.0
77.00	399.0
78.00	377.0
79.00	2115.0
79.80	399.0
80.90	1911.0
82.00	541.0
86.00	216.0
87.00	2541.0
88.00	2489.0
92.00	1996.0
93.00	2402.0
94.10	6995.0
95.10	55304.0
96.10	3886.0
97.00	126.0
103.90	200.0
105.90	255.0
116.00	138.0
116.80	375.0
117.90	357.0
119.00	424.0
127.90	161.0
128.80	213.0
130.00	240.0
134.80	183.0
137.00	232.0
140.80	350.0
143.10	1014.0
144.90	502.0
154.30	106.0
154.90	147.0
157.10	151.0
158.90	142.0
172.10	930.0
174.00	46800.0
175.00	3473.0
176.00	45776.0
177.10	2930.0
206.90	203.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.00	510.0
37.00	2358.0
38.00	2672.0
39.00	1068.0
40.00	803.0
43.90	1014.0
45.10	491.0
46.20	134.0
47.10	857.0
48.00	524.0
49.00	2133.0
50.10	10484.0
51.00	2921.0
53.00	275.0
54.90	189.0
56.10	860.0
57.00	1260.0
60.10	915.0
61.00	2847.0
62.10	2978.0
63.00	2657.0
63.90	470.0
65.10	520.0
67.10	212.0
68.00	5657.0
69.10	5419.0
70.00	329.0
72.10	304.0
73.10	2667.0
74.10	9249.0
75.10	26640.0
76.00	2472.0
77.10	363.0
78.00	258.0
78.90	2121.0
79.80	463.0
80.90	2059.0
82.00	520.0
86.00	209.0
87.00	2544.0
88.00	2412.0
91.00	116.0
92.00	1947.0
93.00	2548.0
94.10	6554.0
95.10	55376.0
96.20	3480.0
103.90	214.0
105.90	182.0
116.00	125.0
116.80	414.0
118.00	306.0
119.00	395.0
127.80	140.0
128.80	205.0
130.10	307.0
137.00	179.0
140.90	416.0
143.10	978.0
144.90	447.0
148.00	104.0
154.90	103.0
157.10	135.0
172.10	902.0
174.00	46768.0
175.00	3260.0
176.00	45504.0
177.10	2971.0
206.90	178.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56