

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041320\
Data File : VU037683.D
Acq On : 13 Apr 2020 14:14
Operator : JC/MD
Sample : VU0413MBL01
Misc : 5.0µ/5.0mL/100uL/10mL/MSVOA_U/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK54

Manual Integrations
APPROVED

MMDadoda
4/14/2020 12:37:04 PM

Quant Time: Apr 14 03:29:37 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 14 03:27:41 2020
Response via : Initial Calibration

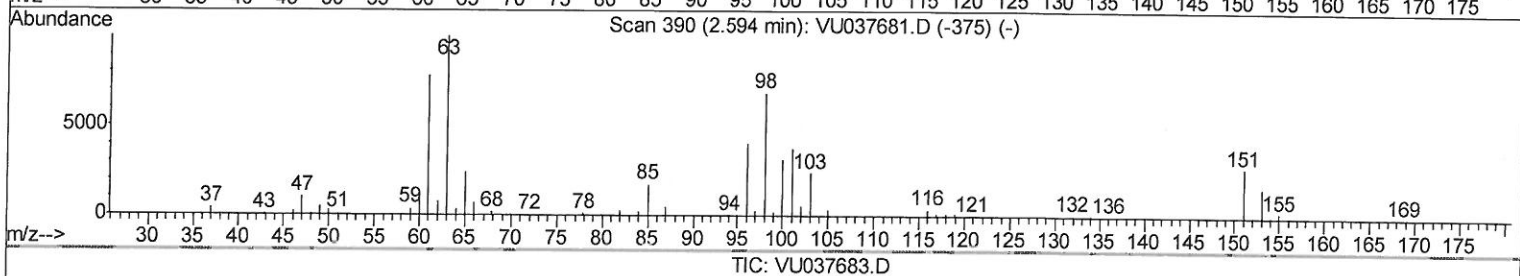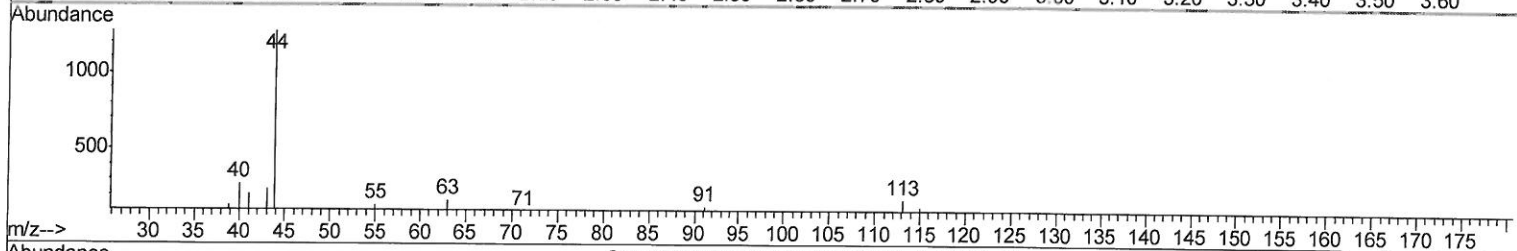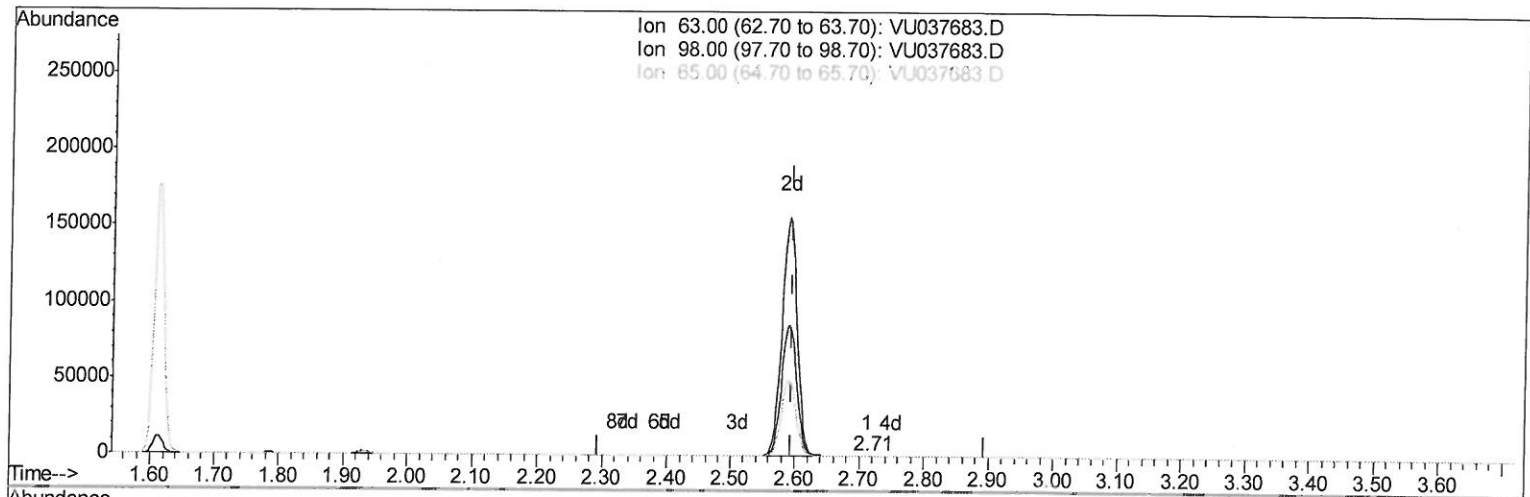

(11) 1,1-Dichloroethene-d2 (S)

2.713min (+0.119) 0.01ug/L

response 132

Ion	Exp%	Act%
63.00	100	100
98.00	70.60	53.03
65.00	23.70	29.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041320\
 Data File : VU037683.D
 Acq On : 13 Apr 2020 14:14
 Operator : JC/MD
 Sample : VU0413MBL01
 Misc : 5.0α/5.0mL/100uL/10mL/MSVOA_U/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK54

Manual Integrations
 APPROVED

MMDadoda
 4/14/2020 12:37:04 PM

Quant Time: Apr 14 03:29:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 14 03:27:41 2020
 Response via : Initial Calibration

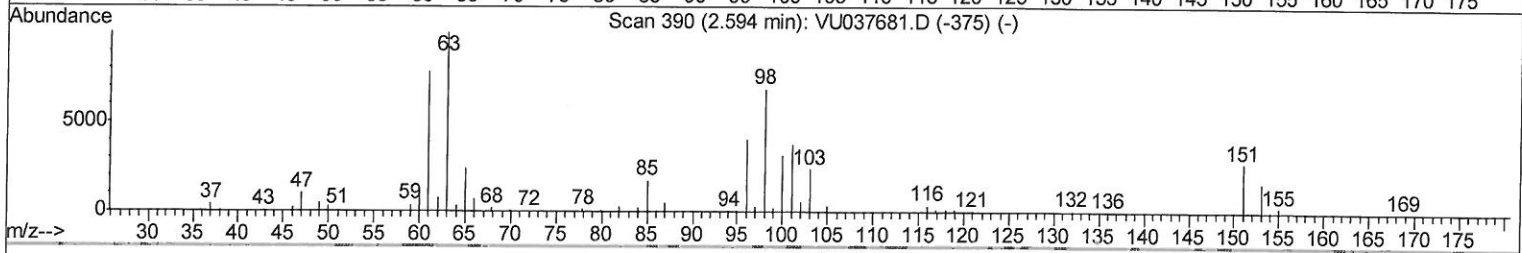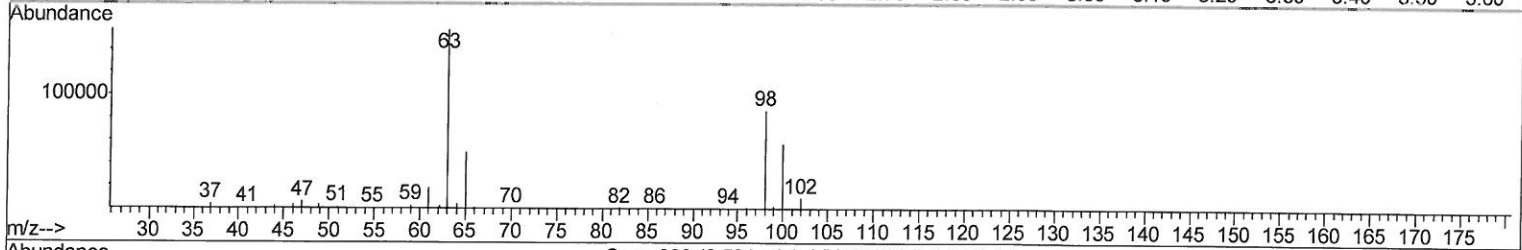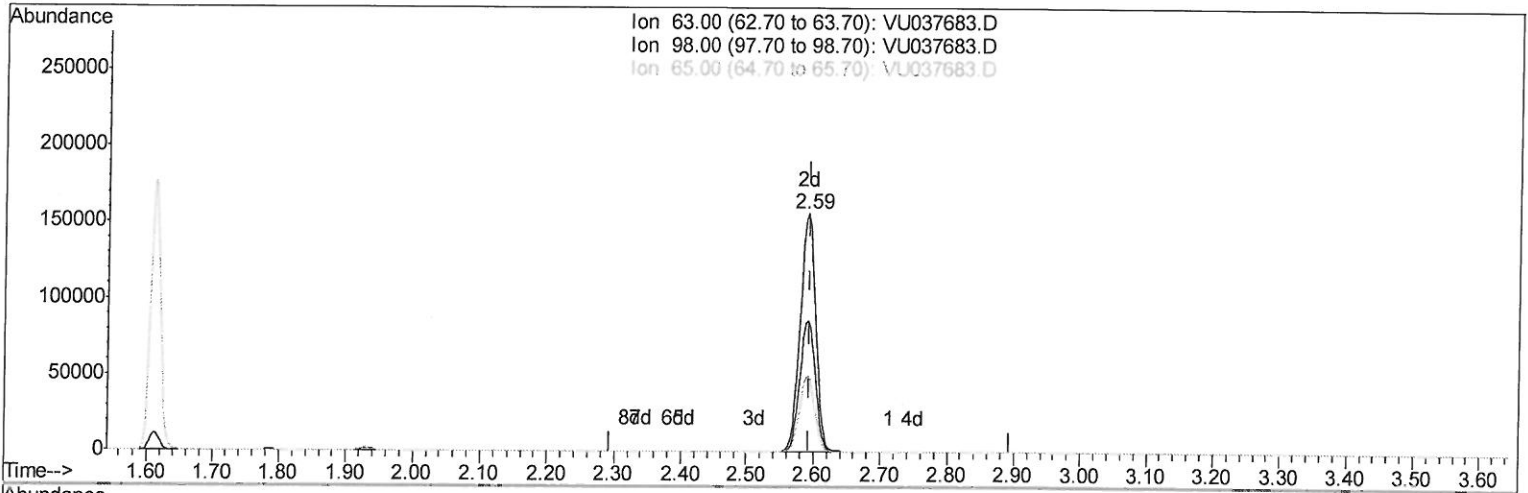

TIC: VU037683.D

(11) 1,1-Dichloroethene-d2 (S)

2.591min (-0.003) 27.83ug/L m

response 254156

Ion	Exp%	Act%
63.00	100	100
98.00	70.60	0.03#
65.00	23.70	0.02#
0.00	0.00	0.00

204/14/2020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041320\
Quantitation Report (LSC Reviewed)

Data File : VU037683.D
Acq On : 13 Apr 2020 14:14
Operator : JC/MD
Sample : VU0413MBL01
Misc : 5.0g/5.0mL/100uL/10mL/MSVOA_U/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK54

Manual Integrations
APPROVED

MMDadoda
4/14/2020 12:37:04 PM

Quant Time: Apr 14 11:52:55 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 14 03:27:41 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	641046	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	616718	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	312089	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	191259	34.13	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.26%		
7) Chloroethane-d5	1.93	69	171775	37.93	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	75.86%		
11) 1,1-Dichloroethene-d2	2.59	63	254156m	27.83	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.66%#		
21) 2-Butanone-d5	4.66	46	348299	76.71	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	76.71%		
24) Chloroform-d	5.10	84	321827	38.21	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	76.42%		
26) 1,2-Dichloroethane-d4	5.74	65	232125	40.57	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.14%		
32) Benzene-d6	5.76	84	718716	39.61	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.22%		
36) 1,2-Dichloropropane-d6	6.72	67	242632	40.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	80.34%		
41) Toluene-d8	7.92	98	657675	39.10	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.20%#		
43) trans-1,3-Dichloropropene-	8.20	79	126187	38.65	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.30%		
47) 2-Hexanone-d5	8.66	63	271041	78.38	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.38%		
57) 1,1,2,2-Tetrachloroethane-	10.78	84	339413	39.79	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	79.58%		
64) 1,2-Dichlorobenzene-d4	12.21	152	254806	39.23	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.46%#		

04/14/2020

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041320\
Quantitation Report (LSC Reviewed)
Data File : VU037683.D
Acq On : 13 Apr 2020 14:14
Operator : JC/MD
Sample : VU0413MBL01
Misc : 5.0g/5.0mL/100uL/10mL/MSVOA_U/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK54

Manual Integrations
APPROVED

MMDadoda
4/14/2020 12:37:04 PM

Quant Time: Apr 14 11:52:55 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 14 03:27:41 2020
Response via : Initial Calibration

