

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041320\
 Data File : VU037685.D
 Acq On : 13 Apr 2020 15:27
 Operator : JC/MD
 Sample : VIBLK50
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	77	84	97	rVB	290168	316376	13.78%	1.620%
2	1.929	175	183	199	rVB	251675	325109	14.16%	1.665%
3	2.591	377	389	412	rVB	439689	728908	31.75%	3.733%
4	2.787	447	450	452	rBV2	1002	554	0.02%	0.003%
5	2.864	471	474	477	rBV4	762	596	0.03%	0.003%
6	2.977	504	509	514	rVB6	1079	1313	0.06%	0.007%
7	3.002	514	517	518	rBV3	849	449	0.02%	0.002%
8	3.070	533	538	542	rBV8	1247	1531	0.07%	0.008%
9	3.141	555	560	562	rBV3	708	503	0.02%	0.003%
10	3.205	574	580	582	rBV6	1014	1026	0.04%	0.005%
11	3.244	591	592	596	rVB3	1088	490	0.02%	0.003%
12	3.356	623	627	628	rBV3	740	517	0.02%	0.003%
13	3.411	641	644	648	rVB4	879	566	0.02%	0.003%
14	3.459	656	659	664	rVB5	812	765	0.03%	0.004%
15	3.671	719	725	728	rVB5	489	615	0.03%	0.003%
16	3.742	742	747	750	rBV3	707	681	0.03%	0.003%
17	3.848	775	780	783	rVV4	519	438	0.02%	0.002%
18	3.890	788	793	795	rVB4	579	453	0.02%	0.002%
19	3.932	803	806	810	rBV3	446	454	0.02%	0.002%
20	3.951	810	812	818	rVB6	774	563	0.02%	0.003%
21	3.999	824	827	831	rBV2	584	449	0.02%	0.002%
22	4.060	844	846	854	rVB5	550	479	0.02%	0.002%
23	4.321	924	927	929	rVB2	780	441	0.02%	0.002%
24	4.462	969	971	978	rVB5	494	476	0.02%	0.002%
25	4.536	989	994	997	rVB2	625	577	0.03%	0.003%
26	4.562	997	1002	1007	rBV3	754	918	0.04%	0.005%
27	4.668	1017	1035	1067	rBV	273486	644471	28.07%	3.300%
28	4.948	1119	1122	1125	rBV2	650	554	0.02%	0.003%
29	4.961	1125	1126	1132	rVB2	698	527	0.02%	0.003%
30	4.993	1132	1136	1138	rBV3	664	484	0.02%	0.002%
31	5.102	1153	1170	1192	rVV	392835	875998	38.16%	4.486%
32	5.198	1197	1200	1203	rBV4	743	712	0.03%	0.004%
33	5.253	1214	1217	1223	rVB4	986	612	0.03%	0.003%
34	5.314	1233	1236	1241	rVV6	1586	1940	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041320\
 Data File : VU037685.D
 Acq On : 13 Apr 2020 15:27
 Operator : JC/MD
 Sample : VIBLK50
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Title : VOC Analysis

35	5.340	1242	1244	1249	rVB4	2172	1463	0.06%	0.007%
36	5.366	1249	1252	1256	rBV4	812	792	0.03%	0.004%
37	5.414	1263	1267	1278	rVB9	1515	2021	0.09%	0.010%
38	5.488	1287	1290	1294	rVV3	698	497	0.02%	0.003%
39	5.610	1323	1328	1330	rVB3	536	482	0.02%	0.002%
40	5.761	1352	1375	1392	rBV2	874945	2295540	100.00%	11.756%
41	5.944	1430	1432	1436	rVB4	949	441	0.02%	0.002%
42	5.996	1446	1448	1452	rBV3	744	459	0.02%	0.002%
43	6.057	1459	1467	1469	rBV7	1327	1550	0.07%	0.008%
44	6.150	1489	1496	1500	rVB6	1090	1372	0.06%	0.007%
45	6.215	1510	1516	1521	rBV7	499	565	0.02%	0.003%
46	6.282	1521	1537	1553	rBV	878737	1635866	71.26%	8.378%
47	6.559	1613	1623	1631	rBV7	7366	13360	0.58%	0.068%
48	6.636	1643	1647	1652	rVB3	738	675	0.03%	0.003%
49	6.723	1659	1674	1691	rBV	549895	1068294	46.54%	5.471%
50	7.012	1760	1764	1766	rBV2	561	427	0.02%	0.002%
51	7.208	1815	1825	1835	rBV4	4291	7144	0.31%	0.037%
52	7.591	1930	1944	1962	rBV	350745	604394	26.33%	3.095%
53	7.922	2025	2047	2066	rBV	1117499	1901274	82.82%	9.737%
54	8.031	2078	2081	2083	rBV3	729	503	0.02%	0.003%
55	8.202	2121	2134	2150	rBV	253755	418934	18.25%	2.145%
56	8.388	2187	2192	2193	rBV2	1357	1103	0.05%	0.006%
57	8.465	2212	2216	2218	rBV3	741	677	0.03%	0.003%
58	8.494	2218	2225	2228	rVV5	1486	1793	0.08%	0.009%
59	8.558	2239	2245	2247	rBV4	851	966	0.04%	0.005%
60	8.655	2262	2275	2302	rVV	862609	1499845	65.34%	7.681%
61	8.890	2339	2348	2353	rBV8	1606	2481	0.11%	0.013%
62	8.938	2356	2363	2367	rBV5	3883	5284	0.23%	0.027%
63	8.986	2376	2378	2382	rVB2	1018	629	0.03%	0.003%
64	9.041	2392	2395	2401	rVB3	780	840	0.04%	0.004%
65	9.076	2401	2406	2409	rBV2	738	751	0.03%	0.004%
66	9.144	2424	2427	2430	rVB5	806	623	0.03%	0.003%
67	9.189	2430	2441	2444	rBV7	1594	2702	0.12%	0.014%
68	9.275	2465	2468	2473	rVB5	667	500	0.02%	0.003%
69	9.349	2485	2491	2492	rBV	1875	1489	0.06%	0.008%
70	9.436	2504	2518	2545	rBV	1231431	2035640	88.68%	10.425%
71	9.697	2597	2599	2601	rBV	961	629	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041320\
 Data File : VU037685.D
 Acq On : 13 Apr 2020 15:27
 Operator : JC/MD
 Sample : VIBLK50
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Title : VOC Analysis

72	9.713	2602	2604	2615	rVB9	1433	2053	0.09%	0.011%
73	9.835	2637	2642	2644	rBV2	485	427	0.02%	0.002%
74	9.935	2667	2673	2679	rBV5	851	1152	0.05%	0.006%
75	10.038	2697	2705	2714	rVB5	2855	4433	0.19%	0.023%
76	10.079	2715	2718	2721	rBV2	859	661	0.03%	0.003%
77	10.121	2725	2731	2734	rBV5	2389	2744	0.12%	0.014%
78	10.182	2744	2750	2755	rBV6	1112	1399	0.06%	0.007%
79	10.359	2800	2805	2806	rBV4	1252	1109	0.05%	0.006%
80	10.404	2814	2819	2830	rVB6	3120	4295	0.19%	0.022%
81	10.558	2862	2867	2868	rBV3	1490	1148	0.05%	0.006%
82	10.636	2887	2891	2898	rVB5	3414	3906	0.17%	0.020%
83	10.674	2901	2903	2910	rVB3	1000	1231	0.05%	0.006%
84	10.774	2916	2934	2950	rBV	736584	1186552	51.69%	6.077%
85	10.890	2965	2970	2971	rBV3	833	637	0.03%	0.003%
86	11.028	3006	3013	3016	rVB5	1520	1599	0.07%	0.008%
87	11.208	3066	3069	3073	rBV4	1130	1027	0.04%	0.005%
88	11.324	3098	3105	3113	rVV6	4286	7309	0.32%	0.037%
89	11.427	3130	3137	3144	rVB3	12432	16295	0.71%	0.083%
90	11.587	3176	3187	3193	rBV6	7306	12235	0.53%	0.063%
91	11.709	3218	3225	3233	rVB9	5670	9083	0.40%	0.047%
92	11.825	3248	3261	3274	rBV	1332058	2073703	90.34%	10.620%
93	12.205	3364	3379	3395	rBV	1099779	1736175	75.63%	8.891%
94	12.336	3415	3420	3423	rBV5	2929	3153	0.14%	0.016%
95	13.613	3811	3817	3825	rBV6	4426	6771	0.29%	0.035%
96	13.825	3880	3883	3885	rBV2	1198	870	0.04%	0.004%
97	13.867	3889	3896	3901	rVV8	2277	3827	0.17%	0.020%
98	13.906	3906	3908	3914	rVV6	1408	1236	0.05%	0.006%
99	14.111	3967	3972	3982	rVB3	8517	12730	0.55%	0.065%
100	15.259	4323	4329	4334	rBV6	5052	6407	0.28%	0.033%


Sum of corrected areas: 19526717

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041320\
Data File : VU037685.D
Acq On : 13 Apr 2020 15:27
Operator : JC/MD
Sample : VIBLK50
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

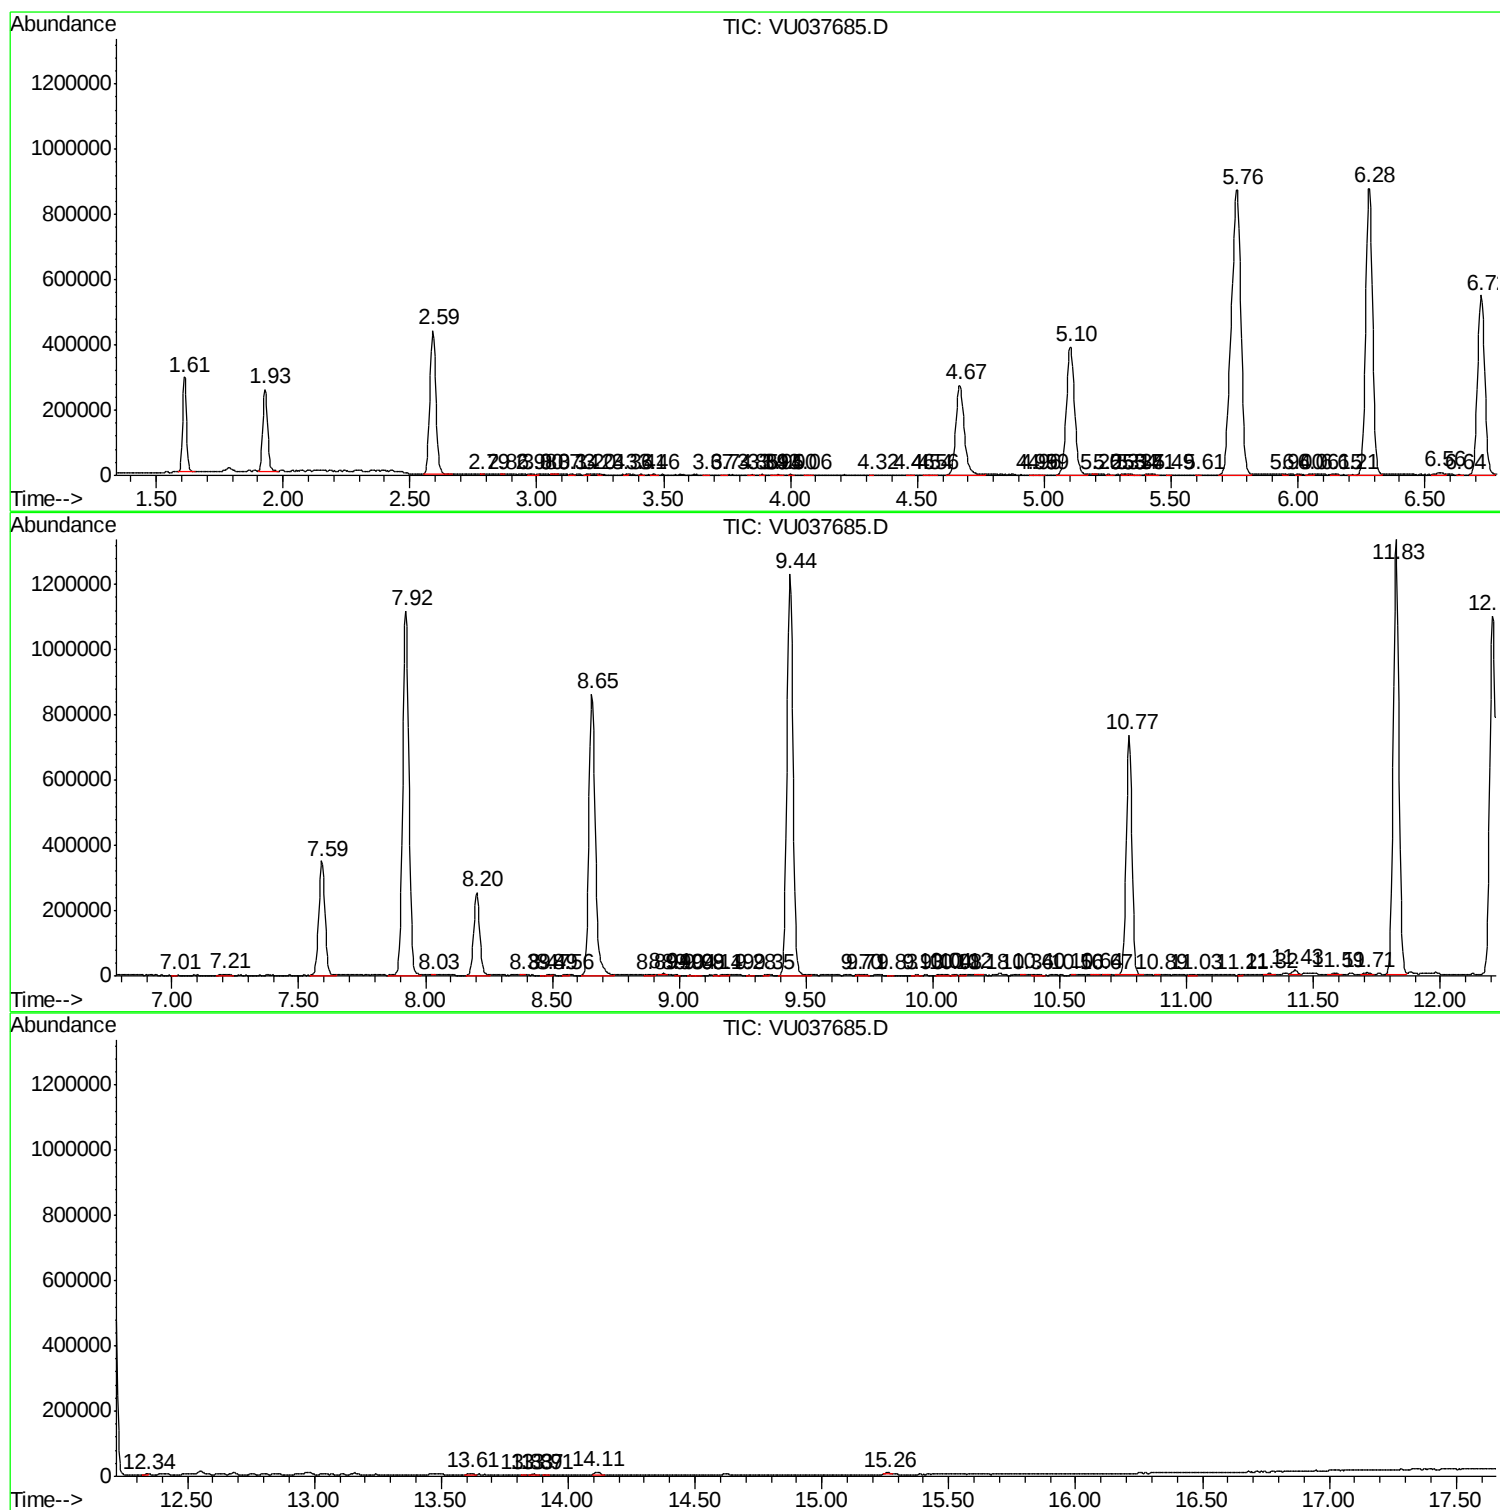

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041320\
Data File : VU037685.D
Acq On : 13 Apr 2020 15:27
Operator : JC/MD
Sample : VIBLK50
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041320\
Data File : VU037685.D
Acq On : 13 Apr 2020 15:27
Operator : JC/MD
Sample : VIBLK50
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc