


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041320\
 Data File : VU037680.D
 Acq On : 13 Apr 2020 09:16
 Operator : JC/MD
 Sample : BFB39
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB39

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040920WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 14 12:57:26 2020

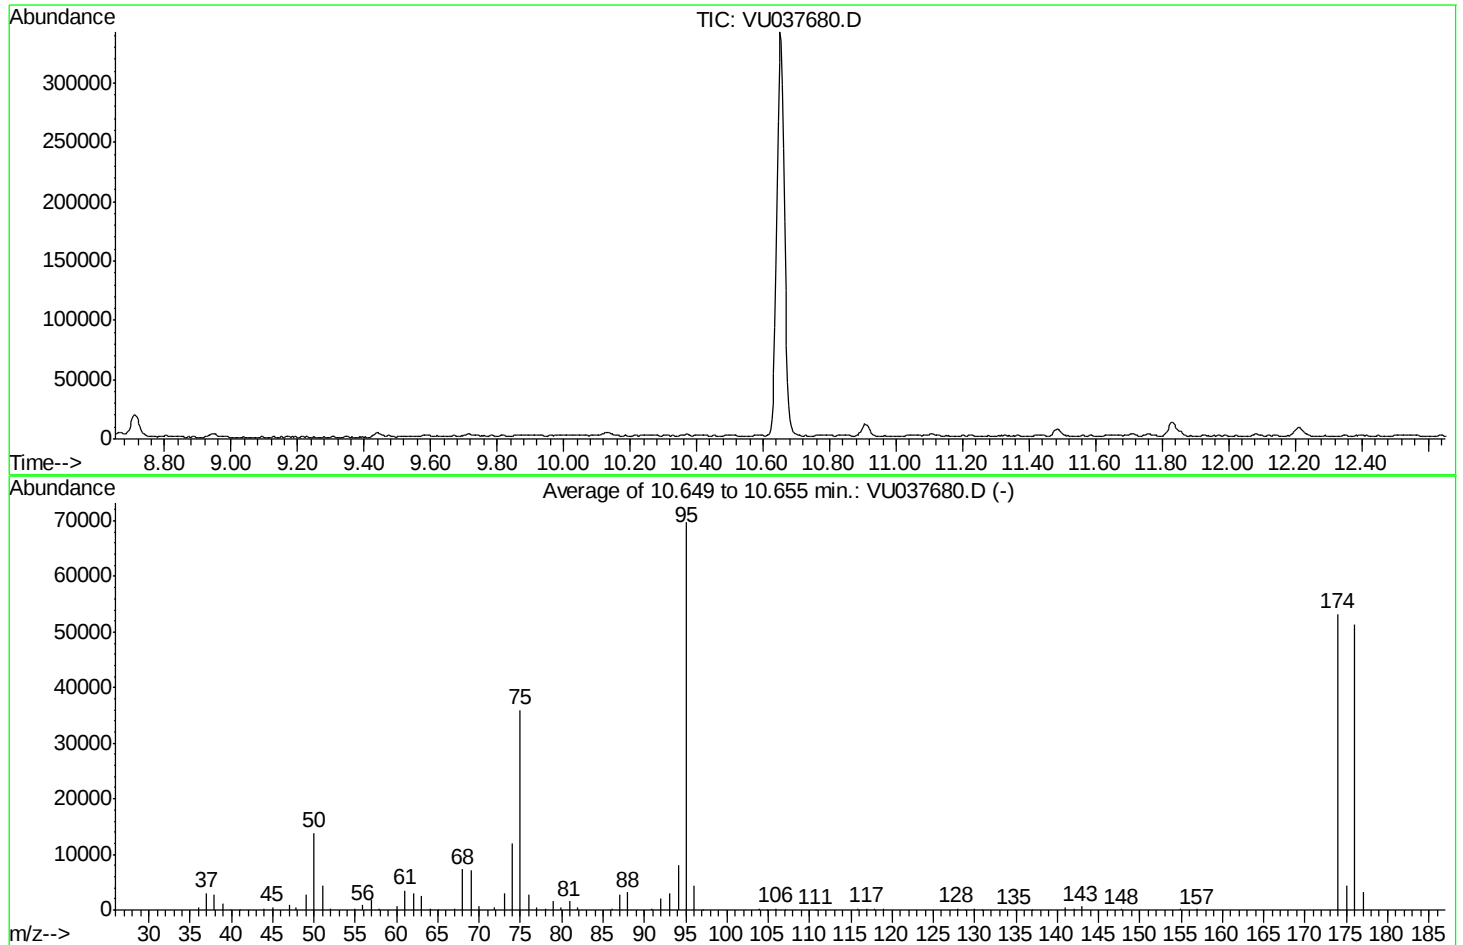

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	13863	PASS
75	95	30	80	51.6	35997	PASS
95	95	100	100	100.0	69733	PASS
96	95	5	9	6.3	4375	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.4	53290	PASS
175	174	5	9	8.1	4299	PASS
176	174	95	101	96.2	51277	PASS
177	176	5	9	6.2	3175	PASS

m/z	Abundance
36.00	1195.0
37.00	3168.0
38.00	2694.0
39.00	1237.0
40.00	249.0
41.00	221.0
42.90	121.0
44.00	1099.0
45.00	540.0
47.10	763.0
47.80	430.0
49.00	2686.0
50.00	13698.0
51.00	4122.0
52.00	160.0
54.90	310.0
55.90	1011.0
57.00	2066.0
58.10	134.0
60.00	710.0
61.00	3330.0
62.00	3069.0
63.10	2582.0
64.20	224.0
67.00	260.0
68.00	6945.0
69.10	7190.0
70.00	620.0
71.90	418.0
73.00	2821.0
74.00	11684.0
75.00	34896.0
76.10	2994.0
76.90	495.0
78.10	362.0
78.90	1720.0
79.90	443.0
80.90	1602.0
81.80	454.0
86.10	133.0
86.90	2702.0
88.00	2871.0
90.90	297.0
92.00	2076.0
93.00	2851.0
94.10	7645.0
95.10	67568.0
96.00	4213.0
103.90	195.0
105.00	106.0
106.00	349.0
107.00	104.0
115.90	195.0
117.00	329.0
117.90	265.0
119.00	290.0
127.90	269.0
129.90	208.0
130.90	113.0
134.80	110.0
140.90	489.0
141.90	118.0
142.90	669.0
147.80	122.0
154.90	127.0
156.90	167.0
174.00	49312.0
175.00	4065.0
176.00	47744.0
177.00	3045.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	1272.0
37.00	3215.0
38.00	3046.0
39.00	1283.0
40.00	283.0
41.00	226.0
42.90	123.0
44.00	1133.0
45.00	602.0
47.10	838.0
47.90	437.0
49.00	2783.0
50.00	14217.0
51.00	4451.0
52.00	194.0
54.90	311.0
55.90	1126.0
57.00	2138.0
57.90	135.0
60.00	692.0
61.00	3685.0
62.00	3102.0
63.10	2596.0
64.20	218.0
65.00	109.0
67.00	315.0
68.00	7595.0
69.00	7427.0
70.00	651.0
71.90	446.0
73.00	3019.0
74.10	12389.0
75.00	37352.0
76.10	2917.0
76.90	513.0
78.10	365.0
78.90	1753.0
79.90	485.0
80.90	1677.0
81.80	477.0
86.10	208.0
86.90	2793.0
88.00	3264.0
90.90	322.0
92.00	2131.0
93.00	3223.0
94.10	8580.0
95.10	71936.0
96.00	4463.0
97.10	108.0
103.90	237.0
104.90	105.0
106.00	369.0
107.00	110.0
115.90	217.0
116.90	346.0
117.90	316.0
119.00	308.0
127.90	263.0
129.90	206.0
130.90	119.0
134.80	103.0
140.90	518.0
142.00	138.0
143.00	695.0
147.80	134.0
155.00	157.0
157.00	165.0
174.00	54688.0
175.00	4441.0
176.00	53392.0
177.00	3309.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	1295.0
37.00	2963.0
38.00	3125.0
39.00	1245.0
40.00	293.0
41.10	215.0
42.90	157.0
44.00	1066.0
45.00	575.0
47.00	877.0
47.90	409.0
49.00	2750.0
50.00	13676.0
51.00	4315.0
51.90	225.0
55.00	259.0
55.90	1027.0
57.00	2015.0
57.90	137.0
60.00	676.0
61.00	3636.0
62.00	2974.0
63.00	2408.0
64.00	147.0
67.00	303.0
68.00	7450.0
69.00	7059.0
70.00	583.0
71.90	370.0
73.00	3013.0
74.10	11784.0
75.00	35744.0
76.00	2535.0
76.90	469.0
78.00	309.0
78.90	1633.0
79.90	582.0
80.90	1625.0
81.90	496.0
86.10	198.0
87.00	2750.0
88.00	3319.0
90.90	299.0
92.00	1949.0
93.00	3141.0
94.10	8240.0
95.10	69696.0
96.00	4449.0
97.10	158.0
103.90	256.0
104.80	104.0
106.00	321.0
110.80	115.0
115.90	223.0
116.90	329.0
117.90	311.0
119.00	313.0
127.90	228.0
128.90	137.0
129.90	156.0
134.90	100.0
136.90	105.0
140.90	542.0
142.10	151.0
143.00	686.0
147.80	132.0
155.00	162.0
157.00	145.0
174.00	55872.0
175.00	4392.0
176.00	52696.0
177.00	3171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
35.90	695.0
37.90	255.0
39.10	124.0
39.90	223.0
40.90	138.0
42.10	129.0
42.90	183.0
44.00	827.0
54.90	136.0
56.00	136.0
57.00	108.0
81.00	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39