

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
 Data File : VU043073.D
 Acq On : 14 Apr 2021 00:15
 Operator : SY/MD
 Sample : M1978-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Apr 14 05:09:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
 Quant Title : SW846 8260
 QLast Update : Mon Apr 12 13:17:29 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.382	168	136392	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	224737	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	215718	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	112160	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	111352	48.56	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.12%	
35) Dibromofluoromethane	5.298	113	78129	46.27	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.54%	
50) Toluene-d8	7.906	98	287973	48.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.38%	
62) 4-Bromofluorobenzene	10.639	95	107881	45.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.16%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.520	50	378	Below Cal	#	41
11) Tert butyl alcohol	3.192	59	1416	2.40	ug/l #	94
16) Acetone	2.633	43	9653	6.86	ug/l	100
17) Carbon Disulfide	2.797	76	1605	0.41	ug/l #	74
25) 2-Butanone	4.716	43	2193	1.05	ug/l	93
27) cis-1,2-Dichloroethene	4.674	96	3068	1.81	ug/l	86
31) Cyclohexane	5.379	56	3870	1.37	ug/l #	42
36) 1,1-Dichloropropene	5.382	75	11509	4.83	ug/l #	50
37) Ethyl Acetate	4.716	43	2193	0.54	ug/l #	71
38) Carbon Tetrachloride	5.382	117	13709	5.36	ug/l #	16
39) Methylcyclohexane	6.742	83	548	0.21	ug/l #	37
40) Benzene	5.780	78	1838	0.27	ug/l	90
43) Isopropyl Acetate	5.906	43	7498	1.29	ug/l #	64
44) Trichloroethene	6.552	130	2162	1.25	ug/l	95
51) 4-Methyl-2-Pentanone	7.806	43	977	0.23	ug/l #	64
52) Toluene	7.973	92	1578	0.37	ug/l	100
55) 1,1,2-Trichloroethane	8.378	97	3378	1.86	ug/l #	16
56) Ethyl methacrylate	8.378	69	992	0.33	ug/l #	1
59) 2-Hexanone	8.684	43	924	0.26	ug/l	70
60) Dibromochloromethane	8.562	129	3371	1.61	ug/l #	11
64) Tetrachloroethene	8.559	164	3820	2.44	ug/l	96
68) m/p-Xylenes	9.700	106	958	0.31	ug/l	93
76) 1,2,3-Trichloropropane	10.639	75	62928	19.20	ug/l #	36
81) trans-1,4-Dichloro-2-b...	10.639	75	62928	56.42	ug/l #	7
85) sec-Butylbenzene	11.652	105	3608	0.47	ug/l	98
86) p-Isopropyltoluene	12.015	119	1588	0.23	ug/l	96
89) n-Butylbenzene	12.195	91	2158	0.33	ug/l #	6
90) Hexachloroethane	12.311	117	619	0.47	ug/l #	6
93) 1,2,4-Trichlorobenzene	13.851	180	104	1.55	ug/l #	1
95) Naphthalene	14.098	128	2580	3.04	ug/l #	79
96) 1,2,3-Trichlorobenzene	14.343	180	47	1.48	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
Data File : VU043073.D
Acq On : 14 Apr 2021 00:15
Operator : SY/MD
Sample : M1978-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Apr 14 05:09:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Quant Title : SW846 8260
QLast Update : Mon Apr 12 13:17:29 2021
Response via : Initial Calibration




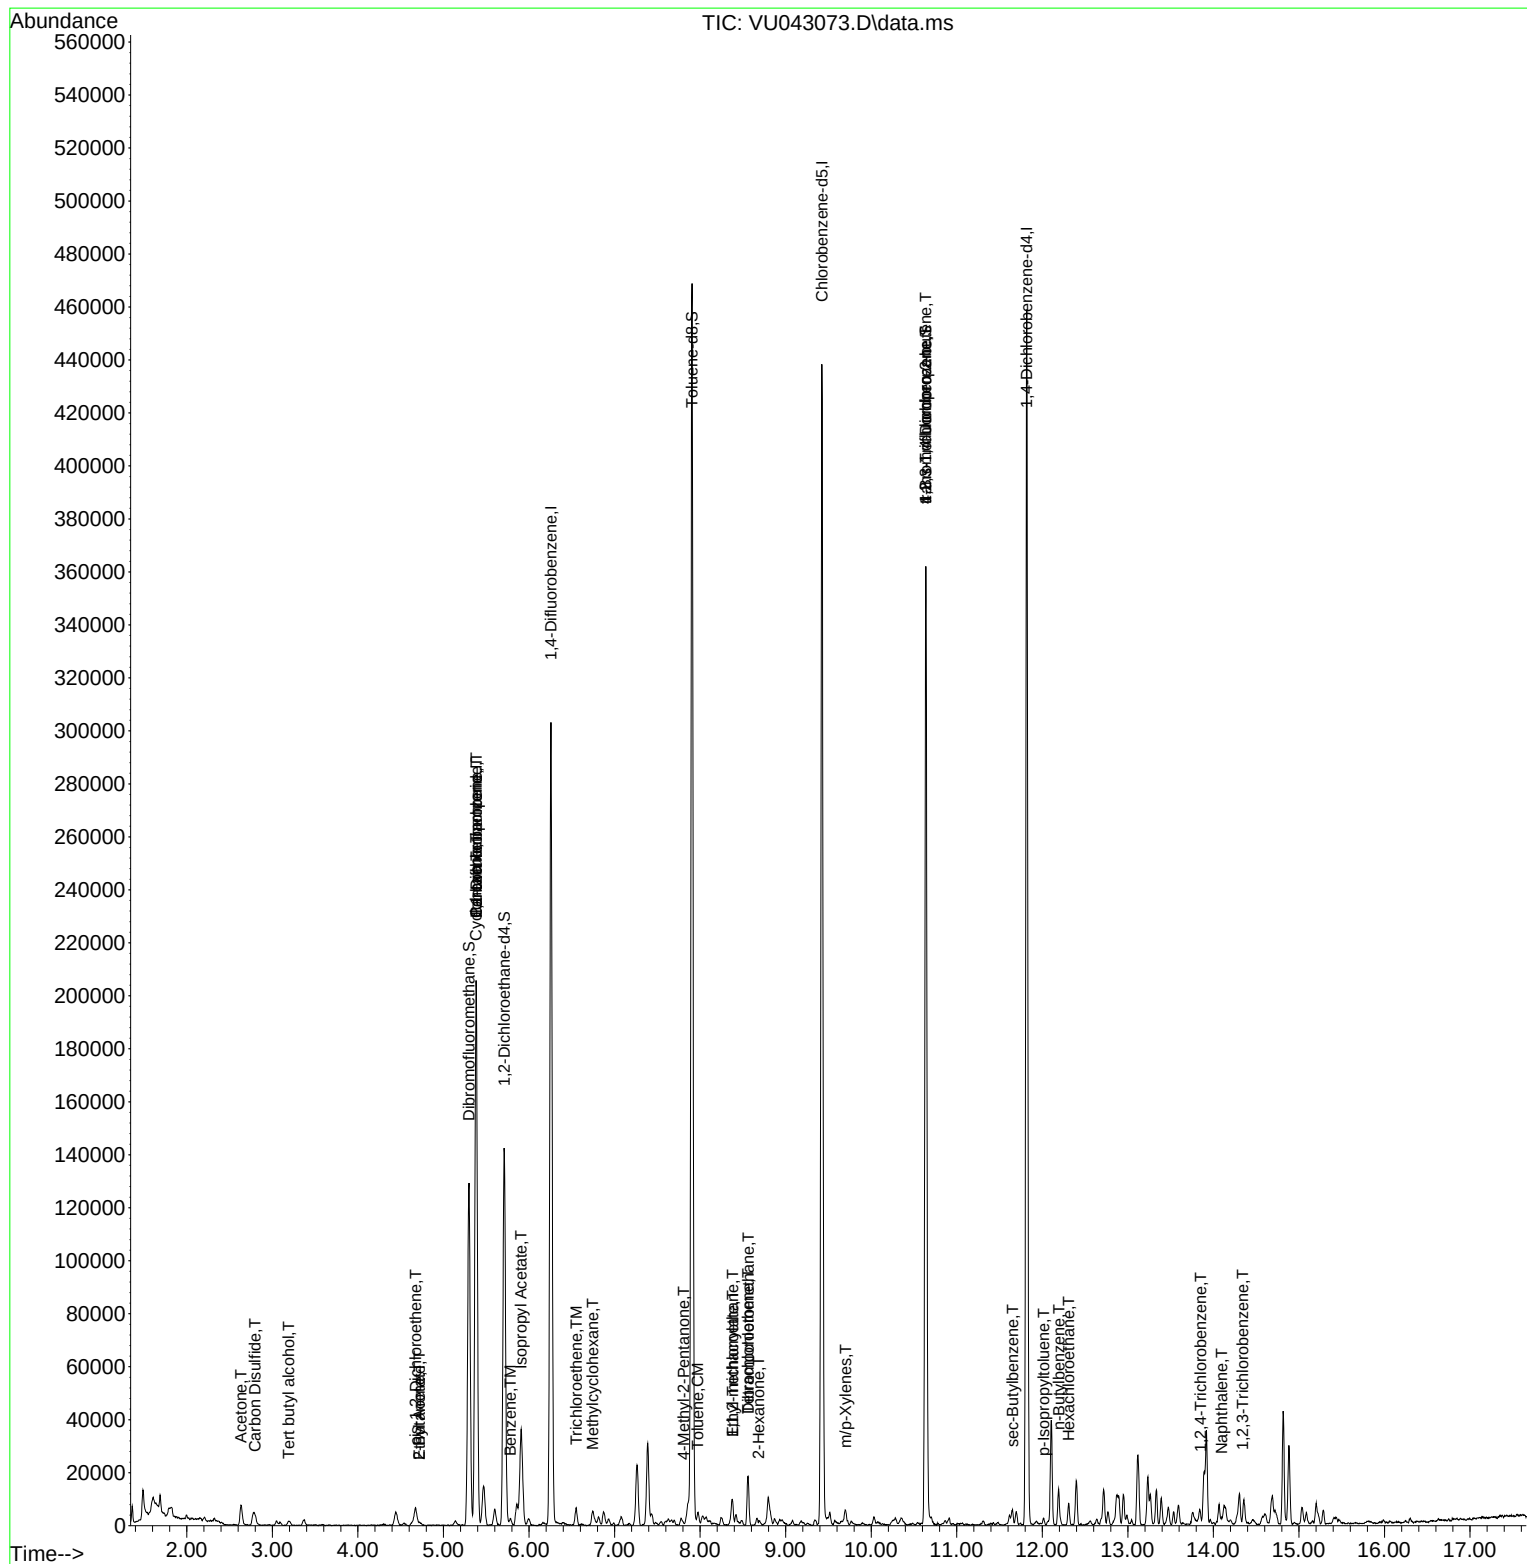




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:168 Resp: 136392
Ion Ratio Lower Upper
168 100
99 56.8 45.0 67.4

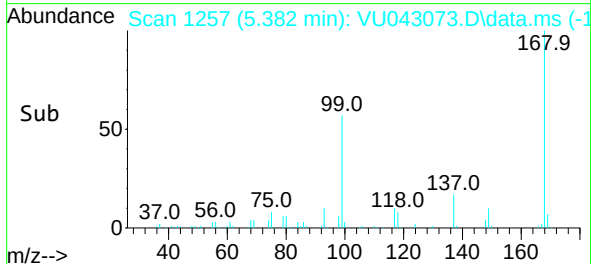

#3
Chloromethane
Concen: Below Cal
RT: 1.520 min Scan# 56
Delta R.T. 0.000 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion: 50 Resp: 378
Ion Ratio Lower Upper
50 100
52 0.0 26.6 40.0#


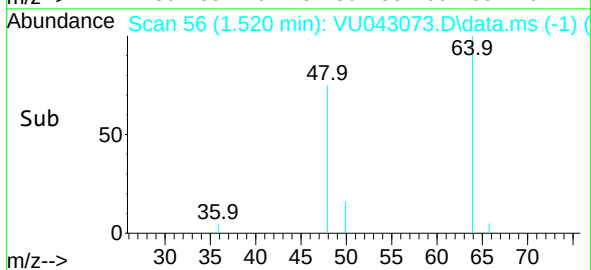

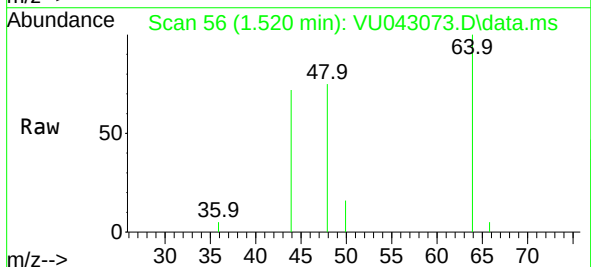


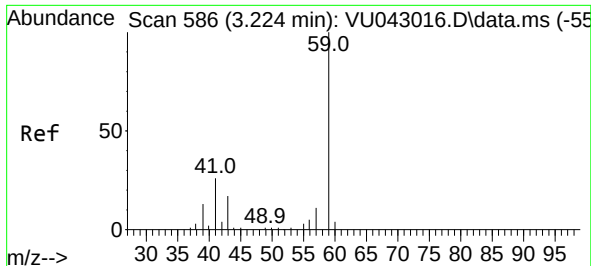

#11
Tert butyl alcohol
Concen: 2.40 ug/l
RT: 3.192 min Scan# 576
Delta R.T. -0.032 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 59 Resp: 1416
Ion Ratio Lower Upper
59 100
57 0.0 1.6 2.4#

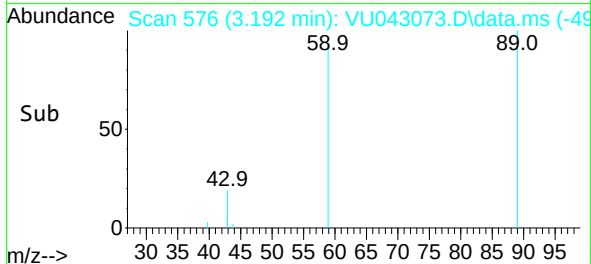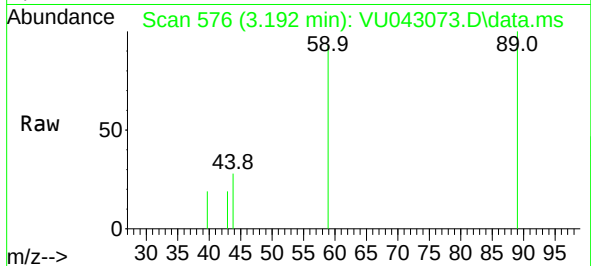

#16
Acetone
Concen: 6.86 ug/l
RT: 2.633 min Scan# 402
Delta R.T. 0.004 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion: 43 Resp: 9653
Ion Ratio Lower Upper
43 100
58 27.0 21.5 32.3


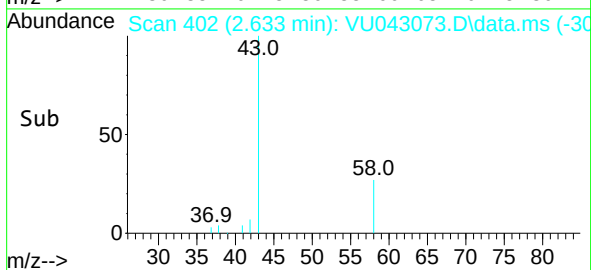

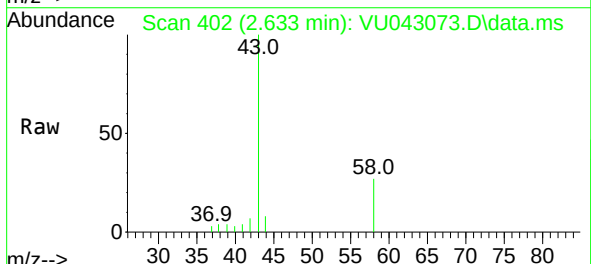




#17
Carbon Disulfide
Concen: 0.41 ug/l
RT: 2.797 min Scan# 453
Delta R.T. -0.000 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 76 Resp: 1605
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#



#25
2-Butanone
Concen: 1.05 ug/l
RT: 4.716 min Scan# 1050
Delta R.T. 0.009 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion: 43 Resp: 2193
Ion Ratio Lower Upper
43 100
72 25.0 17.4 26.0


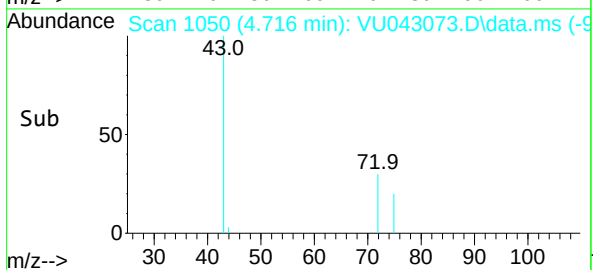

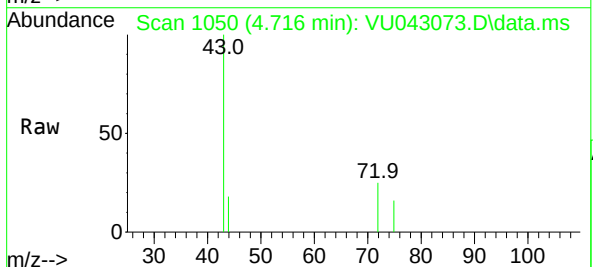




#27
 cis-1,2-Dichloroethene
 Concen: 1.81 ug/l
 RT: 4.674 min Scan# 1037
 Delta R.T. 0.000 min
 Lab File: VU043073.D
 Acq: 14 Apr 2021 00:15




Instrument :
 MSVOA_U
 ClientSampled :


Tgt Ion:	96	Resp:	3068
Ion	Ratio	Lower	Upper
96	100		
61	139.7	0.0	322.2
98	58.0	0.0	128.6

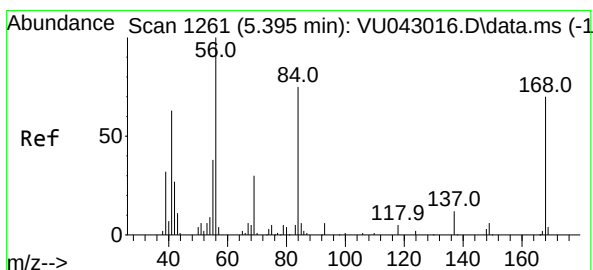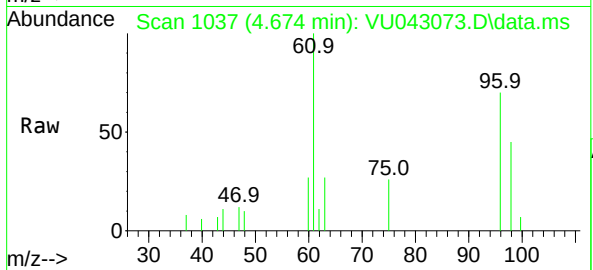

#31
 Cyclohexane
 Concen: 1.37 ug/l
 RT: 5.379 min Scan# 1256
 Delta R.T. -0.016 min
 Lab File: VU043073.D
 Acq: 14 Apr 2021 00:15

Tgt Ion:	56	Resp:	3870
Ion	Ratio	Lower	Upper
56	100		
69	137.6	24.9	37.3#
84	84.6	63.7	95.5

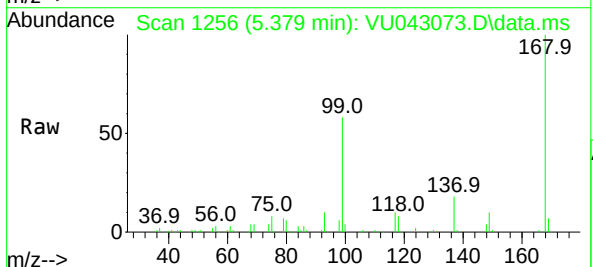



#33

1,2-Dichloroethane-d4

Concen: 48.56 ug/l

RT: 5.710 min Scan# 1359

Delta R.T. -0.000 min

Lab File: VU043073.D





Acq: 14 Apr 2021 00:15

Tgt Ion: 65 Resp: 111352

Ion Ratio Lower Upper

65 100

67 50.2 0.0 99.8



#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.256 min Scan# 1529

Delta R.T. 0.000 min

Lab File: VU043073.D

Acq: 14 Apr 2021 00:15




Tgt Ion: 114 Resp: 224737


Ion Ratio Lower Upper

114 100

63 23.2 0.0 44.2

88 16.6 0.0 33.4

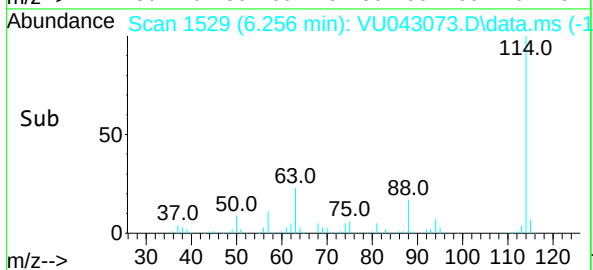



#35

Dibromofluoromethane

Concen: 46.27 ug/l

RT: 5.298 min Scan# 1231





Delta R.T. 0.000 min

Lab File: VU043073.D

Acq: 14 Apr 2021 00:15

Tgt Ion:	113	Resp:	78129
Ion	Ratio	Lower	Upper
113	100		
111	102.1	81.8	122.8
192	22.1	17.2	25.8

Instrument :
MSVOA_U
ClientSampleId :

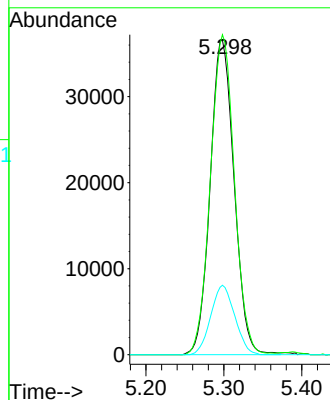

#36

1,1-Dichloropropene

Concen: 4.83 ug/l




RT: 5.382 min Scan# 1257


Delta R.T. -0.151 min

Lab File: VU043073.D

Acq: 14 Apr 2021 00:15

Tgt Ion:	75	Resp:	11509
Ion	Ratio	Lower	Upper
75	100		
110	8.4	16.8	50.3#
77	0.0	24.8	37.2#

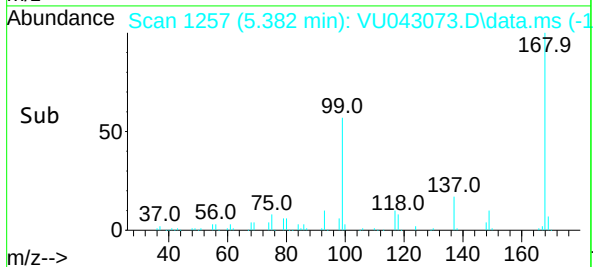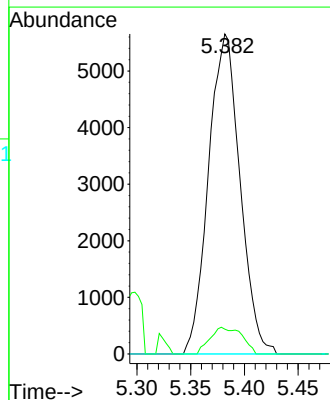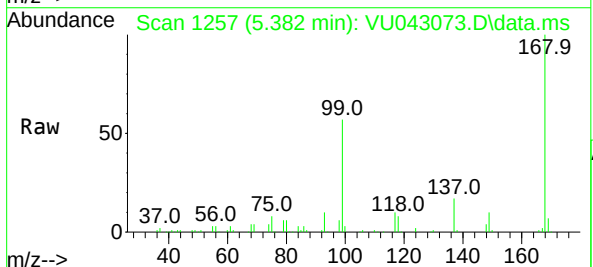



#37

Ethyl Acetate

Concen: 0.54 ug/l

RT: 4.716 min Scan# 1050





Delta R.T. -0.090 min

Lab File: VU043073.D

Acq: 14 Apr 2021 00:15

Tgt Ion: 43	Resp: 2193
Ion Ratio	Lower Upper
43 100	
61 0.0	10.1 15.1#
70 0.0	7.2 10.8#

Instrument :
MSVOA_U
ClientSampleId :

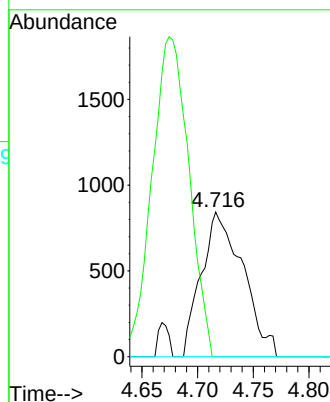

#38

Carbon Tetrachloride

Concen: 5.36 ug/l




RT: 5.382 min Scan# 1257


Delta R.T. -0.151 min

Lab File: VU043073.D

Acq: 14 Apr 2021 00:15

Tgt Ion: 117	Resp: 13709
Ion Ratio	Lower Upper
117 100	
119 4.7	75.5 113.3#
121 0.0	24.7 37.1#

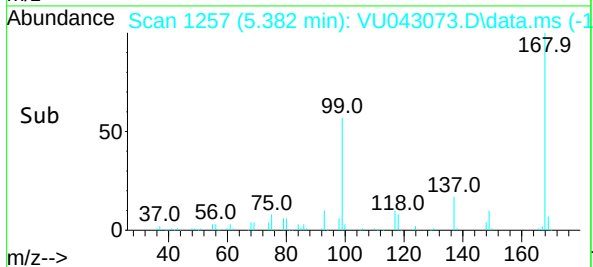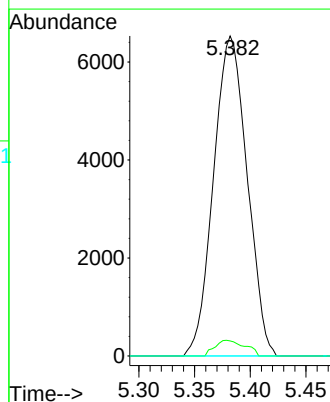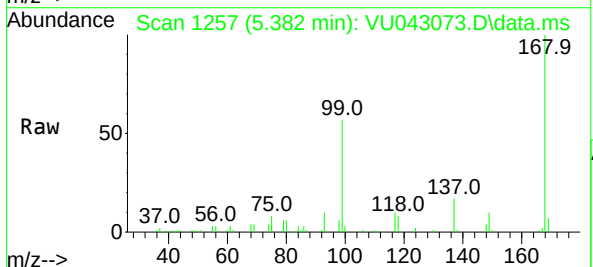



#39

Methylcyclohexane

Concen: 0.21 ug/l

RT: 6.742 min Scan# 1680





Delta R.T. -0.029 min

Lab File: VU043073.D

Acq: 14 Apr 2021 00:15

Tgt Ion:	83	Resp:	548
Ion	Ratio	Lower	Upper
83	100		
55	137.6	66.8	100.2#
98	0.0	36.9	55.3#

Instrument :
MSVOA_U
ClientSampleId :



#40

Benzene

Concen: 0.27 ug/l




RT: 5.780 min Scan# 1381


Delta R.T. 0.000 min

Lab File: VU043073.D

Acq: 14 Apr 2021 00:15

Tgt Ion:	78	Resp:	1838
Ion	Ratio	Lower	Upper
78	100		
77	28.9	19.3	28.9


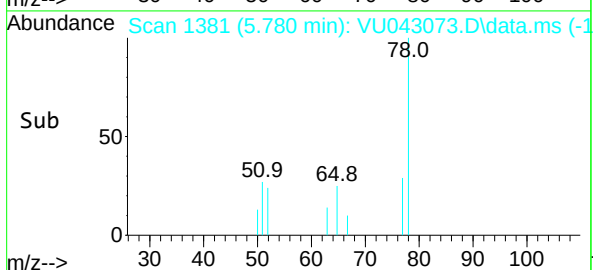






#43
Isopropyl Acetate
Concen: 1.29 ug/l
RT: 5.906 min Scan# 1420
Delta R.T. -0.009 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 43 Resp: 7498
Ion Ratio Lower Upper
43 100
61 0.0 14.4 21.6#
87 0.0 8.8 13.2#



#44
Trichloroethene
Concen: 1.25 ug/l
RT: 6.552 min Scan# 1621
Delta R.T. 0.003 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion:130 Resp: 2162
Ion Ratio Lower Upper
130 100
95 94.1 0.0 197.8


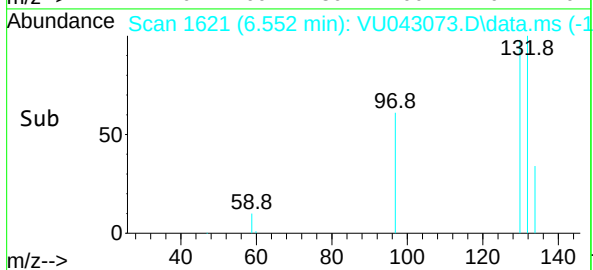

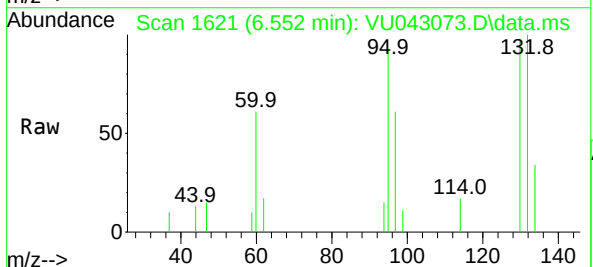




#50
Toluene-d8
Concen: 48.19 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. -0.000 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 98 Resp: 287973
Ion Ratio Lower Upper
98 100
100 62.7 50.2 75.2



#51
4-Methyl-2-Pentanone
Concen: 0.23 ug/l
RT: 7.806 min Scan# 2011
Delta R.T. 0.006 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15


Tgt Ion: 43 Resp: 977
Ion Ratio Lower Upper
43 100
58 13.9 28.1 42.1#

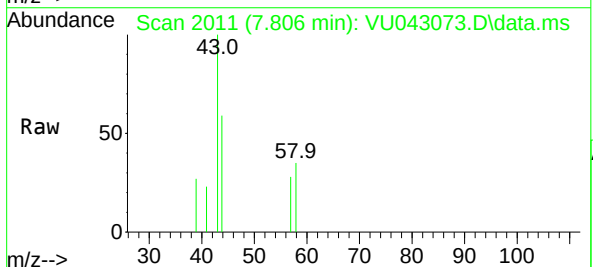






#52
Toluene
Concen: 0.37 ug/l
RT: 7.973 min Scan# 2063
Delta R.T. -0.003 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Instrument :
MSVOA_U
ClientSampled :







Tgt Ion: 92 Resp: 1578
Ion Ratio Lower Upper
92 100
91 175.5 140.3 210.5



#55
1,1,2-Trichloroethane
Concen: 1.86 ug/l
RT: 8.378 min Scan# 2189
Delta R.T. -0.029 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion: 97 Resp: 3378
Ion Ratio Lower Upper
97 100
83 6.4 72.6 109.0#
85 0.0 46.6 69.8#
99 0.0 50.9 76.3#


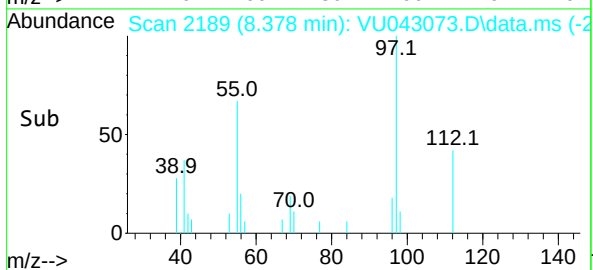

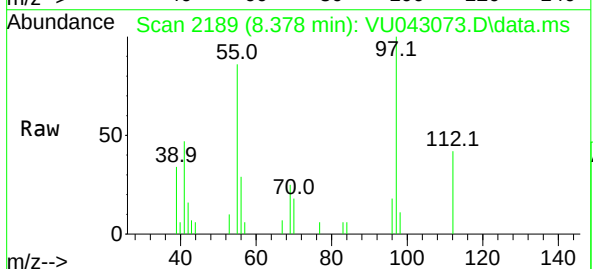




#56
Ethyl methacrylate
Concen: 0.33 ug/l
RT: 8.378 min Scan# 2189
Delta R.T. 0.038 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 69 Resp: 992
Ion Ratio Lower Upper
69 100
41 215.0 62.8 94.2#
39 138.8 36.2 54.2#

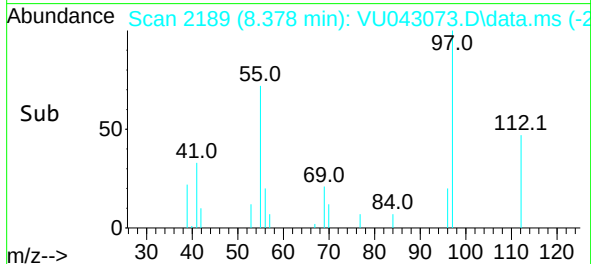

#59
2-Hexanone
Concen: 0.26 ug/l
RT: 8.684 min Scan# 2284
Delta R.T. -0.010 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion: 43 Resp: 924
Ion Ratio Lower Upper
43 100
58 27.9 24.0 72.0


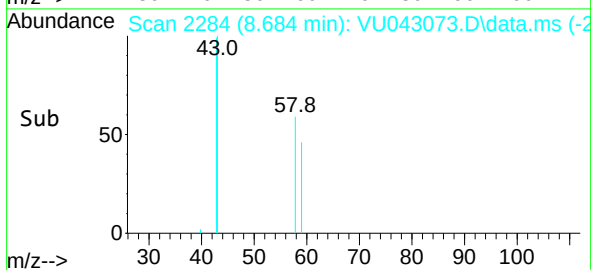

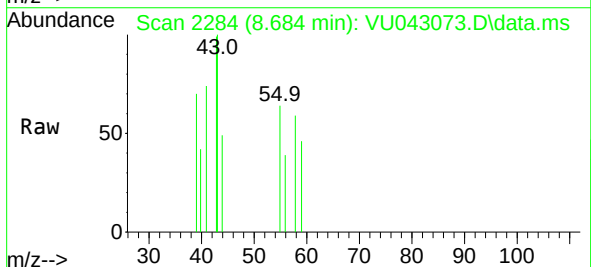


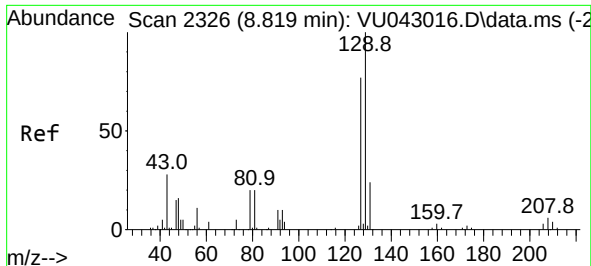

#60
Dibromochloromethane
Concen: 1.61 ug/l
RT: 8.562 min Scan# 2246
Delta R.T. -0.257 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:129 Resp: 3371
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.3#

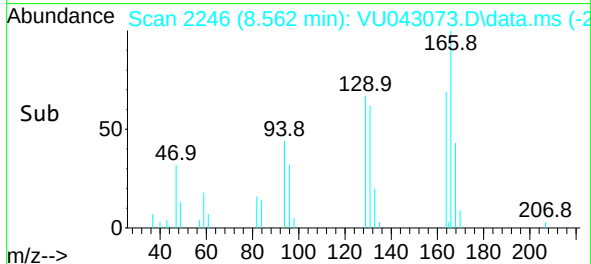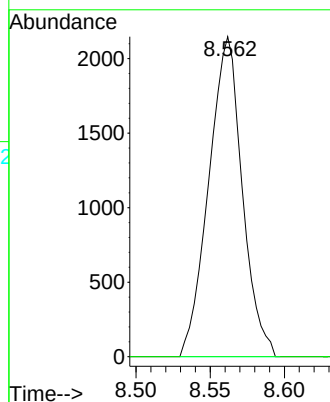

#62
4-Bromofluorobenzene
Concen: 45.08 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion: 95 Resp: 107881
Ion Ratio Lower Upper
95 100
174 87.5 0.0 172.2
176 84.1 0.0 168.8


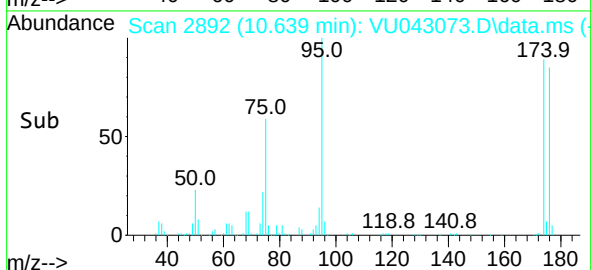
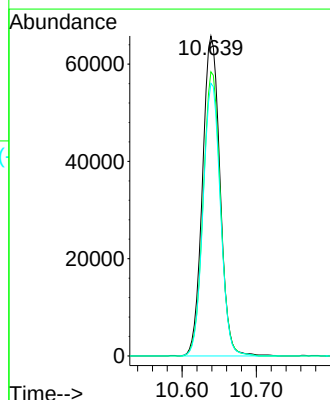
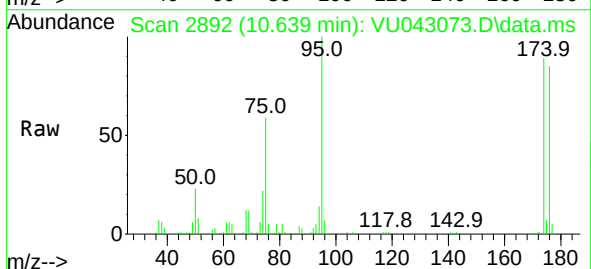




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. 0.000 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:117 Resp: 215718
Ion Ratio Lower Upper
117 100
82 58.3 45.8 68.6
119 32.9 25.8 38.8

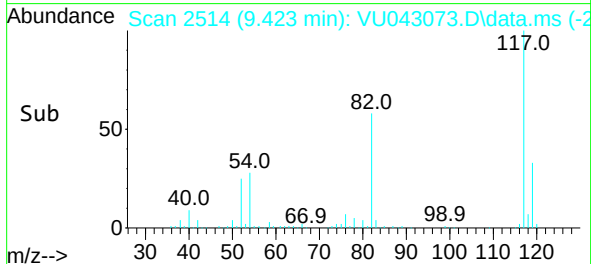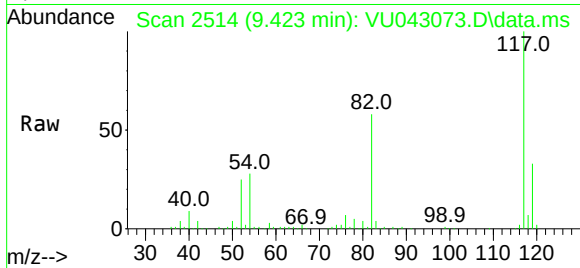

#64
Tetrachloroethene
Concen: 2.44 ug/l
RT: 8.559 min Scan# 2245
Delta R.T. 0.001 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion:164 Resp: 3820
Ion Ratio Lower Upper
164 100
166 131.7 105.3 157.9
129 86.0 75.0 112.6
131 84.5 71.0 106.6


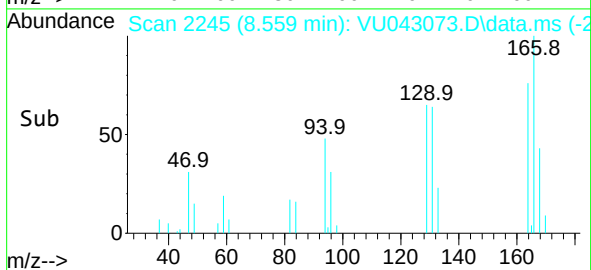

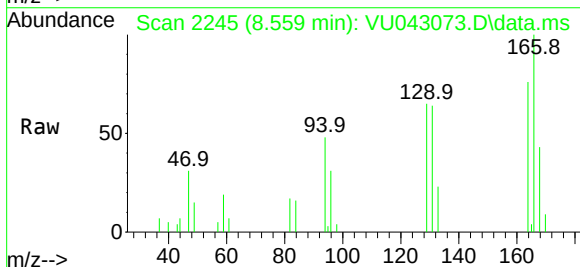




#68
m/p-Xylenes
Concen: 0.31 ug/l
RT: 9.700 min Scan# 2600
Delta R.T. -0.000 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:106 Resp: 958
Ion Ratio Lower Upper
106 100
91 222.7 169.9 254.9

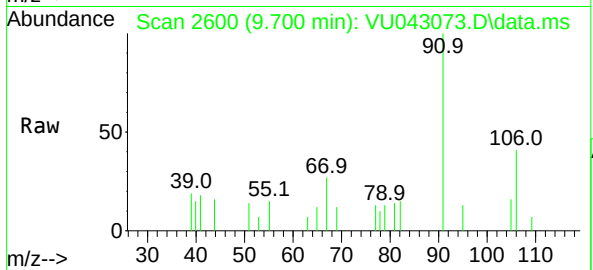

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 11.819 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion:152 Resp: 112160
Ion Ratio Lower Upper
152 100
115 58.8 41.5 124.6
150 153.1 0.0 342.4


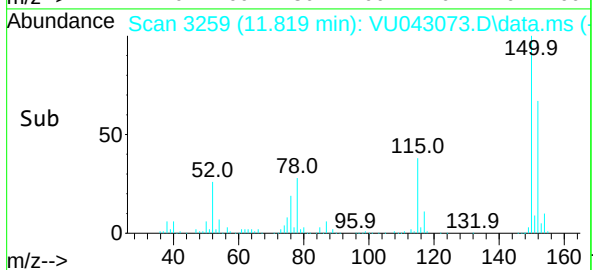

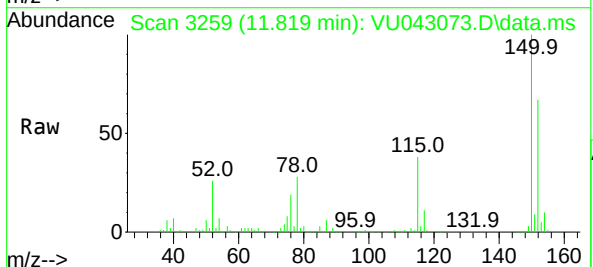


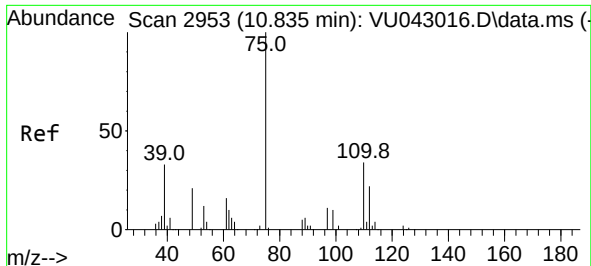

#76
1,2,3-Trichloropropane
Concen: 19.20 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.196 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 75 Resp: 62928
Ion Ratio Lower Upper
75 100
77 0.9 20.2 60.5#

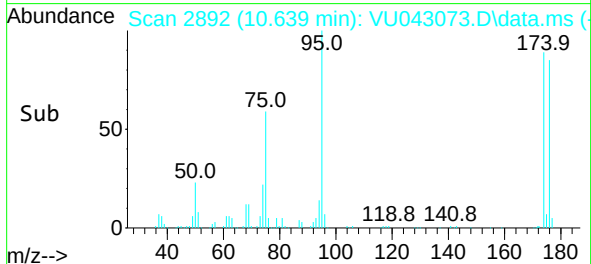

#81
trans-1,4-Dichloro-2-butene
Concen: 56.42 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.084 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Tgt Ion: 75 Resp: 62928
Ion Ratio Lower Upper
75 100
53 0.0 85.6 128.4#
89 0.0 35.7 53.5#


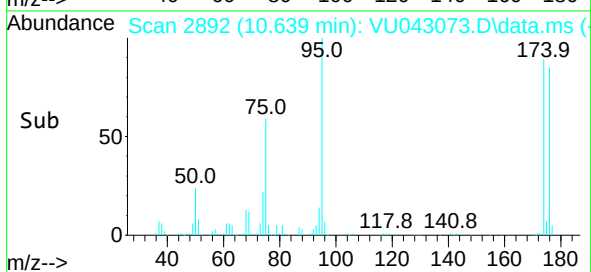

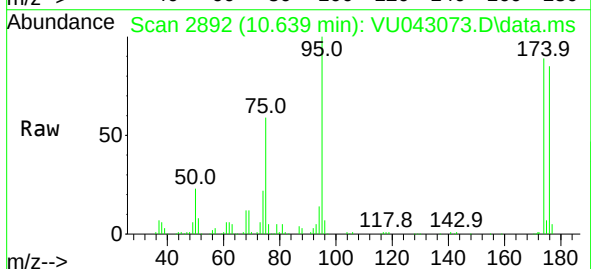


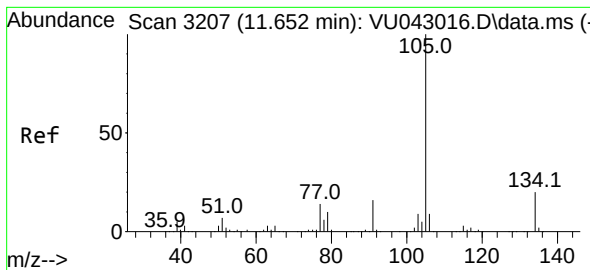

#85
 sec-Butylbenzene
 Concen: 0.47 ug/l
 RT: 11.652 min Scan# 3207
 Delta R.T. -0.000 min
 Lab File: VU043073.D
 Acq: 14 Apr 2021 00:15




Instrument :
 MSVOA_U
 ClientSampled :


Tgt Ion:105 Resp: 3608
 Ion Ratio Lower Upper
 105 100
 134 20.8 10.0 30.0

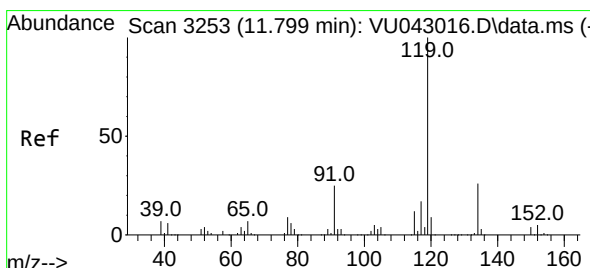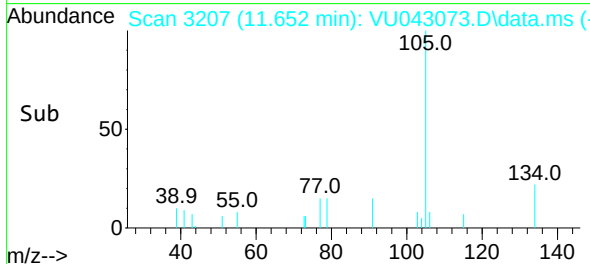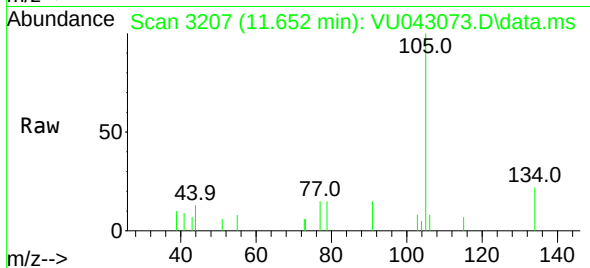

#86
 p-Isopropyltoluene
 Concen: 0.23 ug/l
 RT: 12.015 min Scan# 3320
 Delta R.T. 0.216 min
 Lab File: VU043073.D
 Acq: 14 Apr 2021 00:15

Tgt Ion:119 Resp: 1588
 Ion Ratio Lower Upper
 119 100
 134 23.0 13.2 39.6
 91 24.6 12.8 38.3


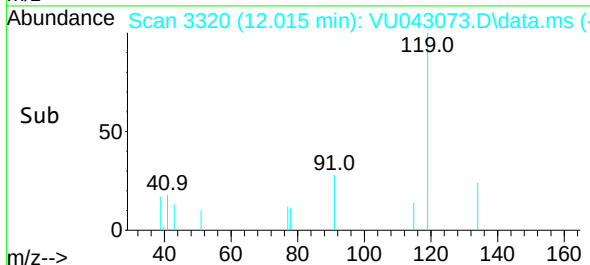

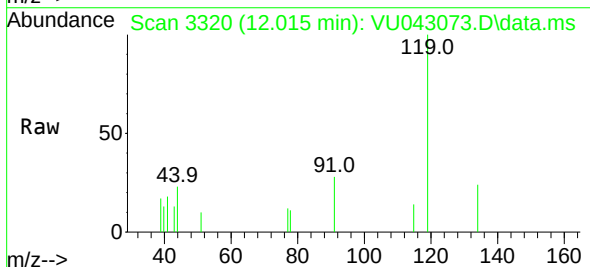


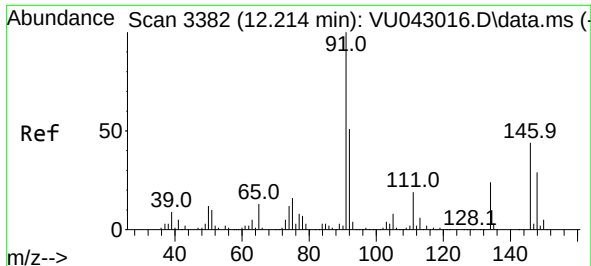

#89
n-Butylbenzene
Concen: 0.33 ug/l
RT: 12.195 min Scan# 3376
Delta R.T. -0.019 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 91 Resp: 2158
Ion Ratio Lower Upper
91 100
92 5.2 26.2 78.6#
134 100.5 12.7 38.1#

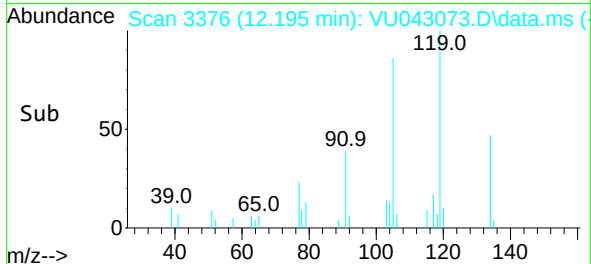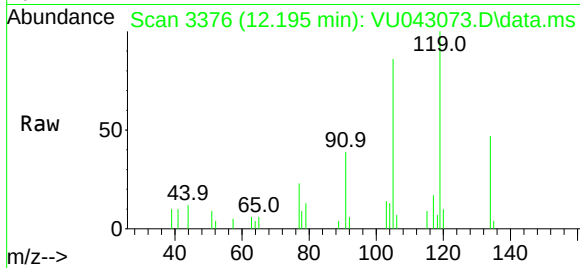

#90
Hexachloroethane
Concen: 0.47 ug/l
RT: 12.311 min Scan# 3412
Delta R.T. -0.173 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15


Tgt Ion: 117 Resp: 619
Ion Ratio Lower Upper
117 100
201 0.0 43.5 130.7#

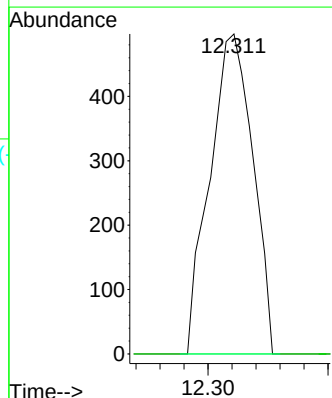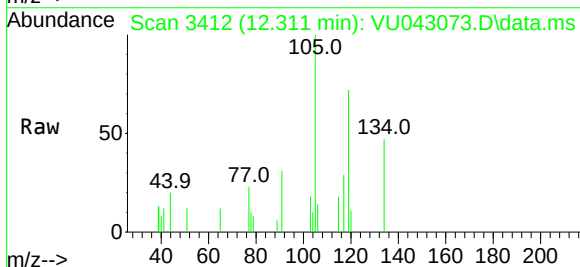



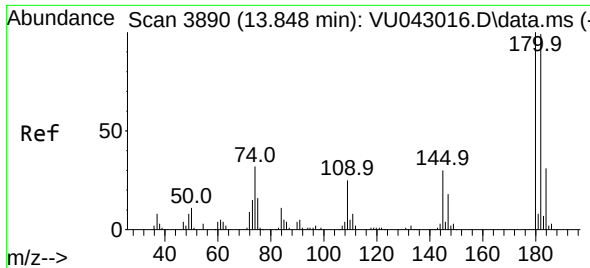


#93
1,2,4-Trichlorobenzene
Concen: 1.55 ug/l
RT: 13.851 min Scan# 3891
Delta R.T. 0.003 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15

Instrument :
MSVOA_U
ClientSampled :



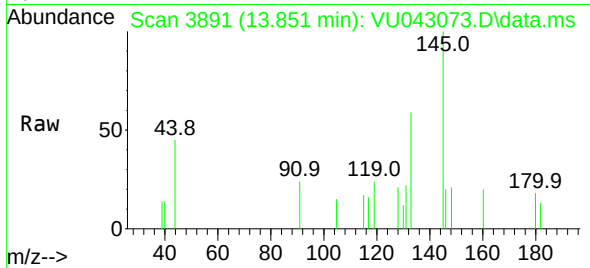



Tgt Ion:180 Resp: 104
Ion Ratio Lower Upper
180 100
182 67.3 46.9 140.8
145 1649.0 14.4 43.4#

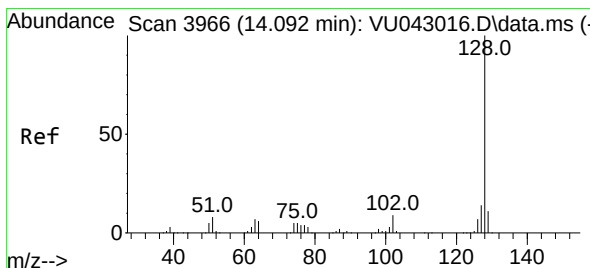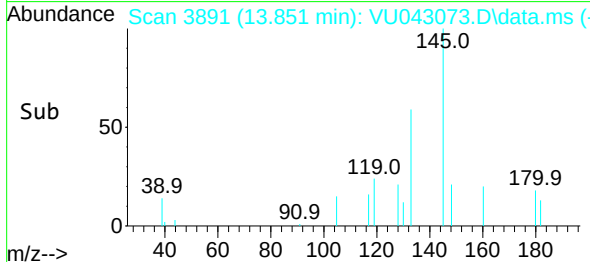

#95
Naphthalene
Concen: 3.04 ug/l
RT: 14.098 min Scan# 3968
Delta R.T. 0.006 min
Lab File: VU043073.D
Acq: 14 Apr 2021 00:15


Tgt Ion:128 Resp: 2580
Ion Ratio Lower Upper
128 100
127 7.3 10.8 16.2#
129 0.0 8.6 13.0#

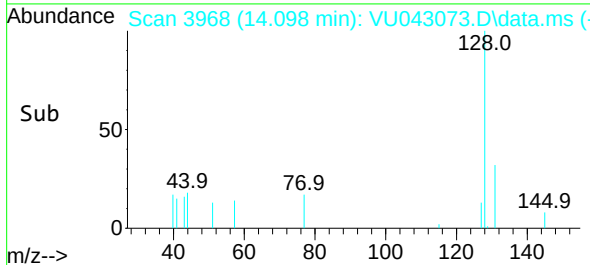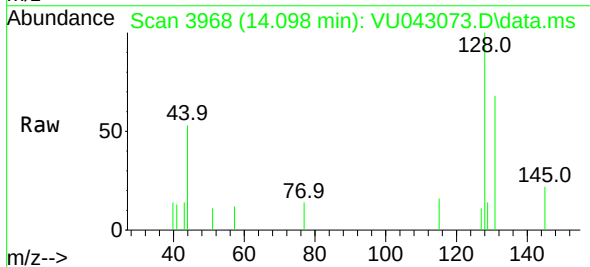

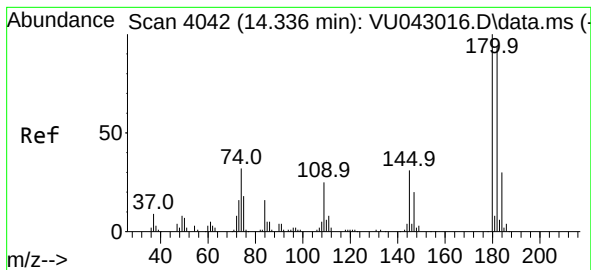

#96
 1,2,3-Trichlorobenzene
 Concen: 1.48 ug/l
 RT: 14.343 min Scan# 4044
 Delta R.T. 0.007 min
 Lab File: VU043073.D
 Acq: 14 Apr 2021 00:15

Instrument :
 MSVOA_U
 ClientSampleId :

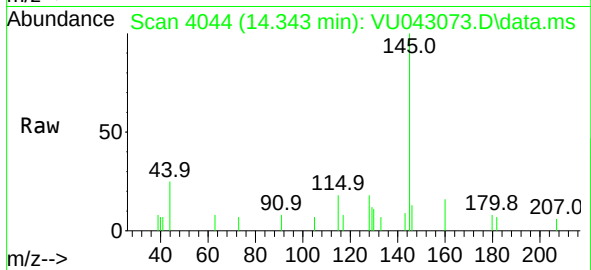

Tgt Ion:180 Resp: 47
 Ion Ratio Lower Upper
 180 100
 182 351.1 48.0 144.0#
 145 12714.9 15.5 46.5#

