

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
 Data File : VU043079.D
 Acq On : 14 Apr 2021 02:33
 Operator : SY/MD
 Sample : M1966-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Apr 14 05:11:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
 Quant Title : SW846 8260
 QLast Update : Mon Apr 12 13:17:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.382	168	130822	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	215371	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	207020	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	103645	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	107231	48.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.52%	
35) Dibromofluoromethane	5.298	113	75853	46.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.74%	
50) Toluene-d8	7.906	98	270394	47.22	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.44%	
62) 4-Bromofluorobenzene	10.639	95	102647	44.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.52%	
Target Compounds						Qvalue
3) Chloromethane	1.523	50	317	Below Cal	#	41
4) Vinyl Chloride	1.736	62	1485	1.01	ug/l #	85
11) Tert butyl alcohol	3.195	59	25628	45.21	ug/l #	97
15) Acrylonitrile	3.189	53	445	0.36	ug/l #	16
16) Acetone	2.636	43	8053	5.93	ug/l	93
18) Methyl Acetate	2.771	43	2068	0.75	ug/l #	55
19) Methyl tert-butyl Ether	3.375	73	1742	0.36	ug/l	92
25) 2-Butanone	4.726	43	1099	0.55	ug/l #	54
26) 2,2-Dichloropropane	4.639	77	2619	1.04	ug/l #	55
29) Tetrahydrofuran	5.070	42	357	0.28	ug/l #	51
31) Cyclohexane	5.382	56	3462	1.28	ug/l #	35
36) 1,1-Dichloropropene	5.382	75	10624	4.65	ug/l #	49
37) Ethyl Acetate	4.726	43	1099	0.28	ug/l #	71
38) Carbon Tetrachloride	5.382	117	13063	5.33	ug/l #	15
40) Benzene	5.784	78	89292	13.68	ug/l	99
42) 1,2-Dichloroethane	5.787	62	1146	0.40	ug/l #	79
43) Isopropyl Acetate	5.973	43	1185	0.21	ug/l #	64
59) 2-Hexanone	8.497	43	3304	0.97	ug/l	75
68) m/p-Xylenes	9.697	106	3788	1.28	ug/l	98
69) o-Xylene	10.105	106	4725	1.63	ug/l	97
74) N-amyl acetate	10.388	43	1203	0.27	ug/l #	50
75) 1,1,2,2-Tetrachloroethane	10.909	83	3074	1.01	ug/l #	26
76) 1,2,3-Trichloropropane	10.639	75	58004	19.15	ug/l #	36
80) 1,3,5-Trimethylbenzene	11.095	105	1868	0.30	ug/l	94
81) trans-1,4-Dichloro-2-b...	10.639	75	58004	56.28	ug/l #	7
84) 1,2,4-Trimethylbenzene	11.475	105	2285	0.36	ug/l	93
85) sec-Butylbenzene	11.475	105	2285	0.32	ug/l #	56
89) n-Butylbenzene	12.102	91	5767	0.95	ug/l #	44
90) Hexachloroethane	12.324	117	727	0.60	ug/l #	6
95) Naphthalene	14.095	128	85613	13.53	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
Data File : VU043079.D
Acq On : 14 Apr 2021 02:33
Operator : SY/MD
Sample : M1966-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Apr 14 05:11:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Quant Title : SW846 8260
QLast Update : Mon Apr 12 13:17:29 2021
Response via : Initial Calibration




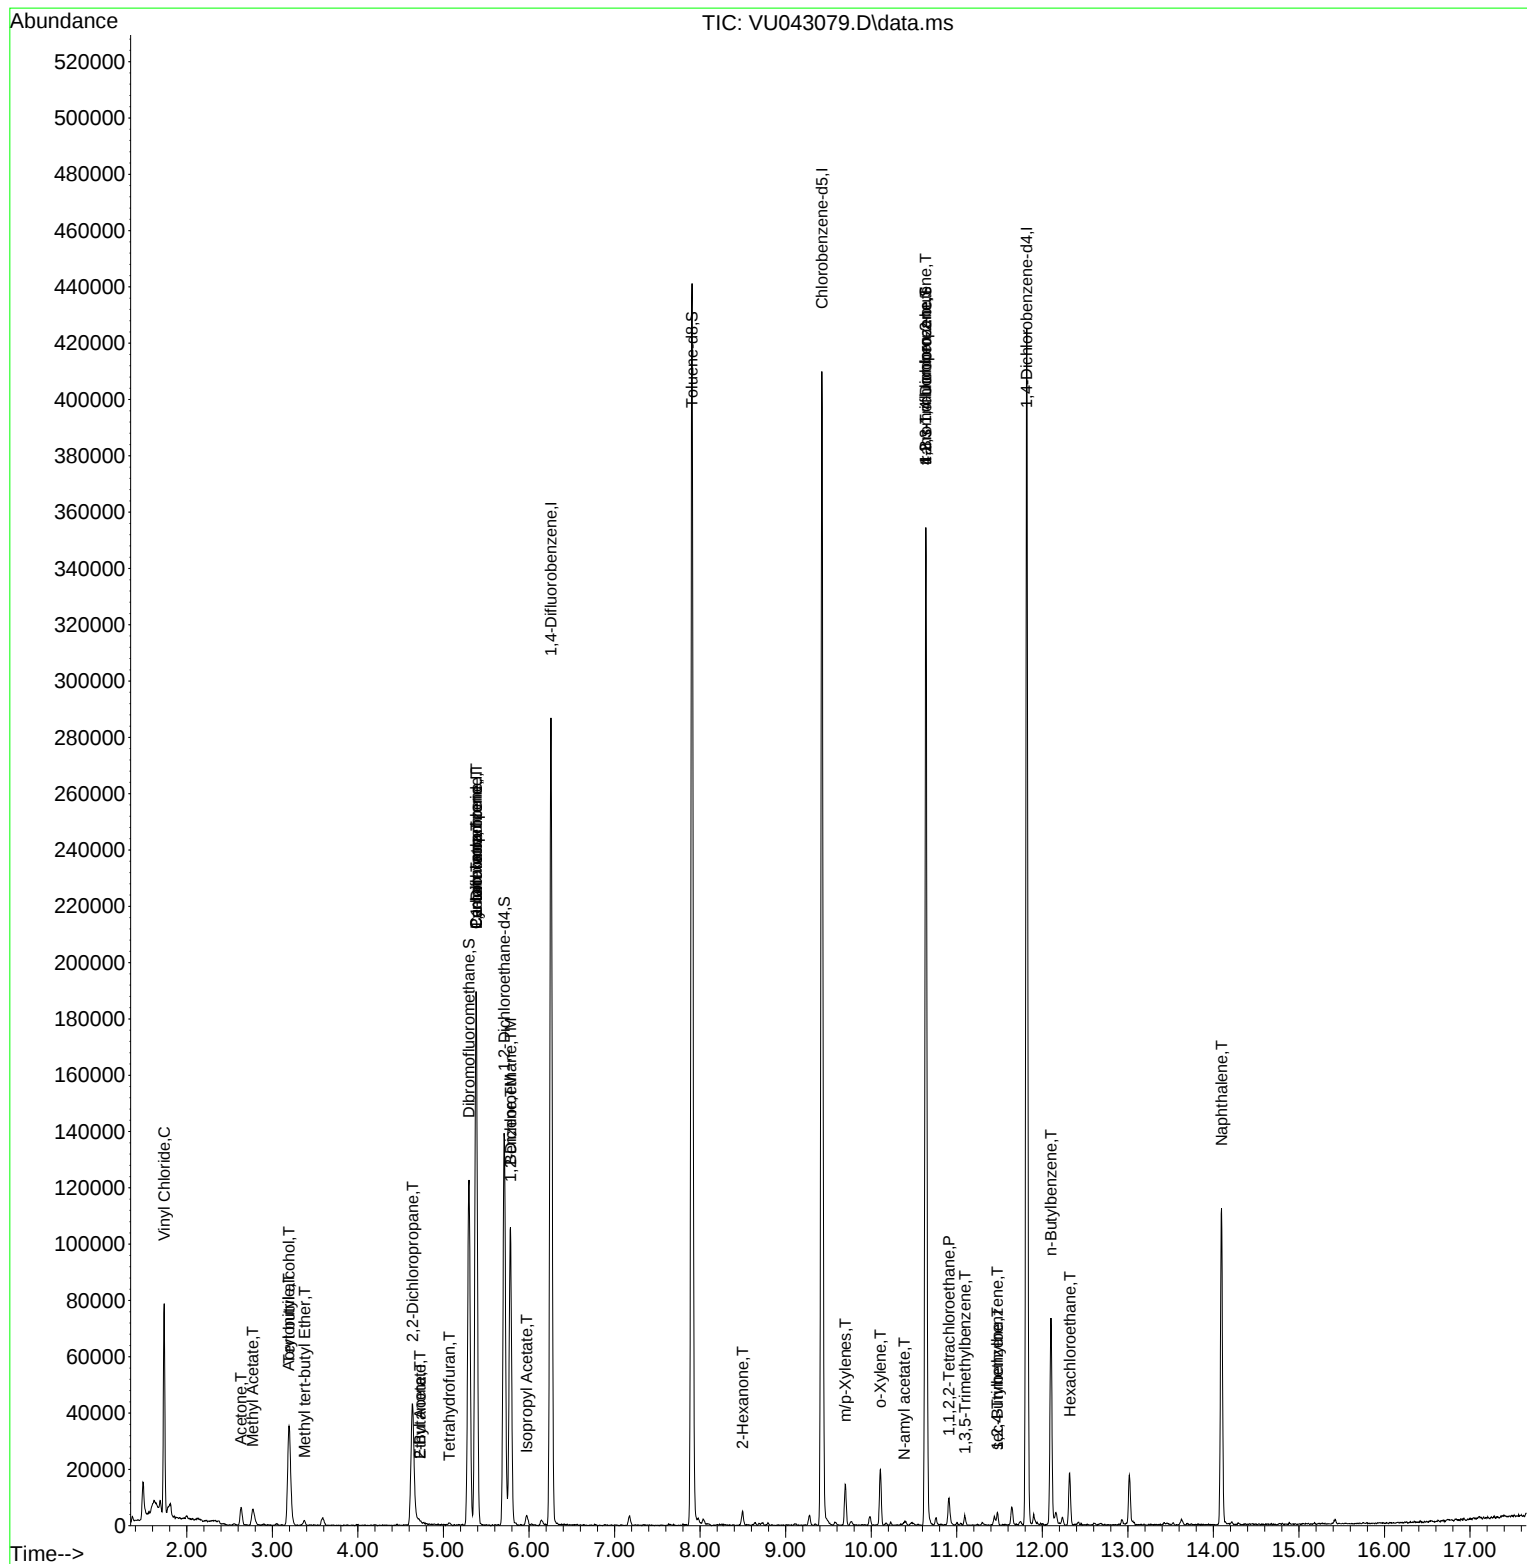




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:168 Resp: 130822
Ion Ratio Lower Upper
168 100
99 58.0 45.0 67.4

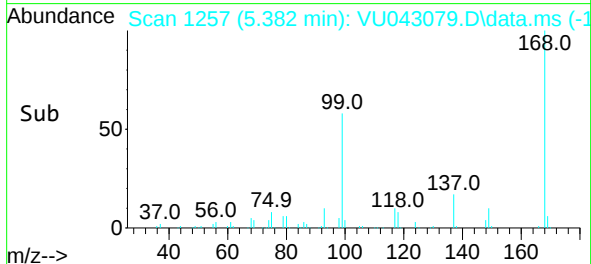

#3
Chloromethane
Concen: Below Cal
RT: 1.523 min Scan# 57
Delta R.T. 0.003 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion: 50 Resp: 317
Ion Ratio Lower Upper
50 100
52 0.0 26.6 40.0#


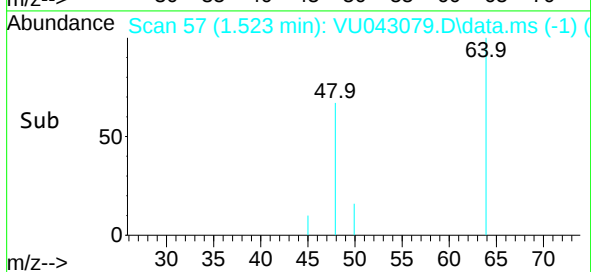

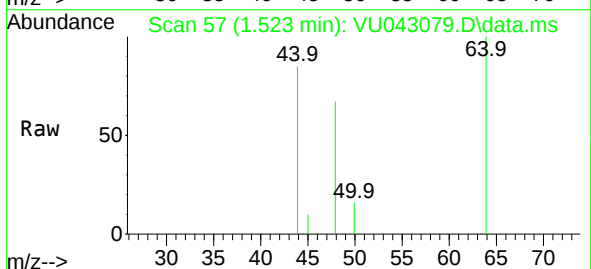


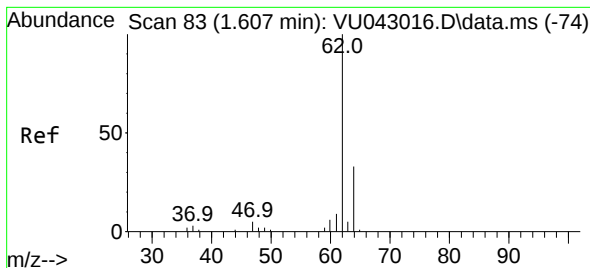

#4
 Vinyl Chloride
 Concen: 1.01 ug/l
 RT: 1.736 min Scan# 123
 Delta R.T. 0.129 min
 Lab File: VU043079.D
 Acq: 14 Apr 2021 02:33




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion: 62 Resp: 1485
 Ion Ratio Lower Upper
 62 100
 64 39.9 25.2 37.8#

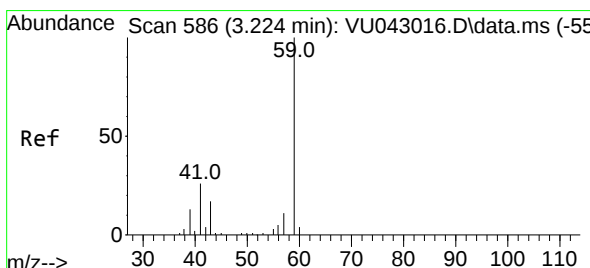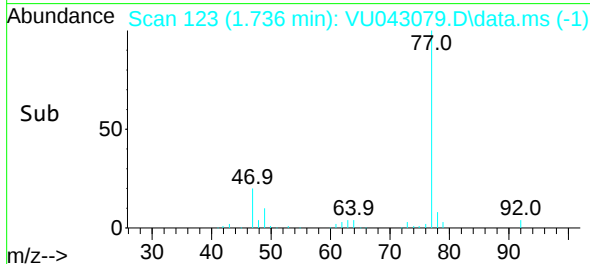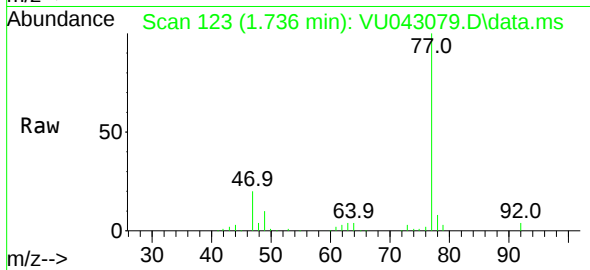

#11
 Tert butyl alcohol
 Concen: 45.21 ug/l
 RT: 3.195 min Scan# 577
 Delta R.T. -0.029 min
 Lab File: VU043079.D
 Acq: 14 Apr 2021 02:33

Tgt Ion: 59 Resp: 25628
 Ion Ratio Lower Upper
 59 100
 57 3.1 1.6 2.4#


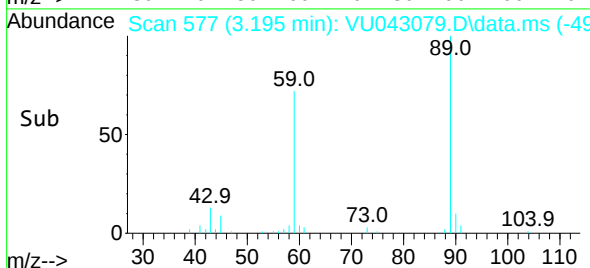

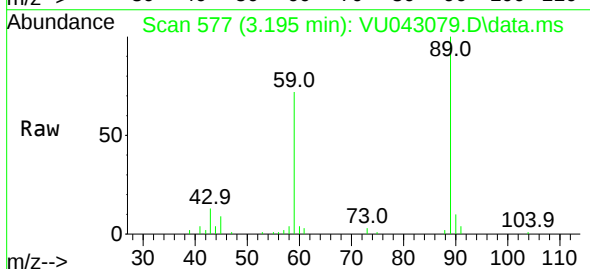




#15
Acrylonitrile
Concen: 0.36 ug/l
RT: 3.189 min Scan# 575
Delta R.T. -0.128 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 53 Resp: 445
Ion Ratio Lower Upper
53 100
52 0.0 68.2 102.2#
51 0.0 29.2 43.8#

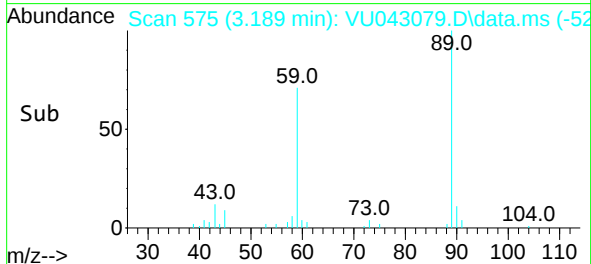

#16
Acetone
Concen: 5.93 ug/l
RT: 2.636 min Scan# 403
Delta R.T. 0.007 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33


Tgt Ion: 43 Resp: 8053
Ion Ratio Lower Upper
43 100
58 23.5 21.5 32.3

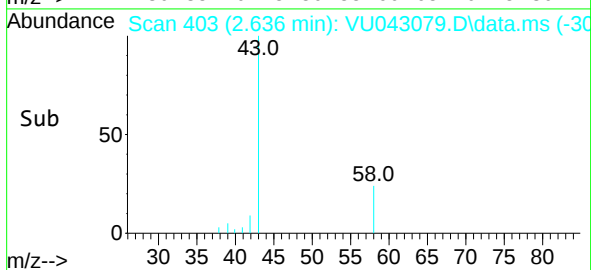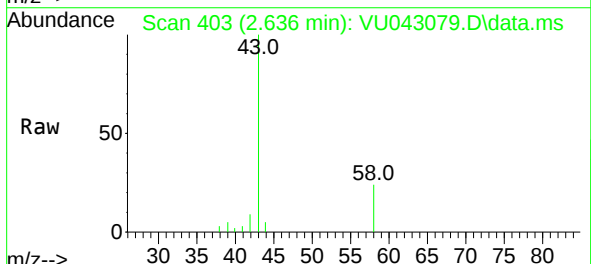






#18
Methyl Acetate
Concen: 0.75 ug/l
RT: 2.771 min Scan# 445
Delta R.T. -0.180 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Instrument :
MSVOA_U
ClientSampled :



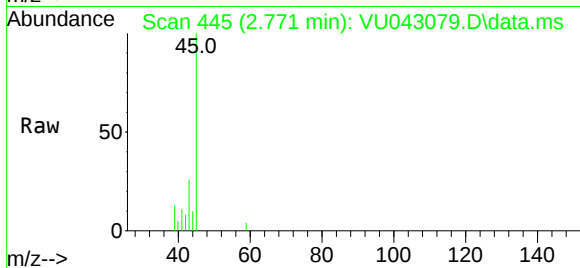



Tgt Ion: 43 Resp: 2068
Ion Ratio Lower Upper
43 100
74 0.0 16.6 25.0#

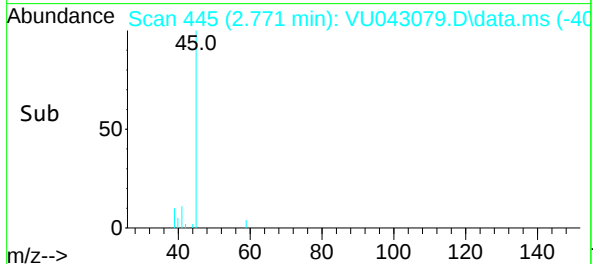

#19
Methyl tert-butyl Ether
Concen: 0.36 ug/l
RT: 3.375 min Scan# 633
Delta R.T. 0.006 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion: 73 Resp: 1742
Ion Ratio Lower Upper
73 100
57 27.3 18.8 28.2


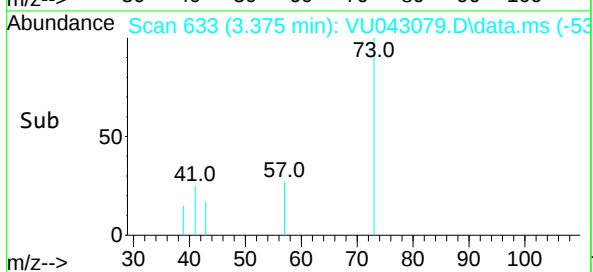

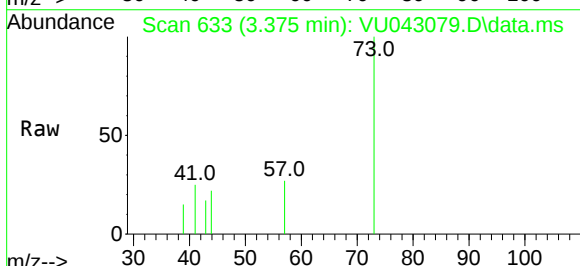




#25
2-Butanone
Concen: 0.55 ug/l
RT: 4.726 min Scan# 1053
Delta R.T. 0.019 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 43 Resp: 1099
Ion Ratio Lower Upper
43 100
72 0.0 17.4 26.0#



#26
2,2-Dichloropropane
Concen: 1.04 ug/l
RT: 4.639 min Scan# 1026
Delta R.T. -0.032 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion: 77 Resp: 2619
Ion Ratio Lower Upper
77 100
97 0.0 10.6 31.8#

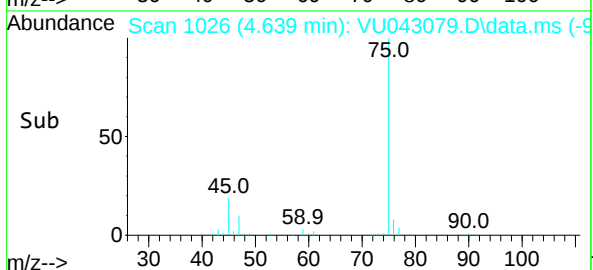



#29

Tetrahydrofuran

Concen: 0.28 ug/l

RT: 5.070 min Scan# 1160





Delta R.T. 0.016 min

Lab File: VU043079.D

Acq: 14 Apr 2021 02:33

Tgt Ion:	42	Resp:	357
Ion	Ratio	Lower	Upper
42	100		
72	16.8	31.5	47.3#
71	0.0	29.5	44.3#

Instrument :
MSVOA_U
ClientSampleId :

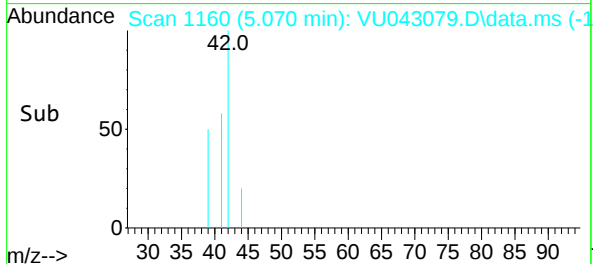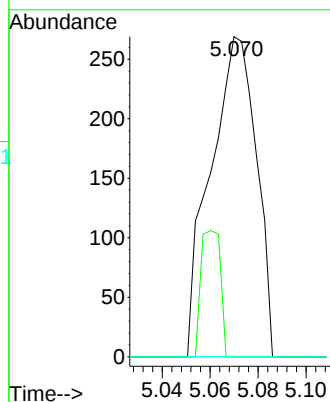

#31

Cyclohexane

Concen: 1.28 ug/l




RT: 5.382 min Scan# 1257


Delta R.T. -0.013 min

Lab File: VU043079.D

Acq: 14 Apr 2021 02:33

Tgt Ion:	56	Resp:	3462
Ion	Ratio	Lower	Upper
56	100		
69	143.7	24.9	37.3#
84	89.3	63.7	95.5


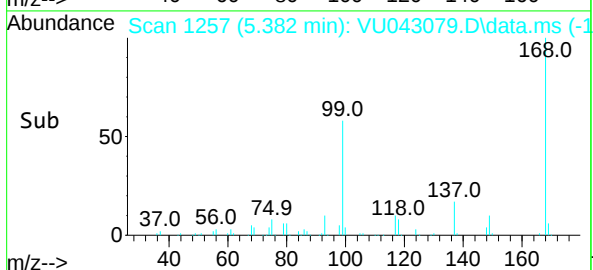
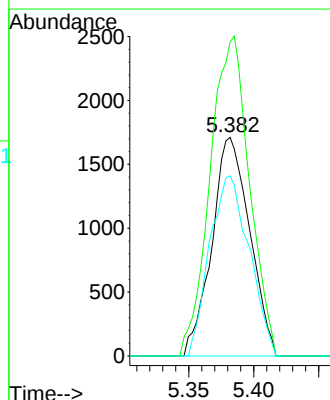





#33
1,2-Dichloroethane-d4
Concen: 48.76 ug/l
RT: 5.710 min Scan# 1359
Delta R.T. -0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 65 Resp: 107231
Ion Ratio Lower Upper
65 100
67 49.6 0.0 99.8

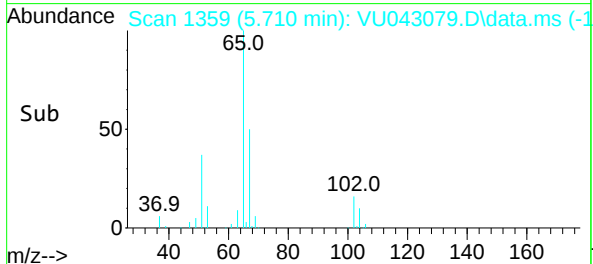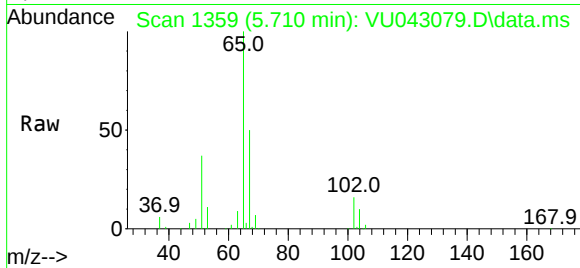

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. 0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion: 114 Resp: 215371
Ion Ratio Lower Upper
114 100
63 22.4 0.0 44.2
88 16.6 0.0 33.4


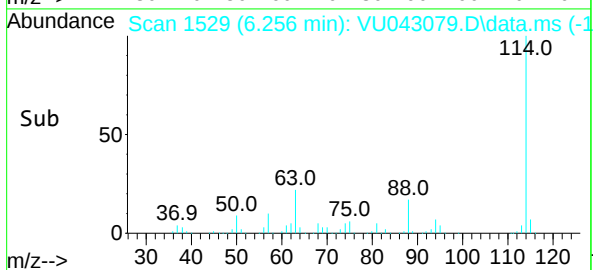

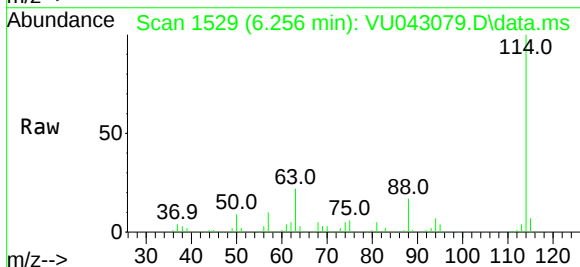




#35
Dibromofluoromethane
Concen: 46.87 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. 0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion:113 Resp: 75853
Ion Ratio Lower Upper
113 100
111 102.8 81.8 122.8
192 21.1 17.2 25.8

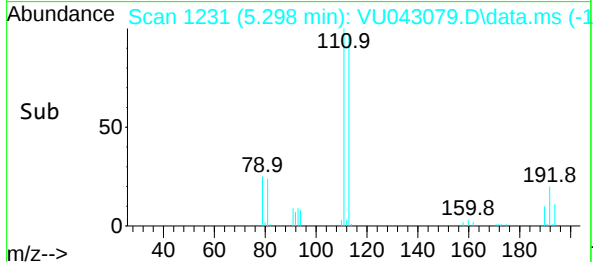

#36
1,1-Dichloropropene
Concen: 4.65 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.151 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion: 75 Resp: 10624
Ion Ratio Lower Upper
75 100
110 7.4 16.8 50.3#
77 0.0 24.8 37.2#

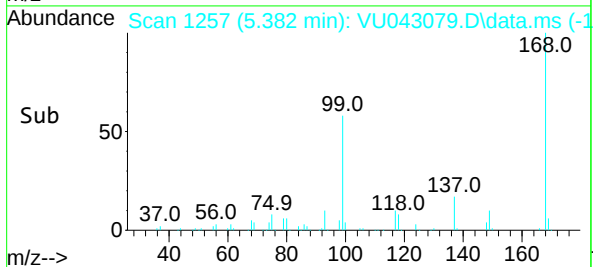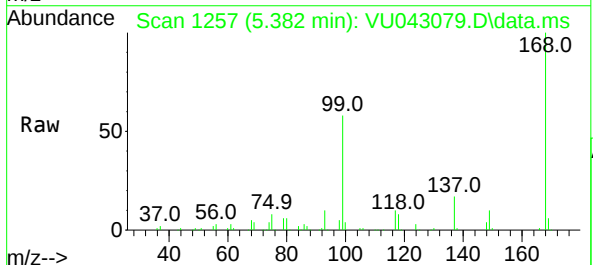



#37

Ethyl Acetate

Concen: 0.28 ug/l

RT: 4.726 min Scan# 1053





Delta R.T. -0.080 min

Lab File: VU043079.D

Acq: 14 Apr 2021 02:33

Tgt Ion:	43	Resp:	1099
Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.1	15.1#
70	0.0	7.2	10.8#

Instrument :
MSVOA_U
ClientSampleId :



#38

Carbon Tetrachloride

Concen: 5.33 ug/l




RT: 5.382 min Scan# 1257


Delta R.T. -0.151 min

Lab File: VU043079.D

Acq: 14 Apr 2021 02:33

Tgt Ion:	117	Resp:	13063
Ion	Ratio	Lower	Upper
117	100		
119	3.6	75.5	113.3#
121	0.0	24.7	37.1#


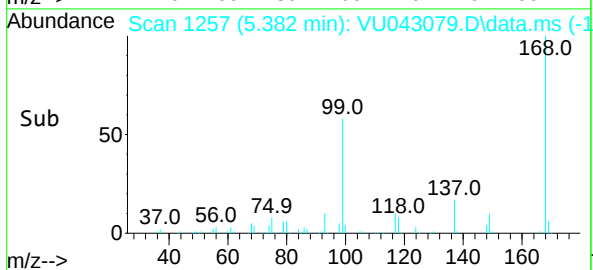

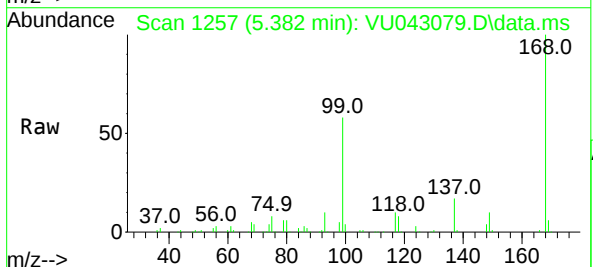




#40
Benzene
Concen: 13.68 ug/l
RT: 5.784 min Scan# 1382
Delta R.T. 0.004 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 78 Resp: 89292
Ion Ratio Lower Upper
78 100
77 24.6 19.3 28.9

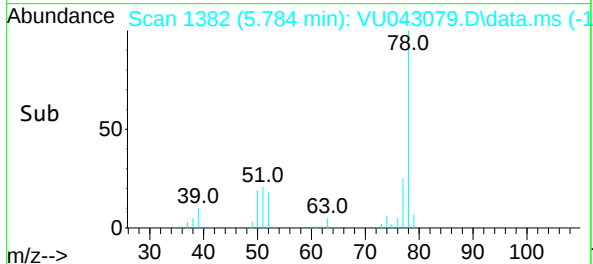

#42
1,2-Dichloroethane
Concen: 0.40 ug/l
RT: 5.787 min Scan# 1383
Delta R.T. -0.013 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion: 62 Resp: 1146
Ion Ratio Lower Upper
62 100
98 0.0 0.0 14.8

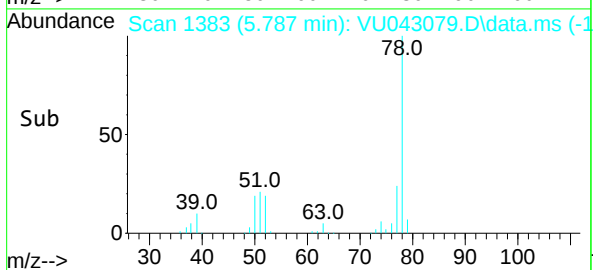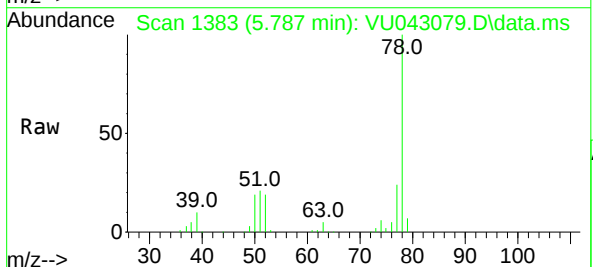







#43

Isopropyl Acetate
 Concen: 0.21 ug/l
 RT: 5.973 min Scan# 1441
 Delta R.T. 0.058 min
 Lab File: VU043079.D
 Acq: 14 Apr 2021 02:33

Instrument :
 MSVOA_U
 ClientSampleId :




Tgt Ion: 43 Resp: 1185
 Ion Ratio Lower Upper
 43 100
 61 0.0 14.4 21.6#
 87 0.0 8.8 13.2#

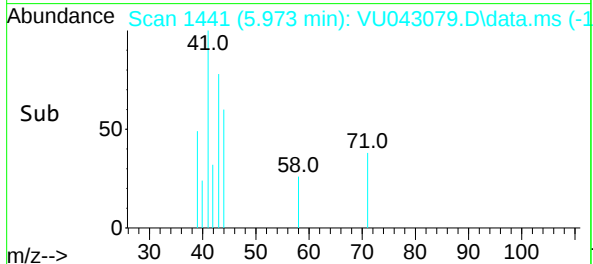


#50

Toluene-d8
 Concen: 47.22 ug/l
 RT: 7.906 min Scan# 2042
 Delta R.T. -0.000 min
 Lab File: VU043079.D
 Acq: 14 Apr 2021 02:33

Tgt Ion: 98 Resp: 270394
 Ion Ratio Lower Upper
 98 100
 100 62.3 50.2 75.2


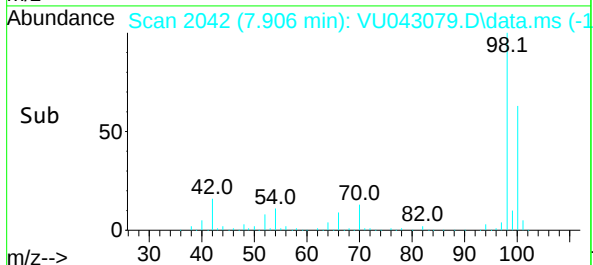

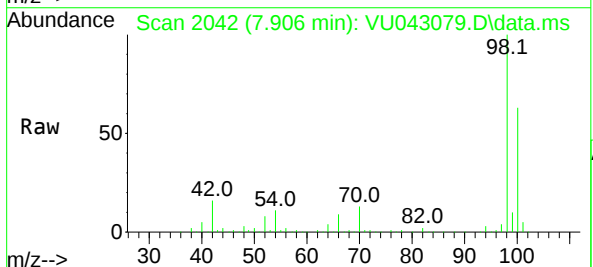




#59
2-Hexanone
Concen: 0.97 ug/l
RT: 8.497 min Scan# 2226
Delta R.T. -0.197 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 43 Resp: 3304
Ion Ratio Lower Upper
43 100
58 30.9 24.0 72.0

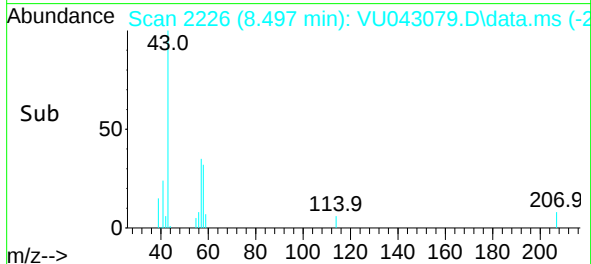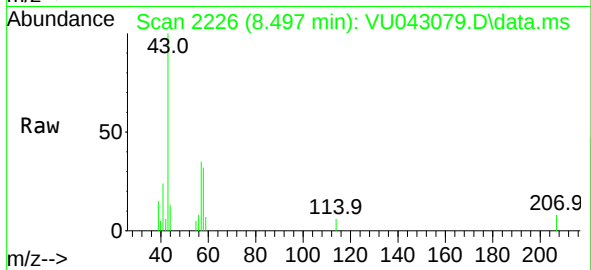

#62
4-Bromofluorobenzene
Concen: 44.76 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33


Tgt Ion: 95 Resp: 102647
Ion Ratio Lower Upper
95 100
174 85.5 0.0 172.2
176 84.2 0.0 168.8

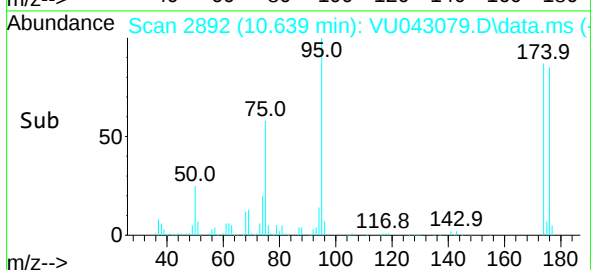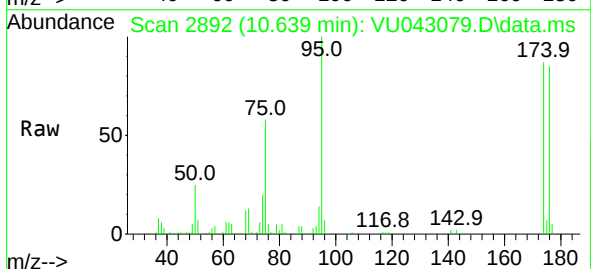






#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. 0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33


Instrument :
MSVOA_U
ClientSampleId :





Tgt Ion:117 Resp: 207020
Ion Ratio Lower Upper
117 100
82 57.4 45.8 68.6
119 32.2 25.8 38.8




#68
m/p-Xylenes
Concen: 1.28 ug/l
RT: 9.697 min Scan# 2599
Delta R.T. -0.003 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33



Tgt Ion:106 Resp: 3788
Ion Ratio Lower Upper
106 100
91 209.6 169.9 254.9




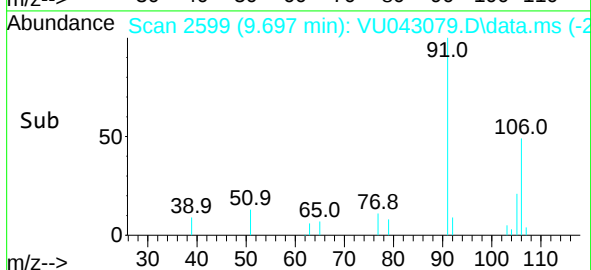




#69
o-Xylene
Concen: 1.63 ug/l
RT: 10.105 min Scan# 2726
Delta R.T. -0.003 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:106 Resp: 4725
Ion Ratio Lower Upper
106 100
91 227.0 111.2 333.6

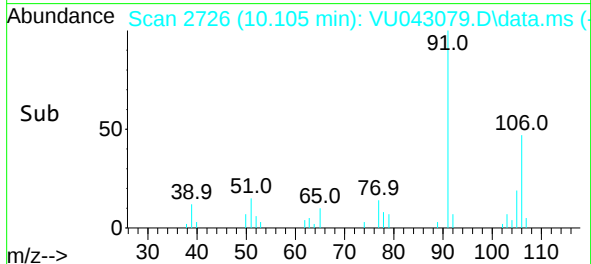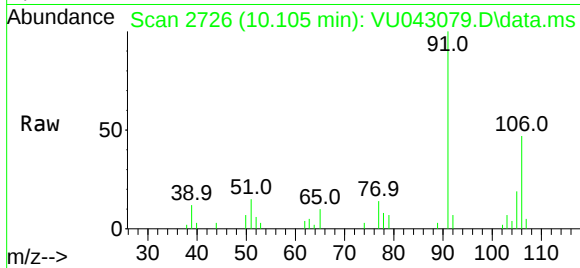

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 11.819 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33


Tgt Ion:152 Resp: 103645
Ion Ratio Lower Upper
152 100
115 58.3 41.5 124.6
150 156.1 0.0 342.4

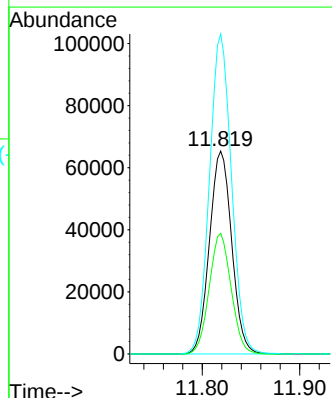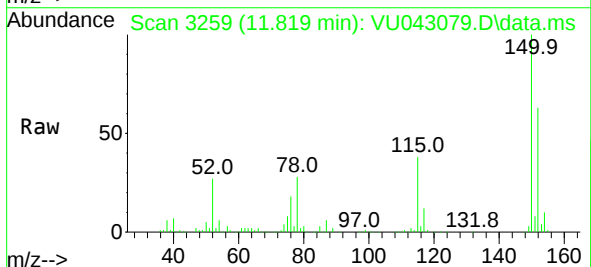






#74
N-amy1 acetate
Concen: 0.27 ug/l
RT: 10.388 min Scan# 2814
Delta R.T. 0.061 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Instrument :
MSVOA_U
ClientSampled :



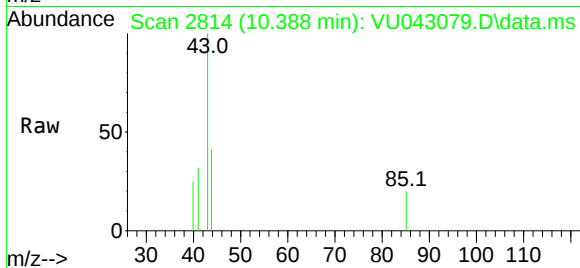



Tgt Ion: 43	Resp: 1203
Ion Ratio	Lower Upper
43 100	
70 0.0	28.3 42.5#
55 3.6	17.2 25.8#
61 0.0	17.3 25.9#

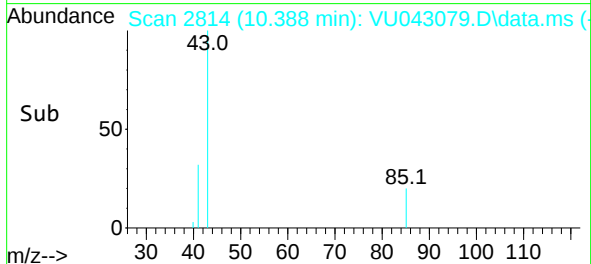

#75
1,1,2,2-Tetrachloroethane
Concen: 1.01 ug/l
RT: 10.909 min Scan# 2976
Delta R.T. 0.119 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion: 83	Resp: 3074
Ion Ratio	Lower Upper
83 100	
131 0.0	5.1 15.2#
85 0.0	31.7 95.1#


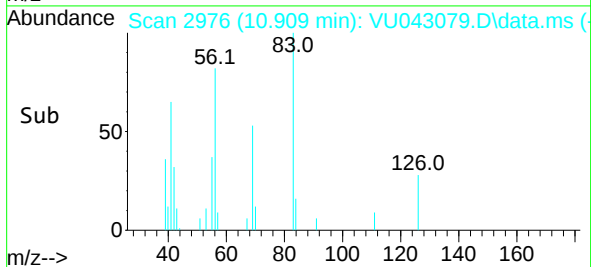

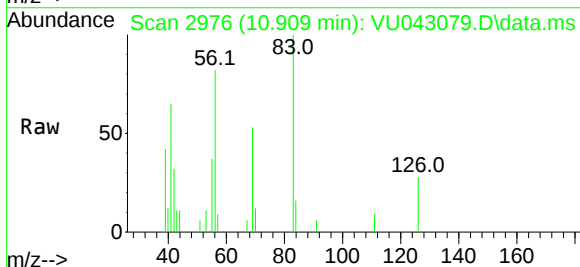




#76
1,2,3-Trichloropropane
Concen: 19.15 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.196 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 75 Resp: 58004
Ion Ratio Lower Upper
75 100
77 0.8 20.2 60.5#

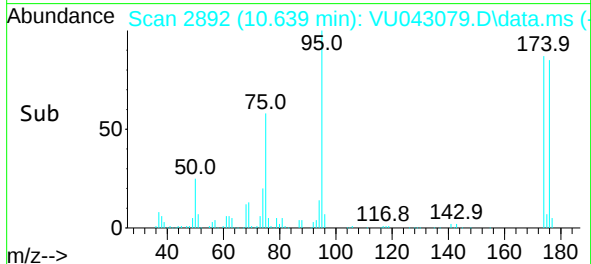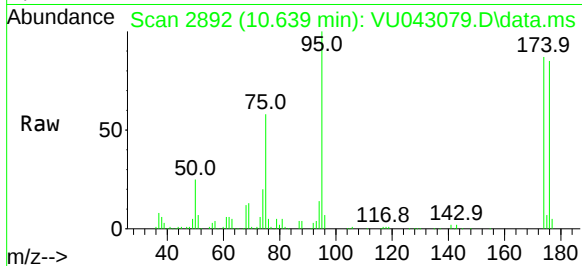

#80
1,3,5-Trimethylbenzene
Concen: 0.30 ug/l
RT: 11.095 min Scan# 3034
Delta R.T. 0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion:105 Resp: 1868
Ion Ratio Lower Upper
105 100
120 51.3 23.8 71.4


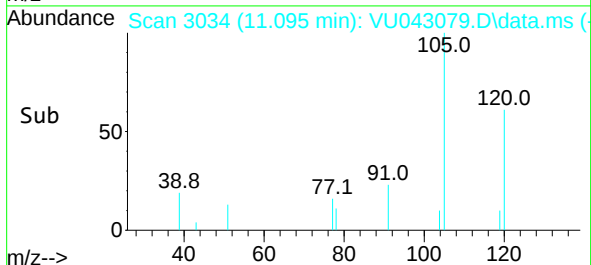

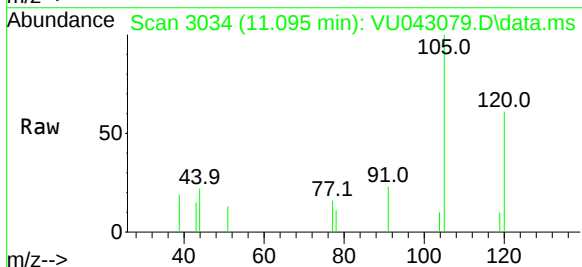




#81
trans-1,4-Dichloro-2-butene
Concen: 56.28 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.084 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 75 Resp: 58004
Ion Ratio Lower Upper
75 100
53 0.0 85.6 128.4#
89 0.0 35.7 53.5#

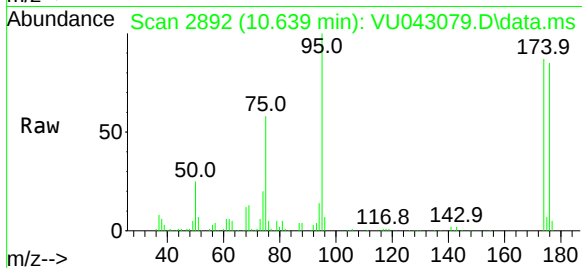

#84
1,2,4-Trimethylbenzene
Concen: 0.36 ug/l
RT: 11.475 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion: 105 Resp: 2285
Ion Ratio Lower Upper
105 100
120 40.2 22.3 66.8


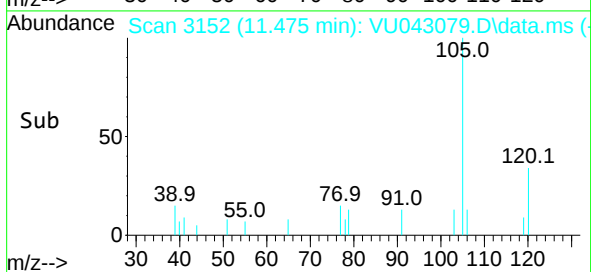

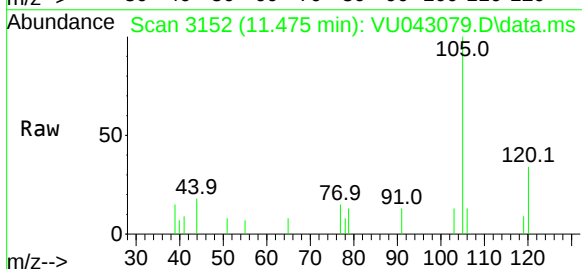




#85
 sec-Butylbenzene
 Concen: 0.32 ug/l
 RT: 11.475 min Scan# 3152
 Delta R.T. -0.177 min
 Lab File: VU043079.D
 Acq: 14 Apr 2021 02:33




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion:105 Resp: 2285
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 30.0#

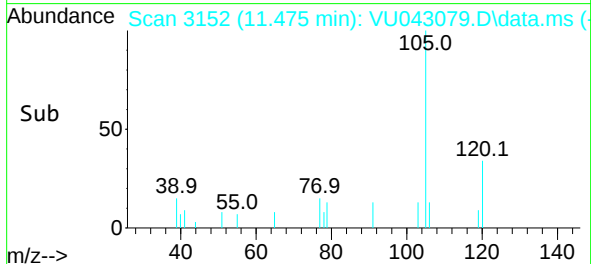

#89
 n-Butylbenzene
 Concen: 0.95 ug/l
 RT: 12.102 min Scan# 3347
 Delta R.T. -0.112 min
 Lab File: VU043079.D
 Acq: 14 Apr 2021 02:33

Tgt Ion: 91 Resp: 5767
 Ion Ratio Lower Upper
 91 100
 92 11.0 26.2 78.6#
 134 0.0 12.7 38.1#


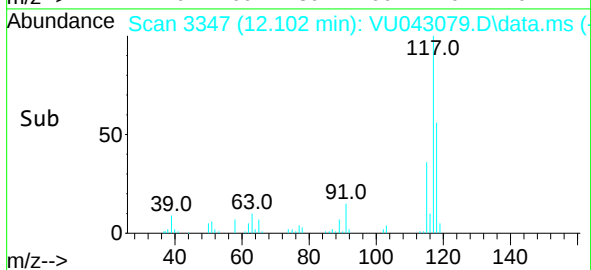

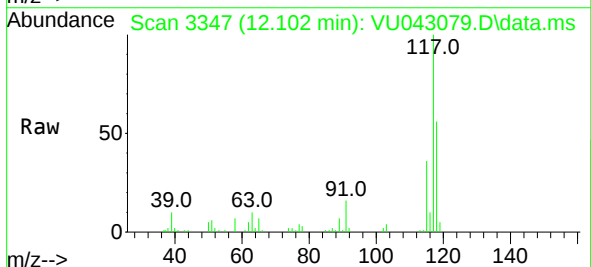


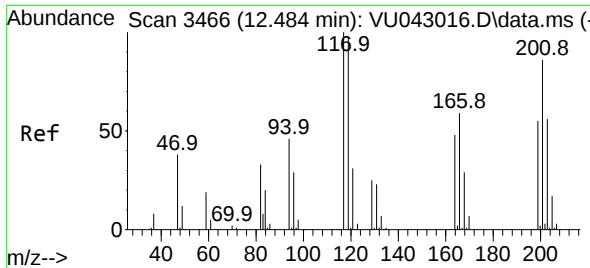

#90
Hexachloroethane
Concen: 0.60 ug/l
RT: 12.324 min Scan# 3416
Delta R.T. -0.160 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Instrument :
MSVOA_U
ClientSampled :

Tgt Ion:117 Resp: 727
Ion Ratio Lower Upper
117 100
201 0.0 43.5 130.7#

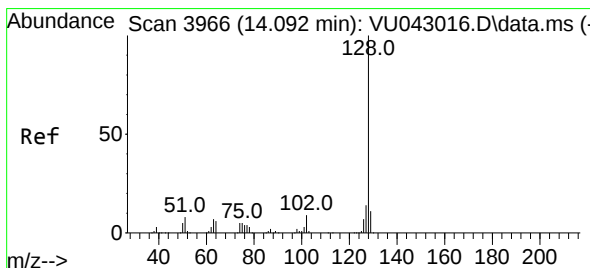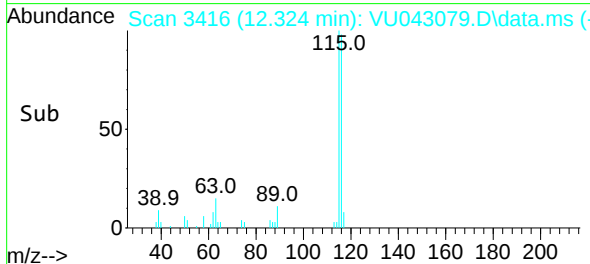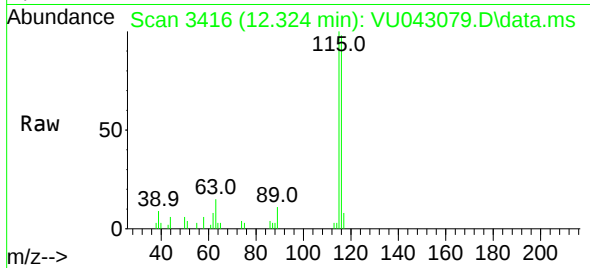

#95
Naphthalene
Concen: 13.53 ug/l
RT: 14.095 min Scan# 3967
Delta R.T. 0.003 min
Lab File: VU043079.D
Acq: 14 Apr 2021 02:33

Tgt Ion:128 Resp: 85613
Ion Ratio Lower Upper
128 100
127 14.0 10.8 16.2
129 11.3 8.6 13.0

