

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
 Data File : VU043078.D
 Acq On : 14 Apr 2021 02:10
 Operator : SY/MD
 Sample : M1966-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-110RR

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
 Title : SW846 8260

Signal : TIC: VU043078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	40	47	63	rBV3	11513	23058	2.94%	0.439%
2	1.736	115	123	132	rVB	57974	71020	9.06%	1.353%
3	2.642	394	405	417	rBV2	5474	10418	1.33%	0.198%
4	3.195	561	577	596	rBV2	26820	69444	8.86%	1.323%
5	4.645	1009	1028	1059	rBV2	43481	136386	17.40%	2.598%
6	5.298	1216	1231	1244	rBV	127157	269588	34.40%	5.135%
7	5.382	1244	1257	1274	rVB	194377	395953	50.53%	7.541%
8	5.710	1344	1359	1371	rBV	140649	288480	36.81%	5.494%
9	5.784	1371	1382	1402	rVB	107650	221828	28.31%	4.225%
10	5.973	1429	1441	1452	rBV6	4123	8018	1.02%	0.153%
11	6.256	1514	1529	1553	rBV	295283	556544	71.02%	10.600%
12	7.906	2024	2042	2058	rBV	456172	783658	100.00%	14.925%
13	8.497	2218	2226	2237	rVB4	5257	8310	1.06%	0.158%
14	9.423	2501	2514	2536	rBV	420650	694828	88.66%	13.234%
15	9.697	2590	2599	2609	rBV2	13920	22008	2.81%	0.419%
16	10.108	2717	2727	2739	rVB	19838	30923	3.95%	0.589%
17	10.639	2879	2892	2913	rBV	356341	571799	72.97%	10.890%
18	10.912	2967	2977	2993	rVB3	9136	17365	2.22%	0.331%
19	11.645	3192	3205	3219	rBV5	7047	11846	1.51%	0.226%
20	11.819	3245	3259	3279	rVB	441472	701385	89.50%	13.358%
21	12.102	3333	3347	3359	rBV	73098	117917	15.05%	2.246%
22	12.317	3404	3414	3426	rBV2	16942	26344	3.36%	0.502%
23	13.018	3622	3632	3645	rBV4	17914	28667	3.66%	0.546%
24	14.095	3953	3967	3983	rBV	112843	184710	23.57%	3.518%




Sum of corrected areas: 5250497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
Data File : VU043078.D
Acq On : 14 Apr 2021 02:10
Operator : SY/MD
Sample : M1966-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-110RR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

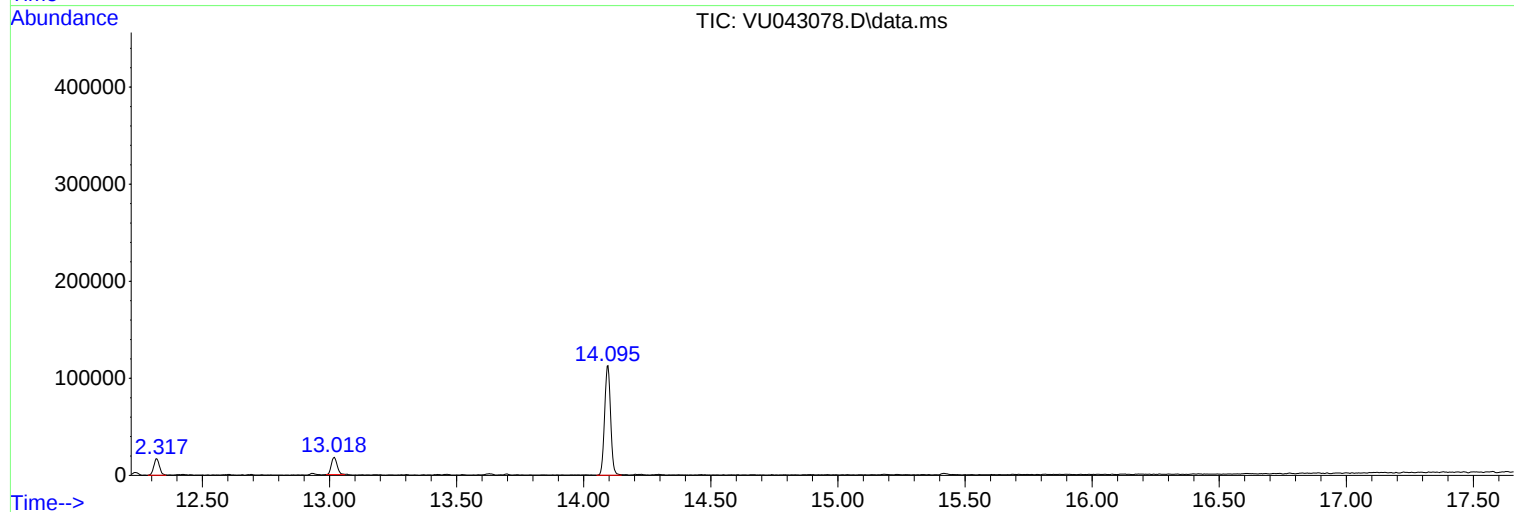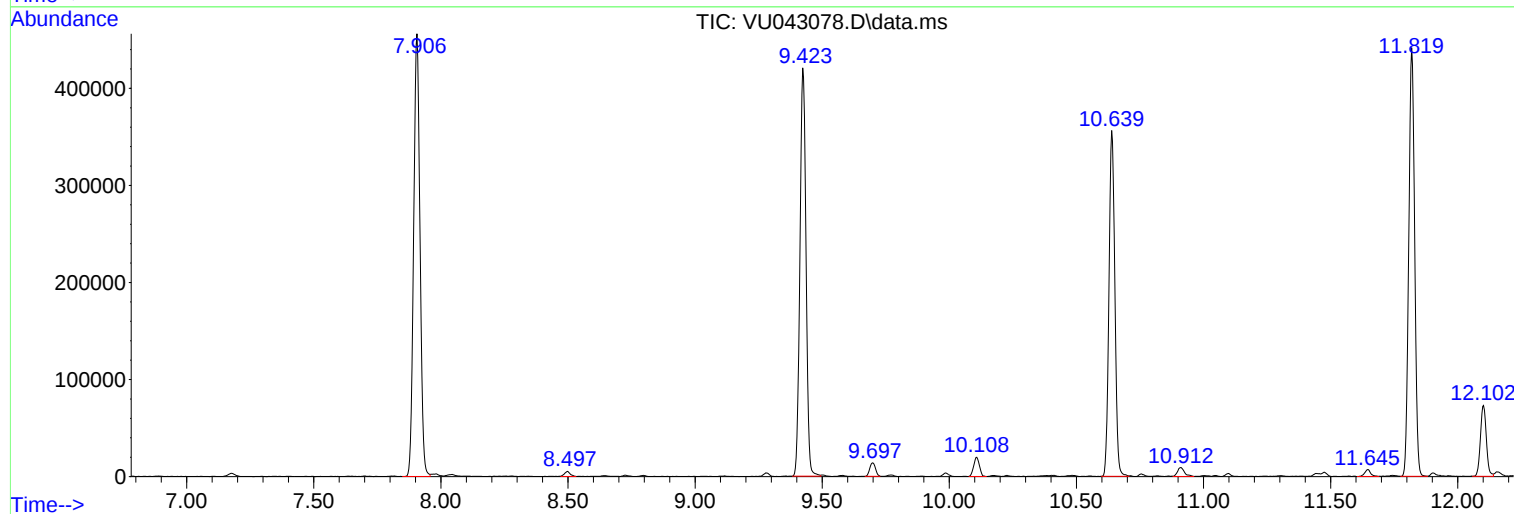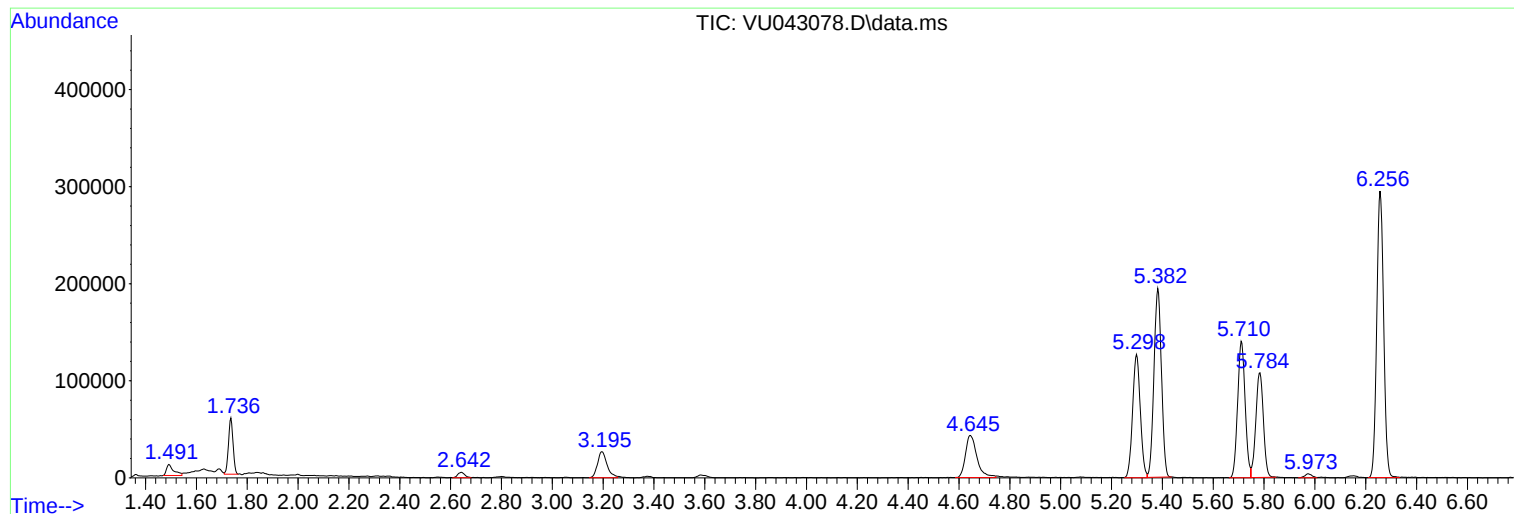

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
Data File : VU043078.D
Acq On : 14 Apr 2021 02:10
Operator : SY/MD
Sample : M1966-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-110RR










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Indane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.102	8.41 ug/l	117917	1,4-Dichlorobenzene-d4	11.819

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indane	118	C9H10	000496-11-7	95
2			Bicyclo[4.2.0]octa-1,3,5-triene,...	118	C9H10	055337-80-9	74
3			Benzene, 1-ethenyl-2-methyl-	118	C9H10	000611-15-4	74
4			Deltacyclene	118	C9H10	007785-10-6	68
5			Benzene, cyclopropyl-	118	C9H10	000873-49-4	64

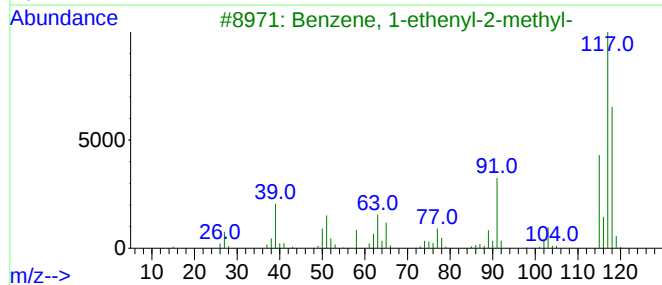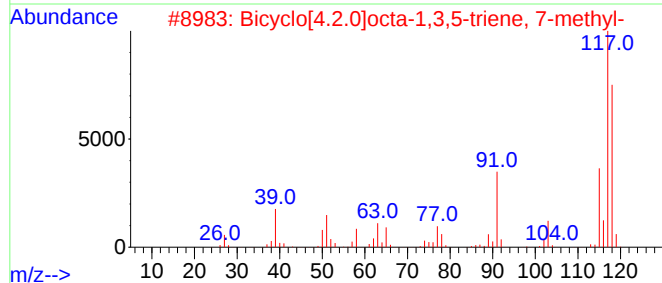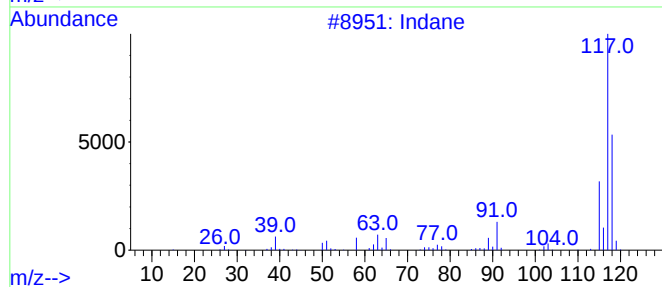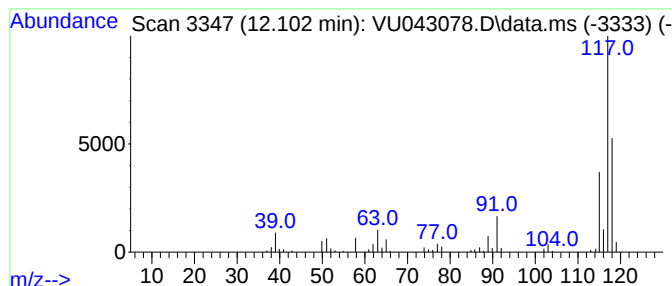

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
Data File : VU043078.D
Acq On : 14 Apr 2021 02:10
Operator : SY/MD
Sample : M1966-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-110RR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	12.102	8.4	ug/l	117917	4	11.819	701385	50.0