
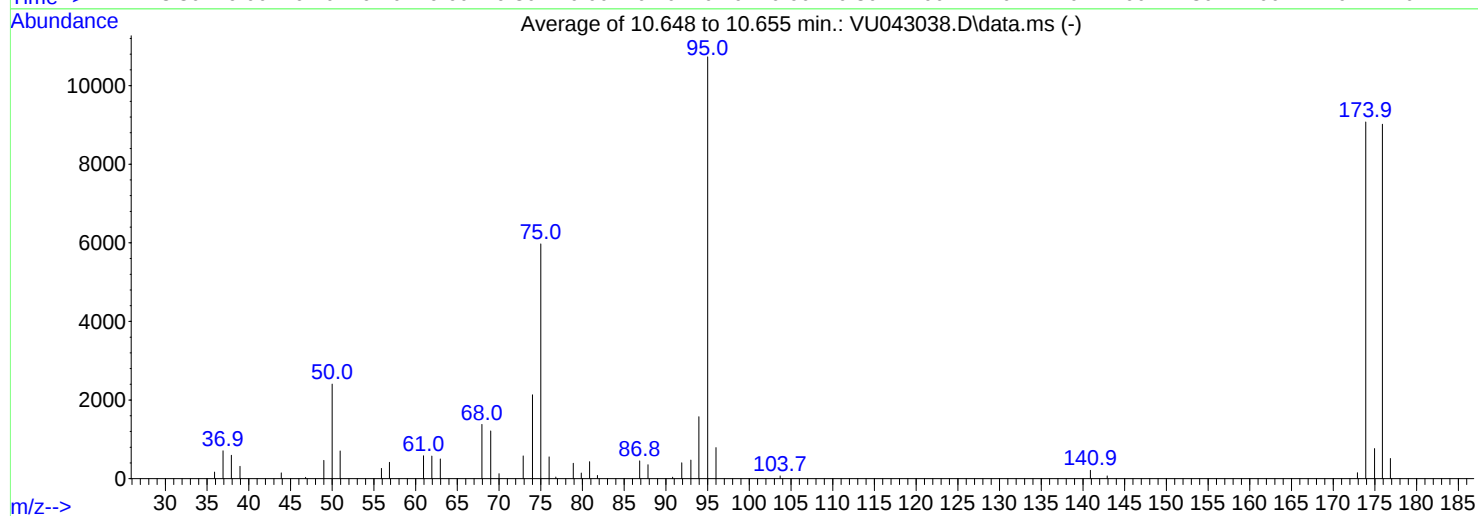


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
 Data File : VU043038.D
 Acq On : 13 Apr 2021 09:30
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
 Title : SW846 8260
 Last Update : Mon Apr 12 13:17:29 2021

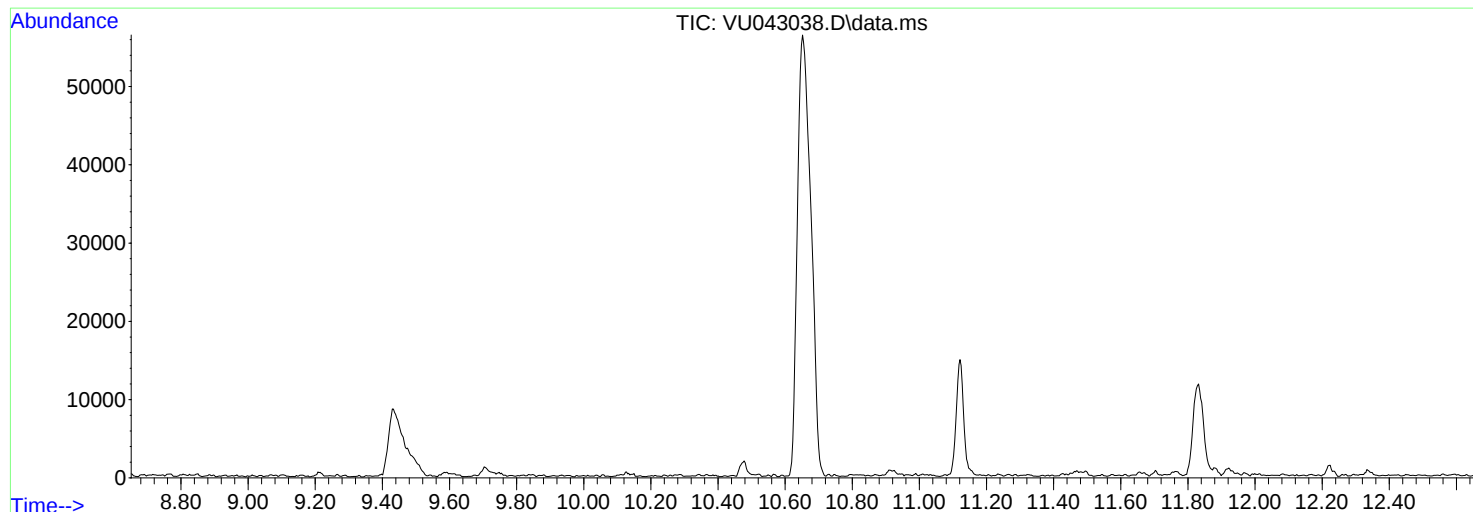

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	2408	PASS
75	95	30	60	55.7	5974	PASS
95	95	100	100	100.0	10731	PASS
96	95	5	9	7.3	788	PASS
173	174	0.00	2	1.7	151	PASS
174	95	50	100	84.5	9072	PASS
175	174	5	9	8.5	767	PASS
176	174	95	101	99.4	9015	PASS
177	176	5	9	5.7	515	PASS