
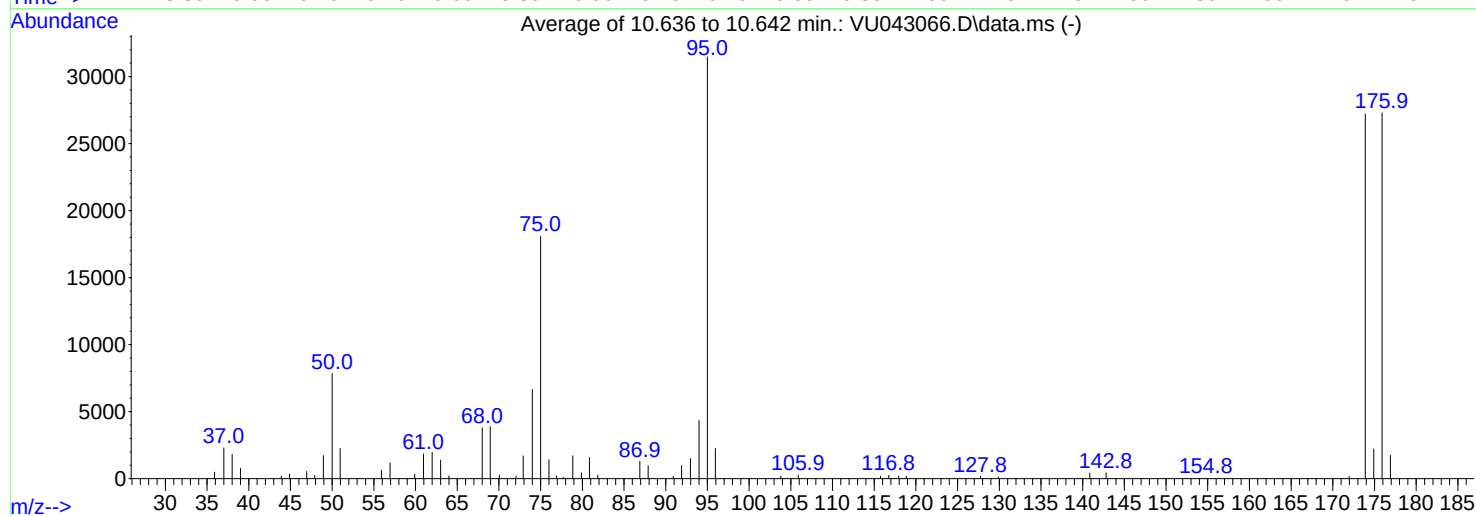


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041321\
Data File : VU043066.D
Acq On : 13 Apr 2021 21:11
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Title : SW846 8260
Last Update : Mon Apr 12 13:17:29 2021

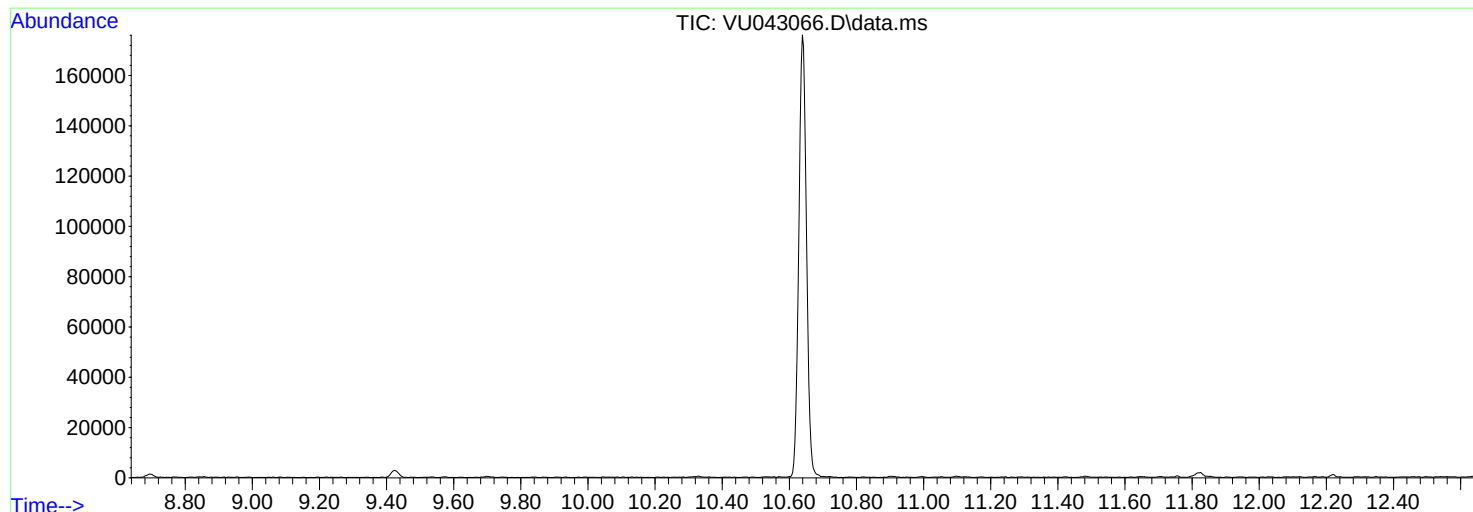

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.9	7849	PASS
75	95	30	60	57.5	18104	PASS
95	95	100	100	100.0	31472	PASS
96	95	5	9	7.1	2246	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.5	27208	PASS
175	174	5	9	8.1	2216	PASS
176	174	95	101	100.3	27296	PASS
177	176	5	9	6.4	1749	PASS