

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041422\
 Data File : VW022542.D
 Acq On : 14 Apr 2022 10:34
 Operator : SY/VA
 Sample : VW0414SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK479

Quant Time: Apr 15 01:30:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 01:29:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	326533	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	313265	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159277	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	118878	16.468	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.880%
7) Chloroethane-d5	2.891	69	88538	19.570	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.280%
11) 1,1-Dichloroethene-d2	4.019	63	126282	13.488	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.960%
21) 2-Butanone-d5	7.074	46	79253	62.885	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.780%
24) Chloroform-d	7.653	84	243913	23.898	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	8.305	65	145291	24.915	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.640%
32) Benzene-d6	8.275	84	435578	22.758	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.040%
36) 1,2-Dichloropropane-d6	9.274	67	136408	24.628	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.520%
41) Toluene-d8	10.323	98	405586	21.637	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.560%
43) trans-1,3-Dichloroprop...	10.579	79	56117	21.468	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.880%
47) 2-Hexanone-d5	10.921	63	63648	61.765	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.520%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	138668	29.445	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	117.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	157749	27.962	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.840%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	5259	0.650	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041422\
Data File : VW022542.D
Acq On : 14 Apr 2022 10:34
Operator : SY/VA
Sample : VW0414SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK479

Quant Time: Apr 15 01:30:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 15 01:29:34 2022
Response via : Initial Calibration

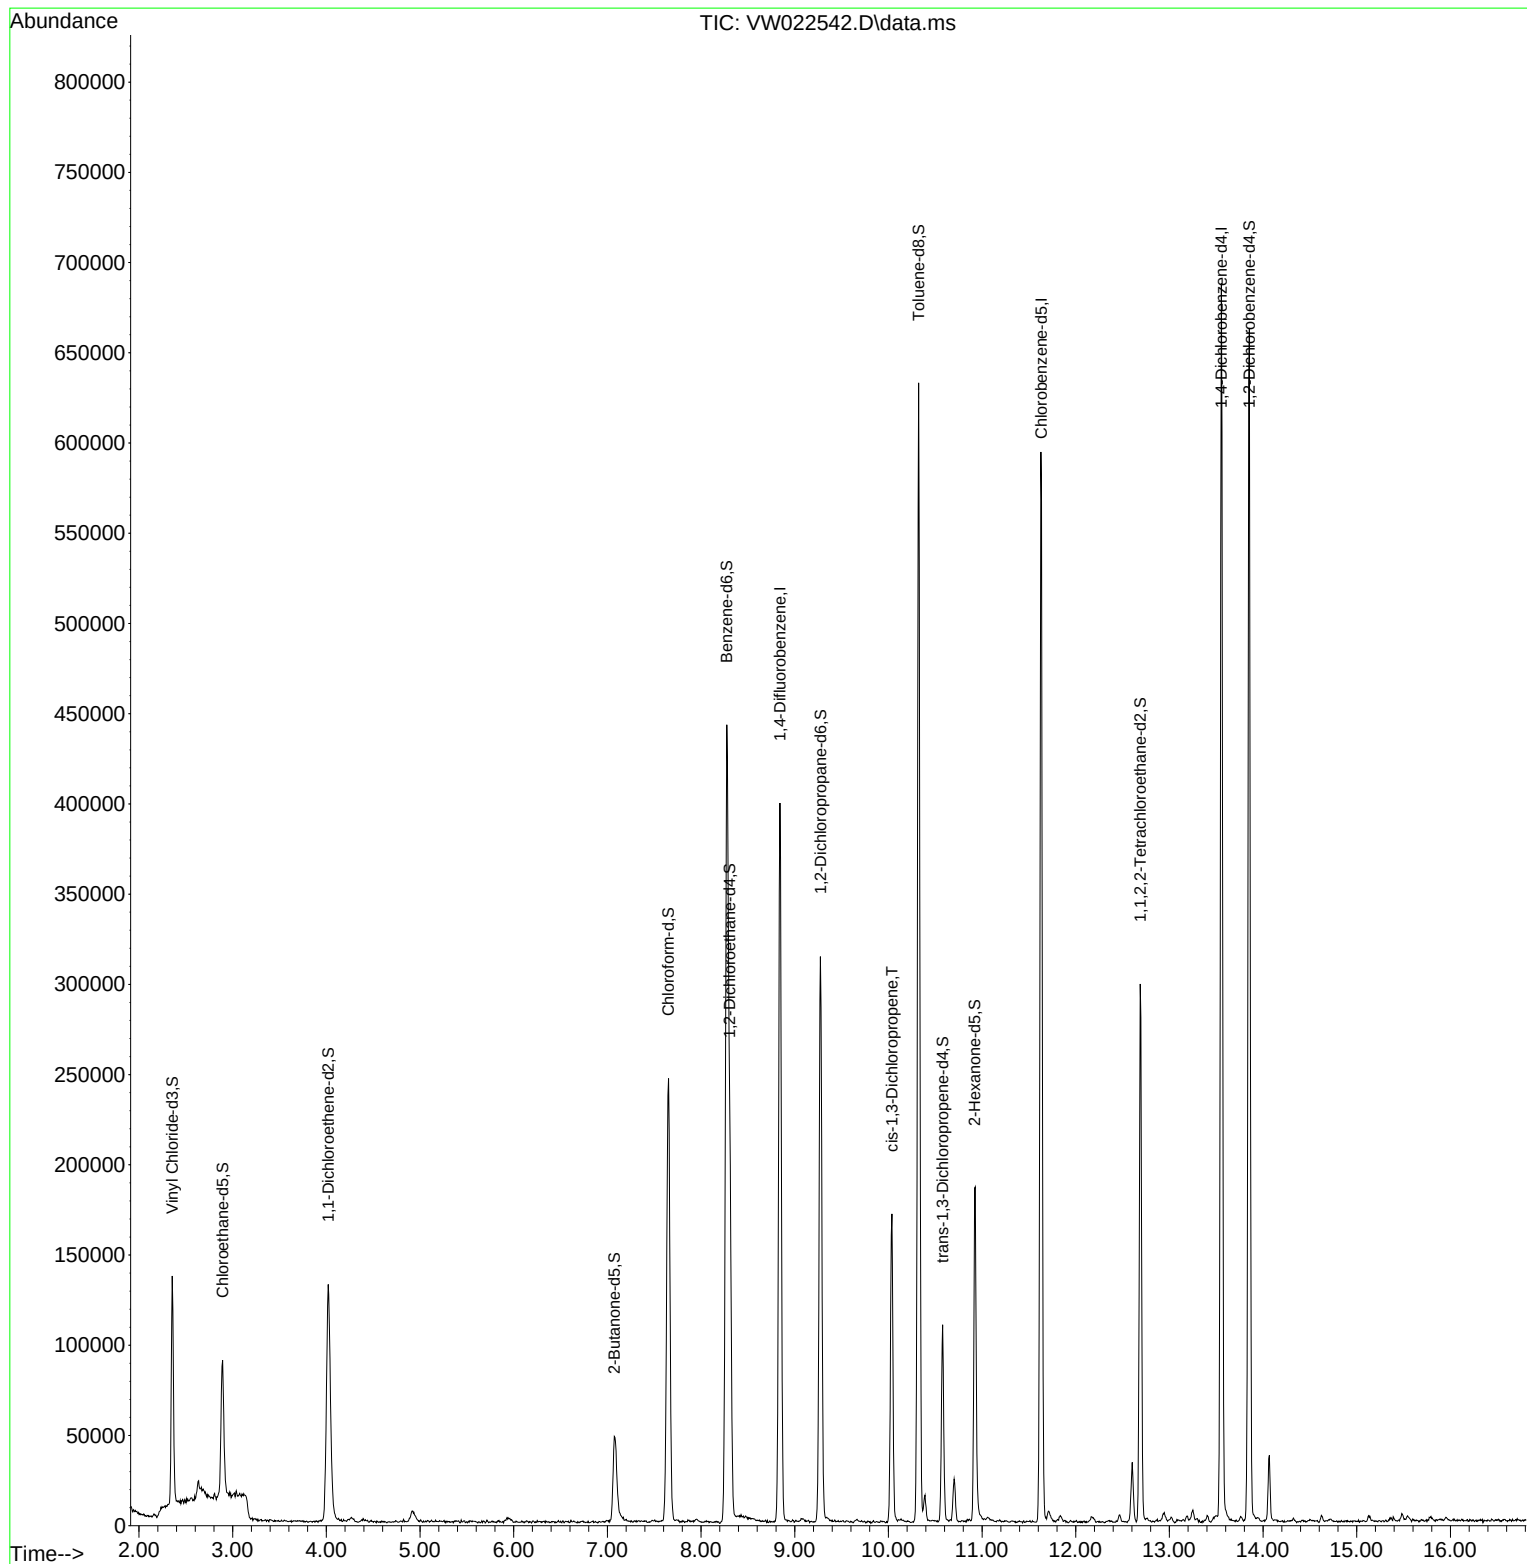

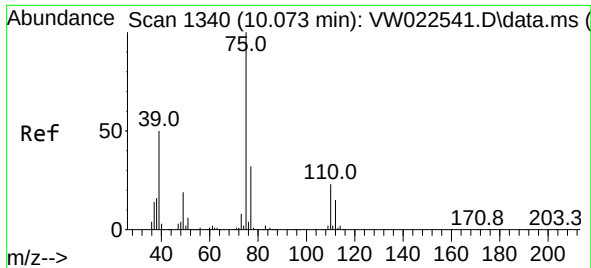

#39

cis-1,3-Dichloropropene

Concen: 0.650 ug/L

RT: 10.037 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW022542.D


Acq: 14 Apr 2022 10:34

Instrument :

MSVOA_U

ClientSampleId :

VBLK479

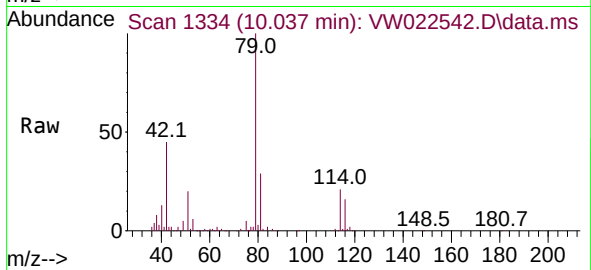

Tgt Ion: 75 Resp: 5259

Ion Ratio Lower Upper

75 100

77 36.6 22.6 42.0

