

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041422\
 Data File : VW022545.D
 Acq On : 14 Apr 2022 11:46
 Operator : SY/VA
 Sample : N2358-06
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Quant Time: Apr 15 01:30:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 01:29:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	302137	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	300491	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	152269	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	108960	16.313	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.240%
7) Chloroethane-d5	2.885	69	84638	20.219	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.880%
11) 1,1-Dichloroethene-d2	4.019	63	113135	13.059	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.240%
21) 2-Butanone-d5	7.080	46	62404	53.514	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.020%
24) Chloroform-d	7.653	84	215783	22.849	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.400%
26) 1,2-Dichloroethane-d4	8.305	65	127523	23.634	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.520%
32) Benzene-d6	8.275	84	387569	21.111	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.440%
36) 1,2-Dichloropropane-d6	9.274	67	122356	23.030	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.120%
41) Toluene-d8	10.323	98	357720	19.895	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.560%
43) trans-1,3-Dichloroprop...	10.573	79	47080	18.777	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.120%
47) 2-Hexanone-d5	10.920	63	51716	52.319	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.640%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	115604	25.591	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	138701	25.717	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	5001	0.645	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041422\
Data File : VW022545.D
Acq On : 14 Apr 2022 11:46
Operator : SY/VA
Sample : N2358-06
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Time: Apr 15 01:30:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 15 01:29:34 2022
Response via : Initial Calibration

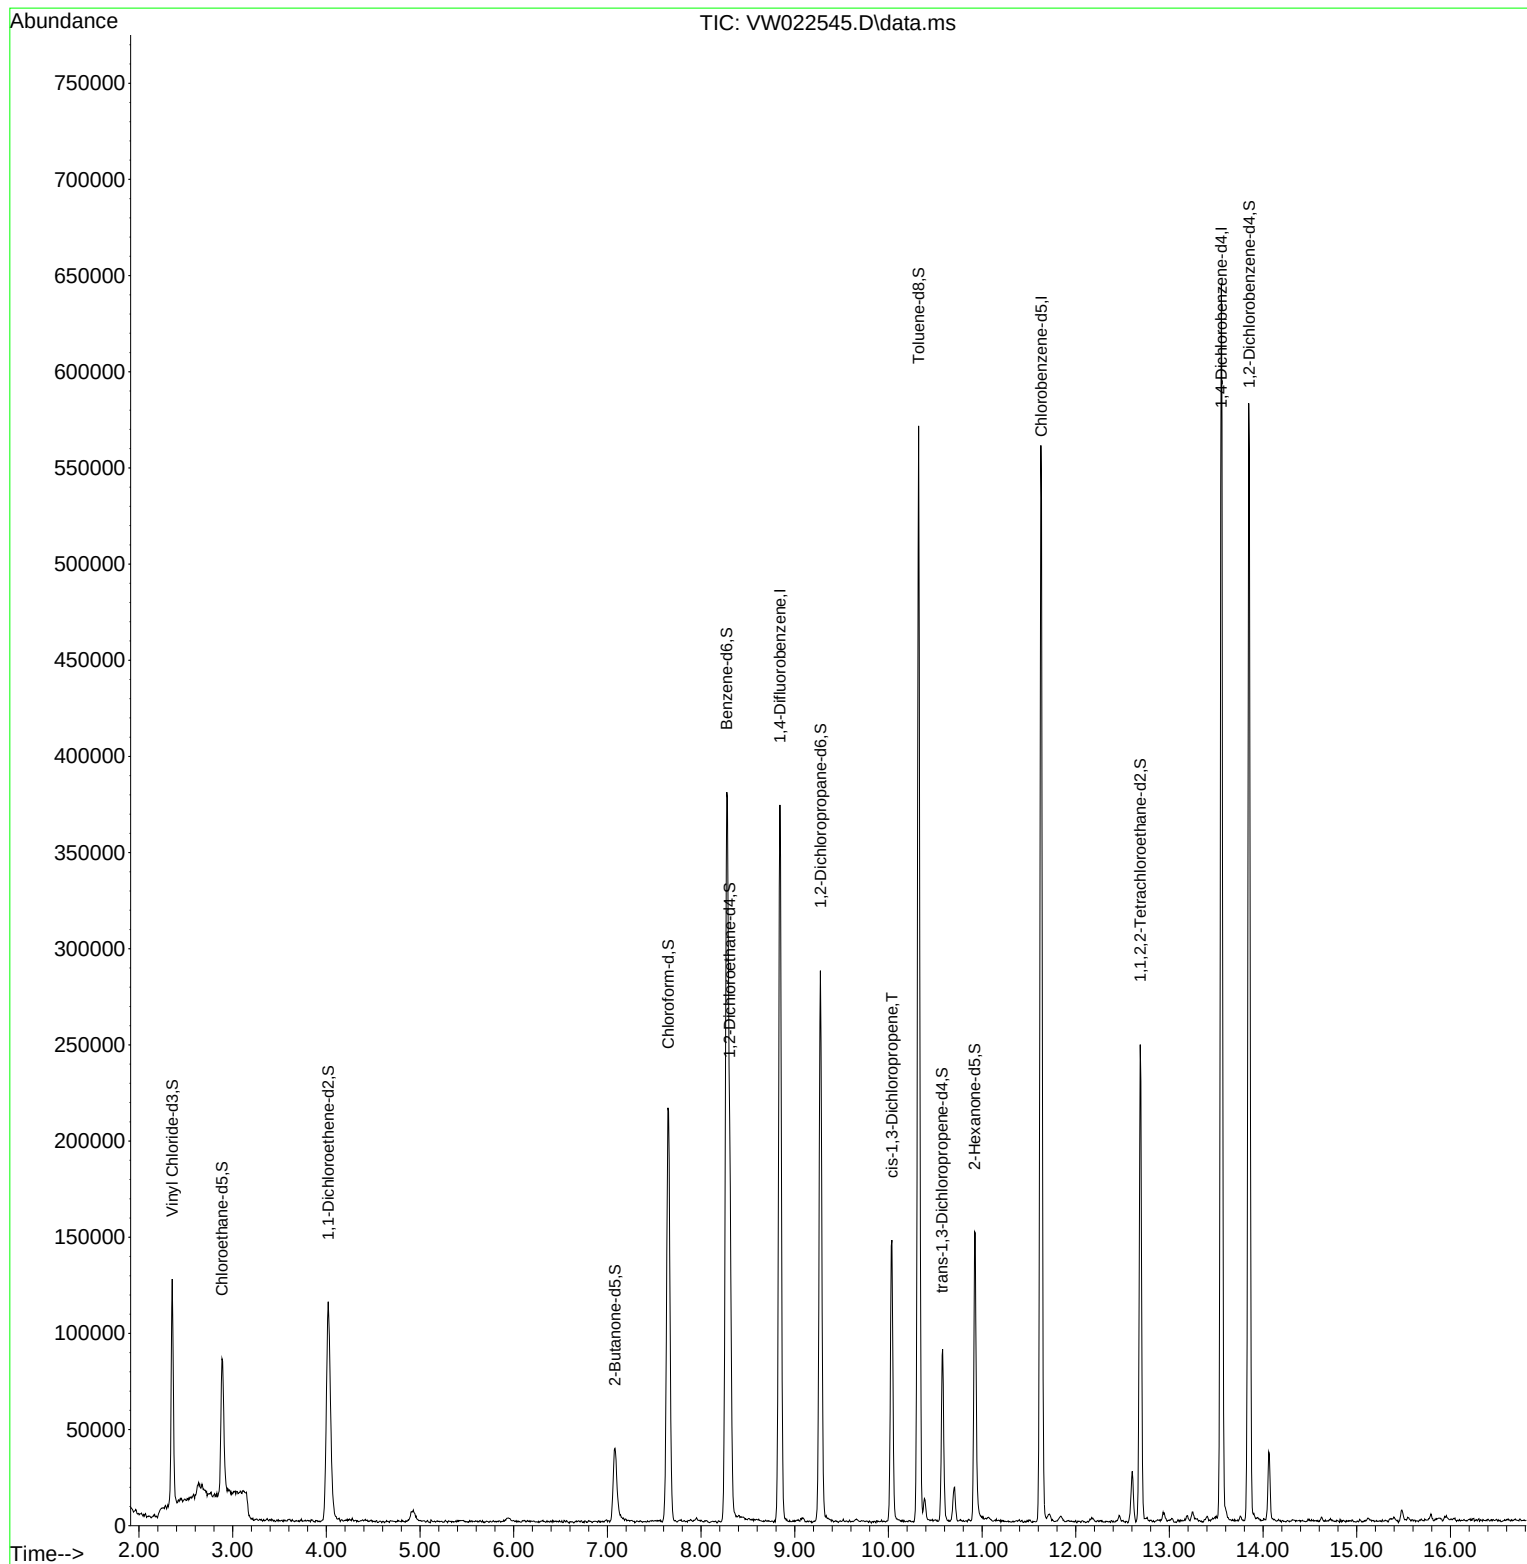

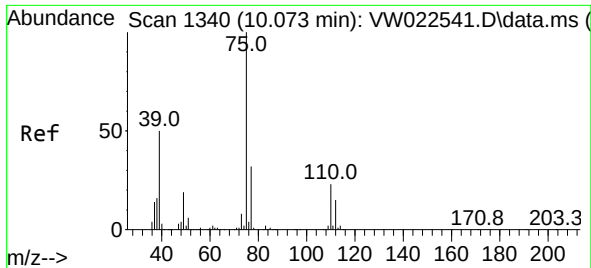

#39

cis-1,3-Dichloropropene

Concen: 0.645 ug/L

RT: 10.037 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW022545.D


Acq: 14 Apr 2022 11:46

Instrument :

MSVOA_U

ClientSampleId :

VHBLK002

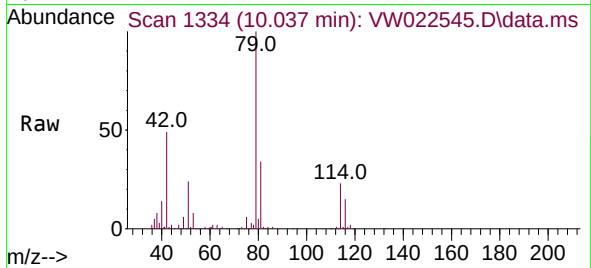

Tgt Ion: 75 Resp: 5001

Ion Ratio Lower Upper

75 100

77 50.2 22.6 42.0#

