

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU047999.D
 Acq On : 13 Apr 2022 13:30
 Operator : SY/MD
 Sample : N2345-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J86

Quant Time: Apr 14 03:08:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 14 02:49:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	366269	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	379606	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	212907	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	117146	44.105	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.220%
7) Chloroethane-d5	1.916	69	99629	47.571	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.140%
11) 1,1-Dichloroethene-d2	2.568	63	152492	31.380	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.760%
21) 2-Butanone-d5	4.626	46	193182	84.738	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.740%
24) Chloroform-d	5.067	84	216310	44.509	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.020%
26) 1,2-Dichloroethane-d4	5.703	65	139498	46.801	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.600%
32) Benzene-d6	5.729	84	446377	46.731	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.460%
36) 1,2-Dichloropropane-d6	6.694	67	143949	49.071	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.140%
41) Toluene-d8	7.899	98	400158	42.998	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.000%
43) trans-1,3-Dichloroprop...	8.179	79	62360	41.960	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.920%
47) 2-Hexanone-d5	8.632	63	148888	86.701	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.700%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	217191	43.142	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.280%
66) 1,2-Dichlorobenzene-d4	12.195	152	179854	47.482	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.960%
Target Compounds						
					Qvalue	
51) Chlorobenzene	9.449	112	6625	0.809	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU047999.D
Acq On : 13 Apr 2022 13:30
Operator : SY/MD
Sample : N2345-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J86


Quant Time: Apr 14 03:08:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 14 02:49:33 2022
Response via : Initial Calibration

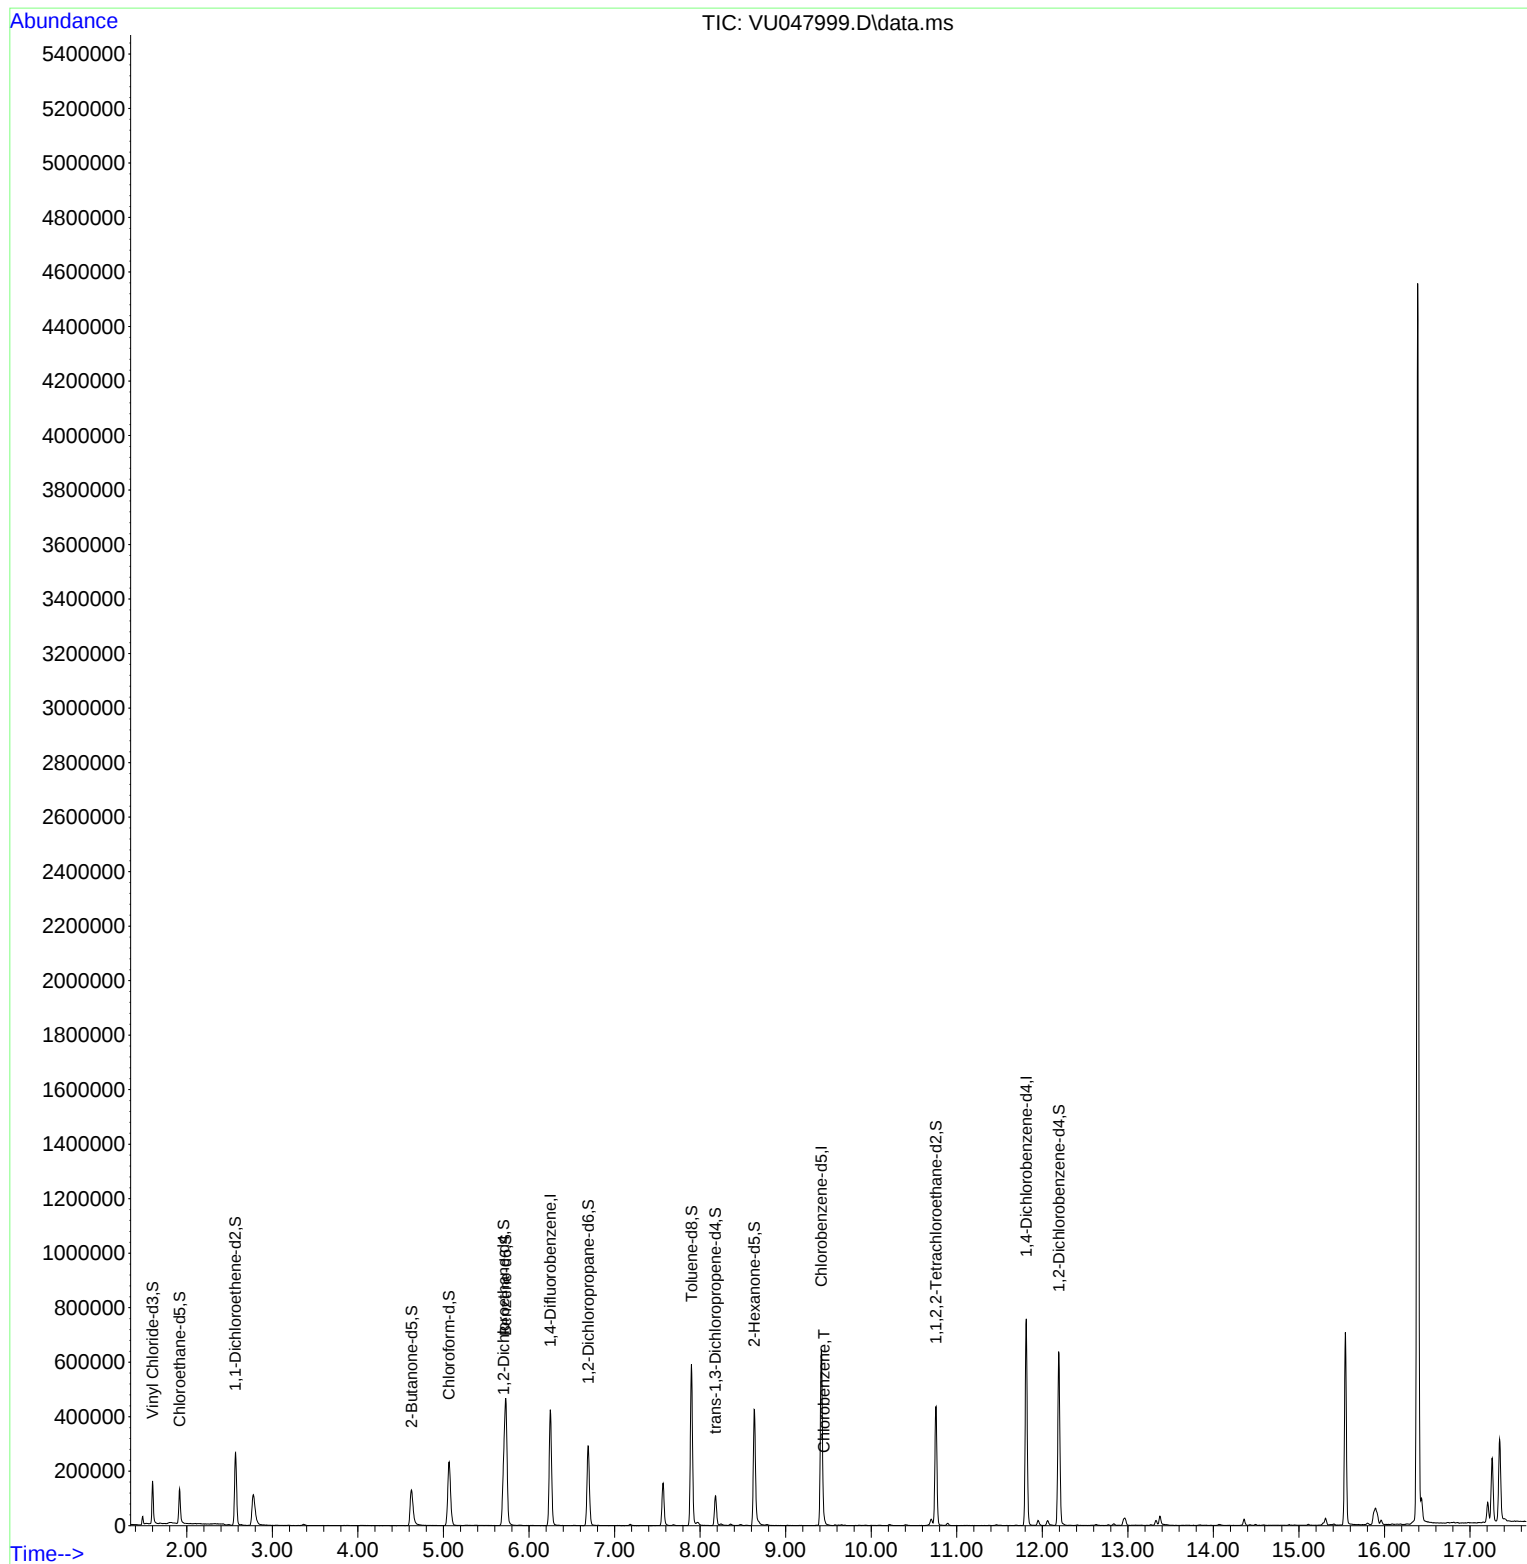

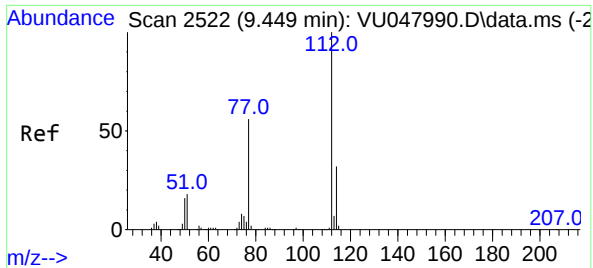

#51
Chlorobenzene
Concen: 0.809 ug/L
RT: 9.449 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU047999.D
Acq: 13 Apr 2022 13:30

Instrument :
MSVOA_U
ClientSampleId :
C0J86

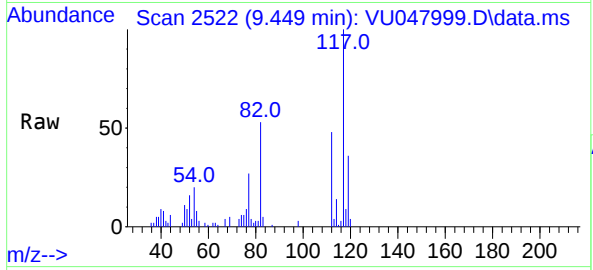

Tgt Ion:	112	Resp:	6625
Ion	Ratio	Lower	Upper
112	100		
114	29.9	22.1	41.1
77	56.0	43.4	65.0

