

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
 Data File : VU048002.D
 Acq On : 13 Apr 2022 14:39
 Operator : SY/MD
 Sample : N2345-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J87

Quant Time: Apr 14 03:08:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 14 02:49:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	351515	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	365074	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	193737	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	119944	47.054	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.100%
7) Chloroethane-d5	1.916	69	105844	52.660	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.320%
11) 1,1-Dichloroethene-d2	2.568	63	155880	33.424	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.840%
21) 2-Butanone-d5	4.633	46	205561	93.953	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.950%
24) Chloroform-d	5.067	84	220273	47.227	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.460%
26) 1,2-Dichloroethane-d4	5.703	65	143019	49.996	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.000%
32) Benzene-d6	5.729	84	451399	49.138	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.280%
36) 1,2-Dichloropropane-d6	6.694	67	144839	51.340	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.680%
41) Toluene-d8	7.899	98	398624	44.538	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.080%
43) trans-1,3-Dichloroprop...	8.182	79	62083	43.437	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.880%
47) 2-Hexanone-d5	8.636	63	152182	92.146	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.150%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	219824	45.403	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	171758	49.832	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.660%
Target Compounds						
					Qvalue	
51) Chlorobenzene	9.446	112	6879	0.874	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041322\
Data File : VU048002.D
Acq On : 13 Apr 2022 14:39
Operator : SY/MD
Sample : N2345-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J87


Quant Time: Apr 14 03:08:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 14 02:49:33 2022
Response via : Initial Calibration

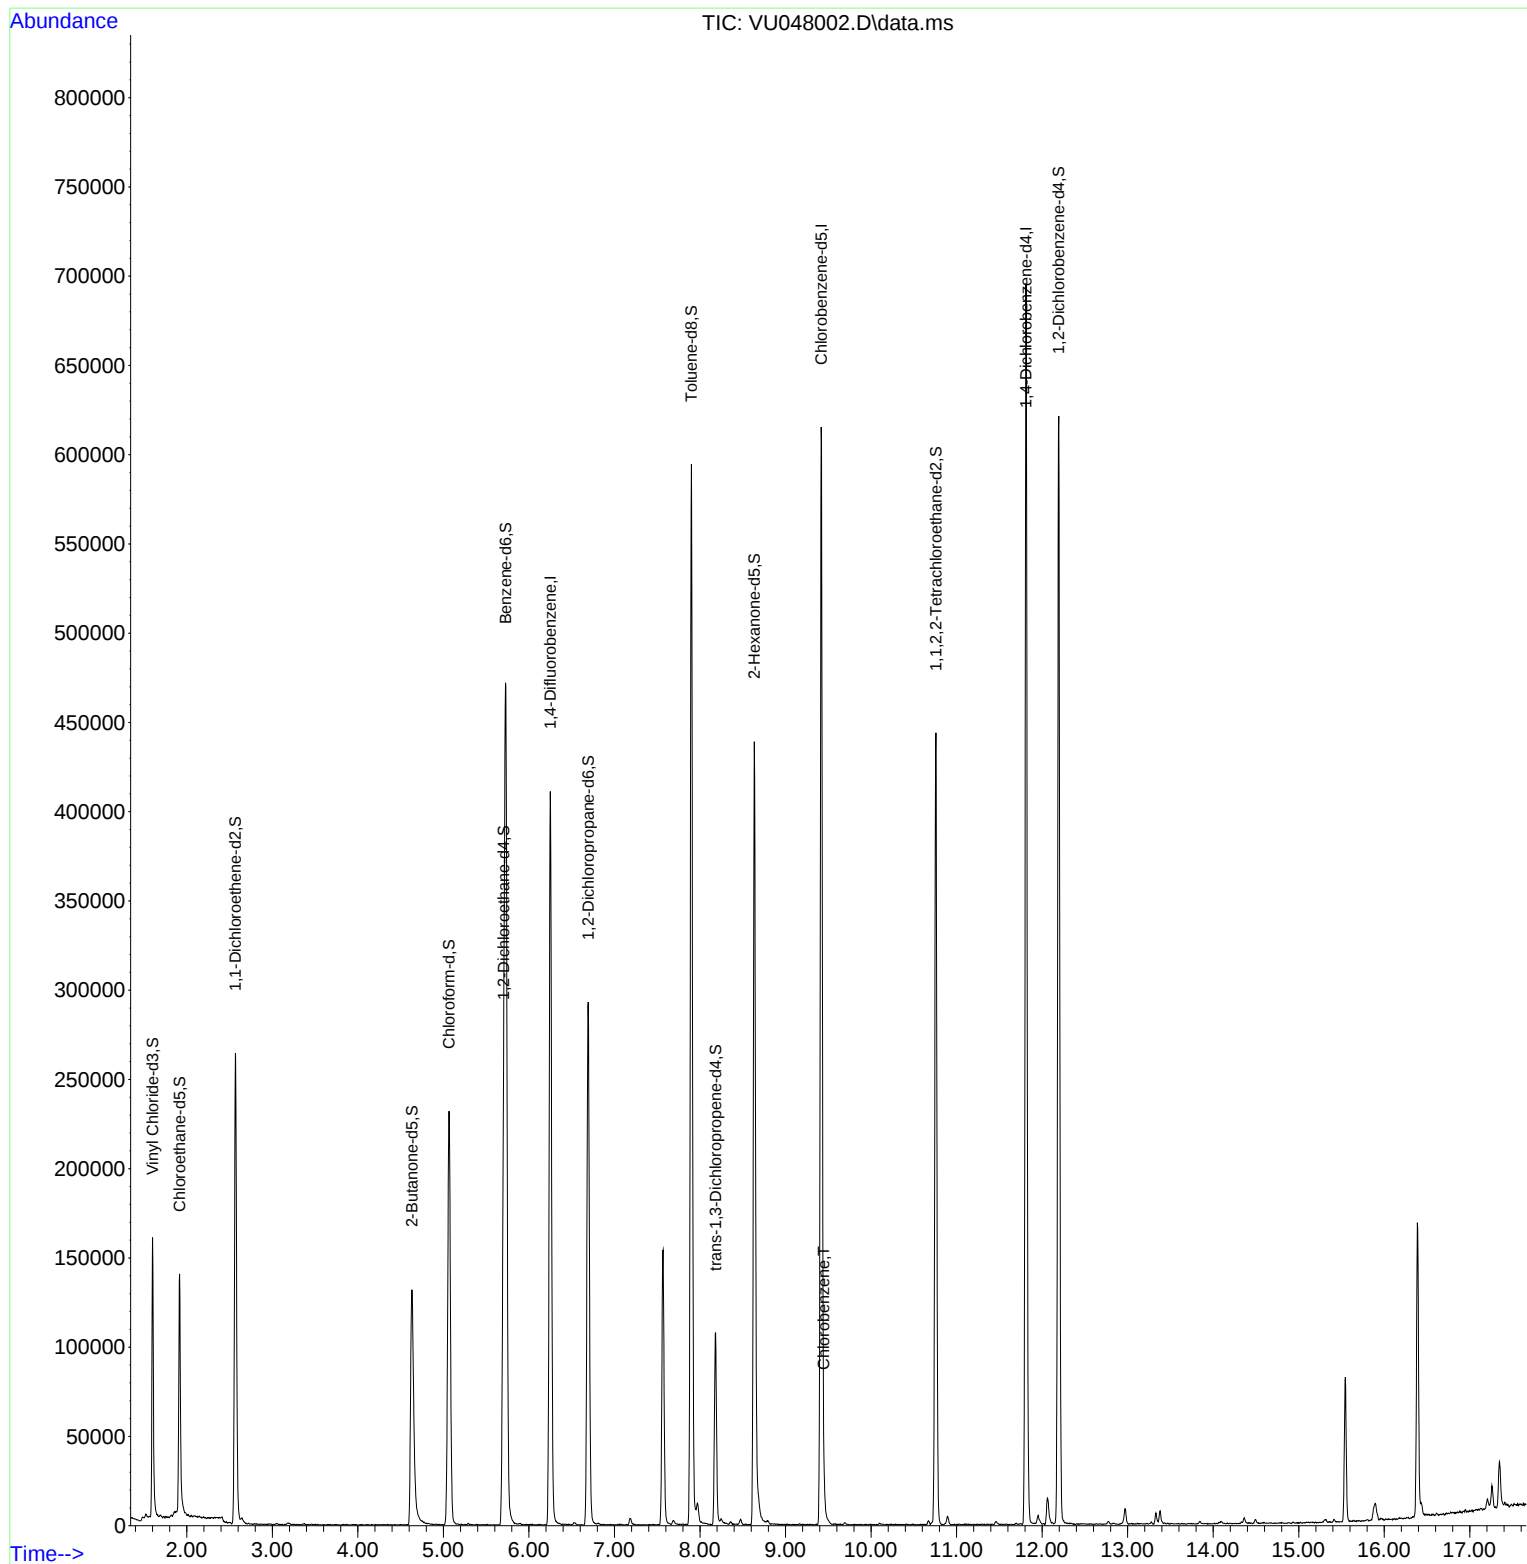

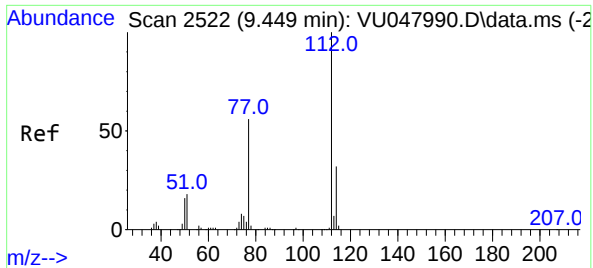

#51
Chlorobenzene
Concen: 0.874 ug/L
RT: 9.446 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU048002.D
Acq: 13 Apr 2022 14:39

Instrument :
MSVOA_U
ClientSampleId :
C0J87

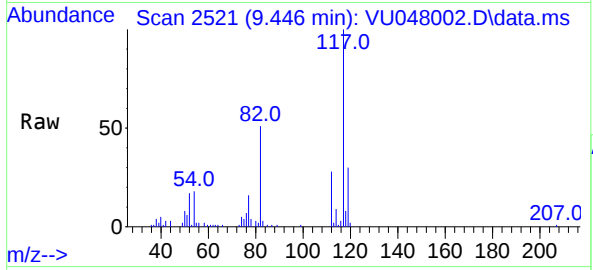

Tgt Ion:	112	Resp:	6879
Ion	Ratio	Lower	Upper
112	100		
114	32.9	22.1	41.1
77	59.4	43.4	65.0

